

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112021\
 Data File : BG051162.D
 Acq On : 21 Nov 2021 00:46
 Operator : CG/JU
 Sample : M4768-06
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-FIELD

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG051162.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.264	295	302	310	rBV	34195	56046	2.23%	0.628%
2	5.740	377	383	391	rBV	283387	468499	18.68%	5.252%
3	7.356	651	658	671	rVB	192072	345414	13.77%	3.872%
4	8.202	795	802	808	rBV	102235	178446	7.12%	2.001%
5	9.377	993	1002	1017	rBV	349378	653098	26.04%	7.322%
6	11.028	1276	1283	1296	rVB	135440	250304	9.98%	2.806%
7	13.455	1689	1696	1705	rBV	936000	1450178	57.82%	16.258%
8	14.836	1922	1931	1940	rBV	220205	344176	13.72%	3.859%
9	16.322	2178	2184	2195	rBV	676146	1041792	41.54%	11.680%
10	17.585	2392	2399	2408	rBV	281857	442031	17.63%	4.956%
11	20.176	2833	2840	2845	rBV	1864651	2507945	100.00%	28.117%
12	21.575	3073	3078	3084	rBV	38108	60553	2.41%	0.679%
13	21.880	3123	3130	3139	rBV2	299512	513985	20.49%	5.762%
14	24.236	3527	3531	3539	rVB7	15968	27042	1.08%	0.303%
15	25.282	3694	3709	3720	rVB2	172085	537512	21.43%	6.026%
16	26.422	3896	3903	3915	rVB6	12765	42733	1.70%	0.479%




Sum of corrected areas: 8919754

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112021\
Data File : BG051162.D
Acq On : 21 Nov 2021 00:46
Operator : CG/JU
Sample : M4768-06
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-FIELD

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

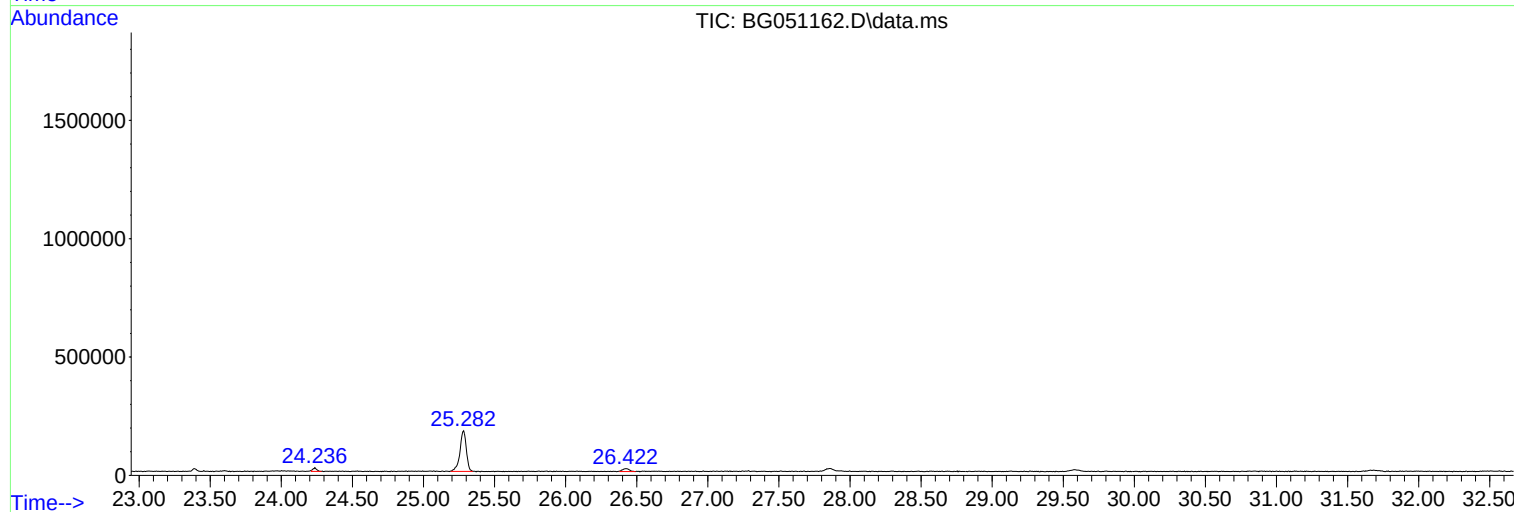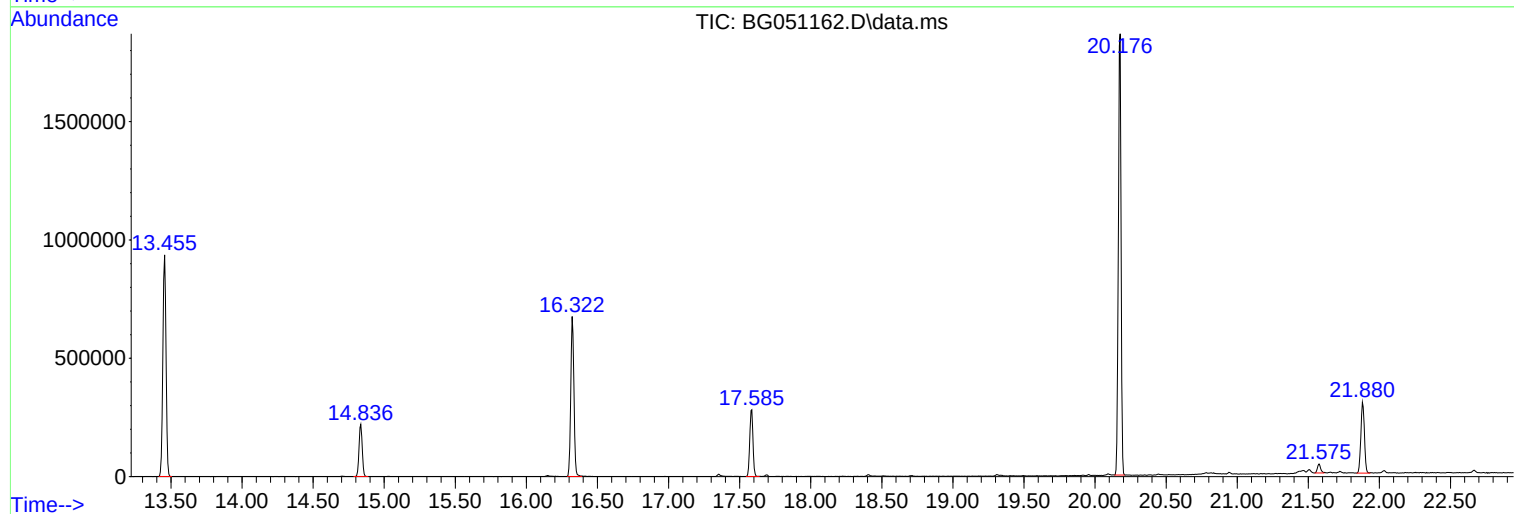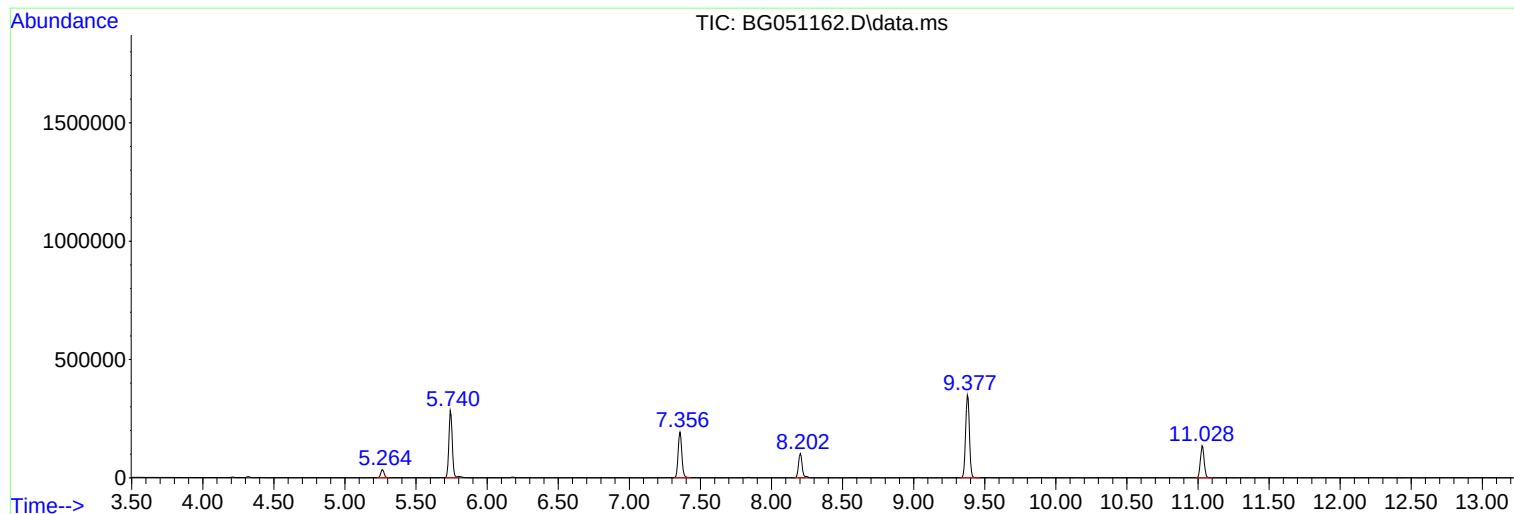

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112021\
Data File : BG051162.D
Acq On : 21 Nov 2021 00:46
Operator : CG/JU
Sample : M4768-06
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-FIELD

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112021\
Data File : BG051162.D
Acq On : 21 Nov 2021 00:46
Operator : CG/JU
Sample : M4768-06
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-FIELD

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------