


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112021\
 Data File : BG051146.D
 Acq On : 20 Nov 2021 13:47
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Nov 19 16:26:22 2021

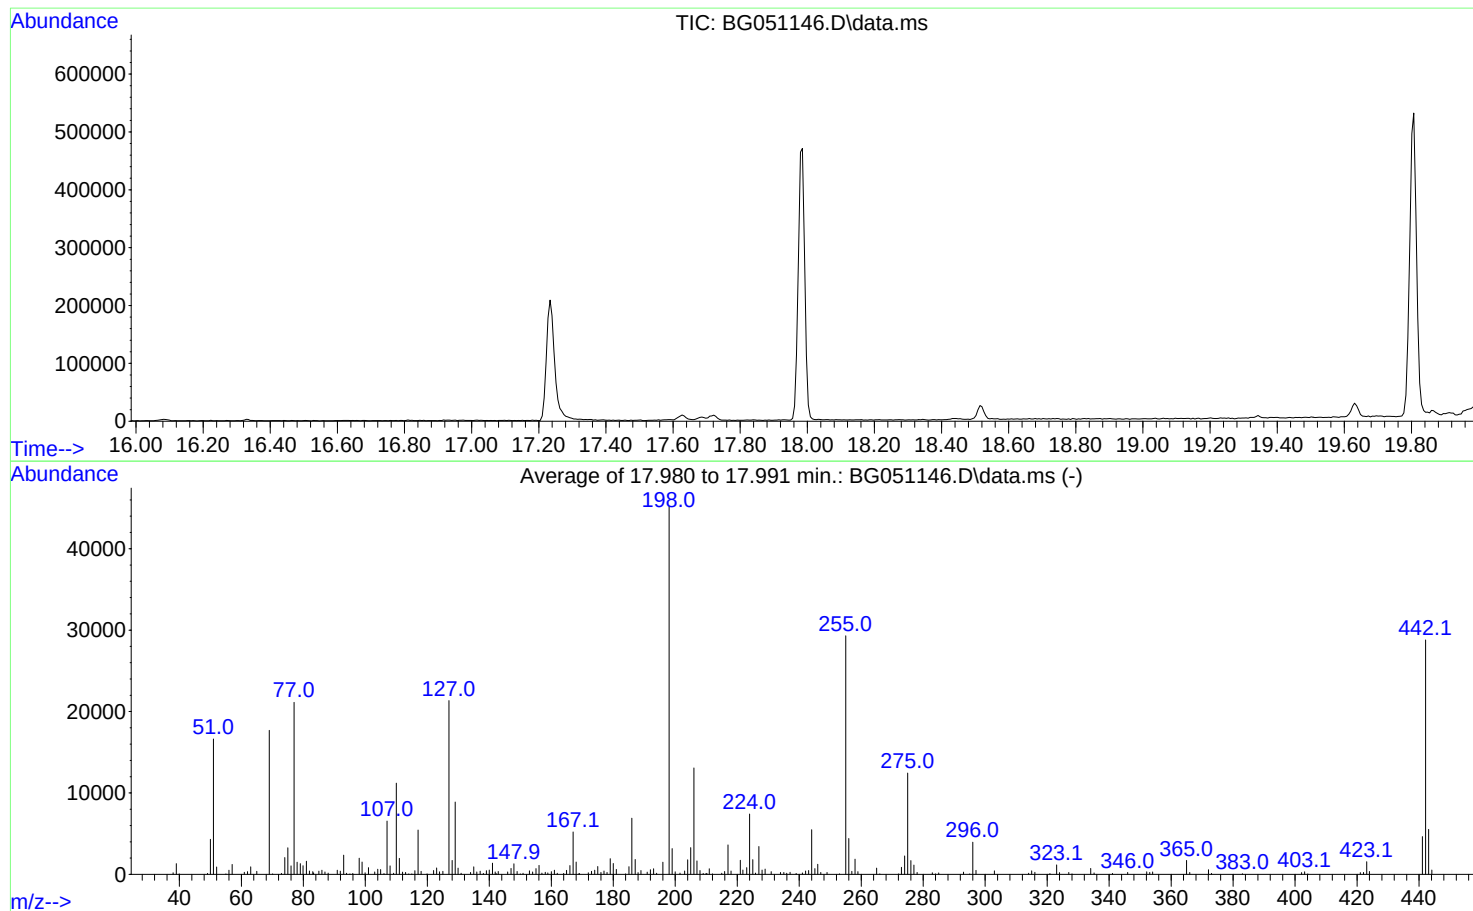




AutoFind: Scans 2466, 2467, 2468; Background Corrected with Scan 2459

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.8	16620	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	39.1	17691	PASS
70	69	0.00	2	0.3	56	PASS
127	198	10	80	47.2	21350	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	45189	PASS
199	198	5	9	7.0	3160	PASS
275	198	10	60	27.5	12436	PASS
365	198	1	100	3.8	1703	PASS
441	198	0.01	100	10.3	4641	PASS
442	442	50	100	100.0	28795	PASS
443	442	15	24	19.2	5526	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112021\
Data File : BG051146.D
Acq On : 20 Nov 2021 13:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 22 02:57:24 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG11921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 19 16:26:22 2021
Response via : Initial Calibration

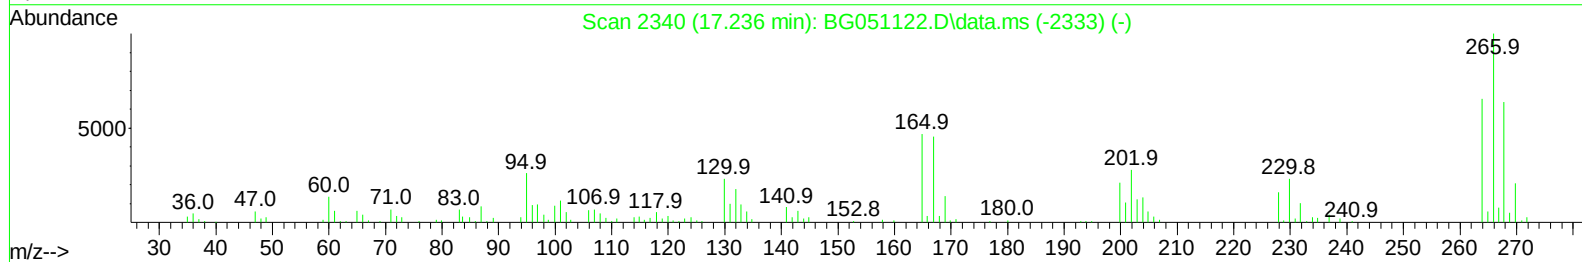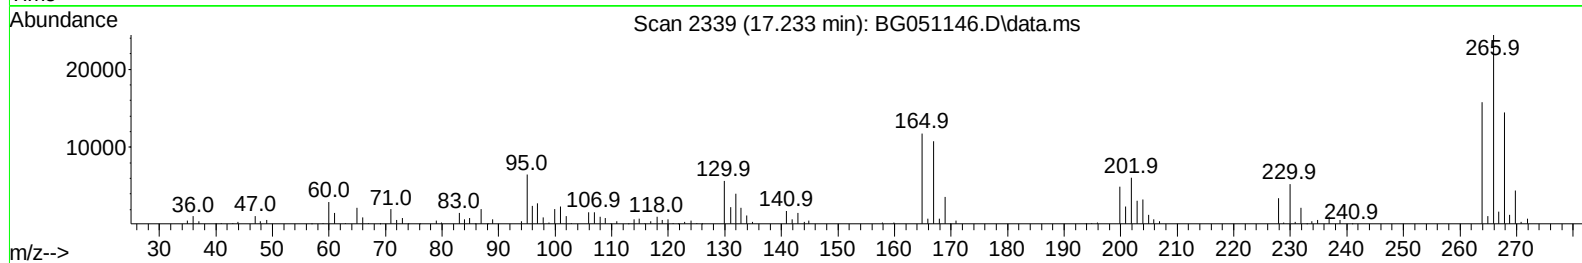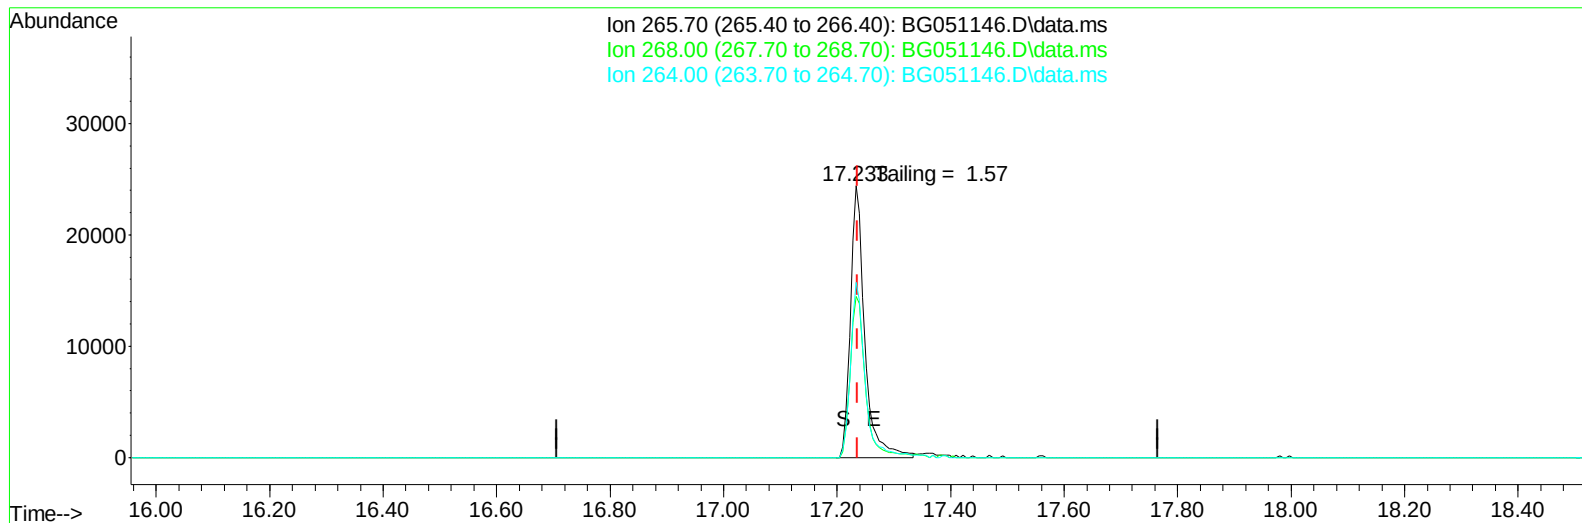

TIC: BG051146.D\data.ms

(70) Pentachlorophenol (C)

17.233min (-0.002) 5643.56 ng




response 43040

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	59.29
264.00	61.30	64.55
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112021\
Data File : BG051146.D
Acq On : 20 Nov 2021 13:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 22 02:57:24 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG11921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 19 16:26:22 2021
Response via : Initial Calibration

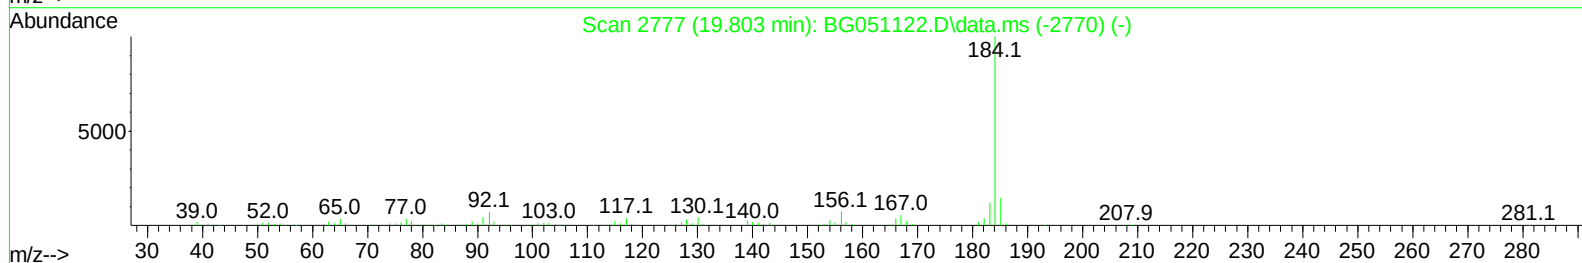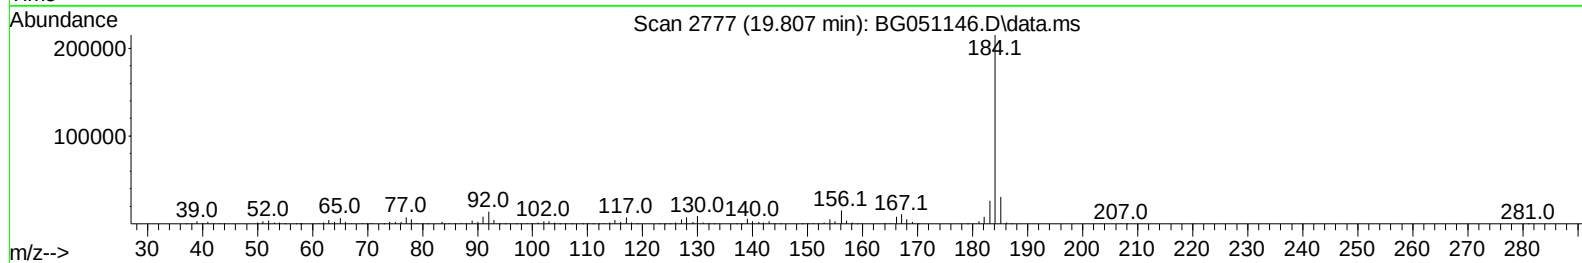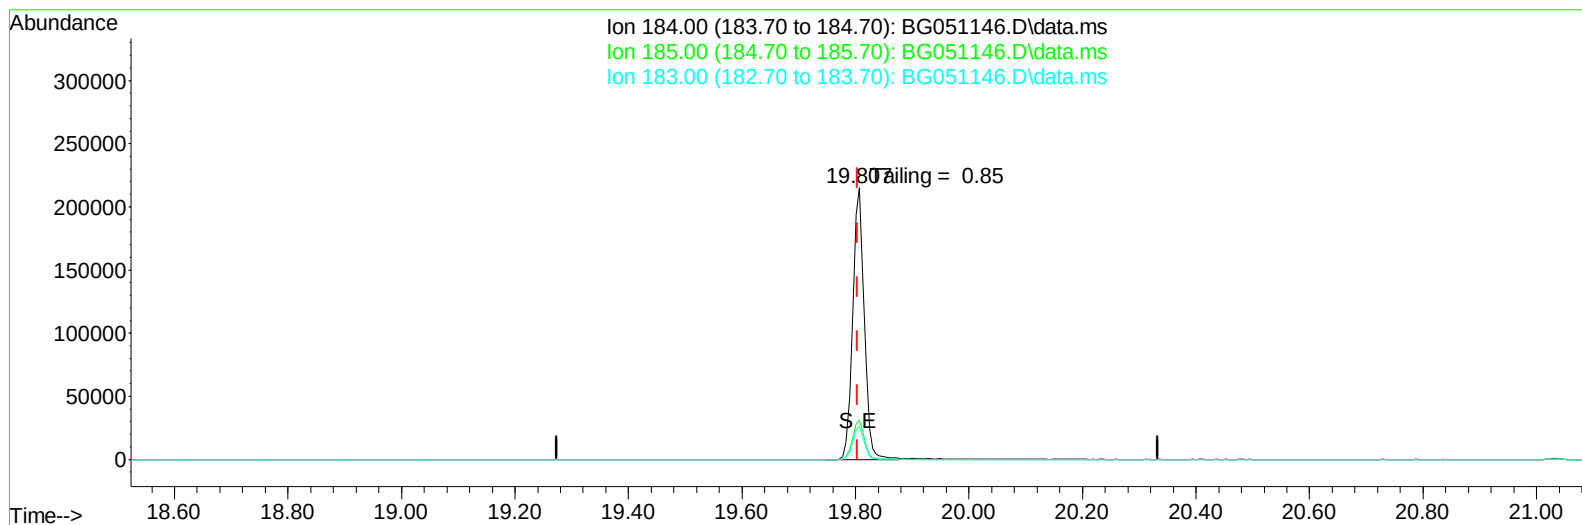

TIC: BG051146.D\data.ms

(77) Benzidine

19.807min (+ 0.004) 51022.59 ng

response 306635

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.42
183.00	11.70	12.18
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/20/2021	BNA_G	BG051146.D
Compound Name	Response	Retention Time
DDT	167956	21.035
DDD	5996	20.582
DDE	0	19.9
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5996	173952	3.45

Instrument :
BNA_G
ClientSampleId :
DFTPP