

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG112116\
 Data File : BG024878.D
 Acq On : 22 Nov 2016 3:36
 Operator : UM/SJ
 Sample : H5694-20
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JHSS7

Quant Time: Nov 22 06:25:54 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG111416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 22 01:29:33 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.26	152	125075	20.00	ng/ul	0.00
18) Naphthalene-d8	11.08	136	545944	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.88	164	471306	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.72	188	637972	20.00	ng/ul	0.10
75) Chrysene-d12	21.92	240	1201417	20.00	ng/ul	0.00
83) Perylene-d12	25.35	264	1264965	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.62	96	5359	2.22	ng/uL	0.00
5) Phenol-d5	7.40	99	137433	12.83	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.57	67	95324	14.14	ng/ul	0.00
9) 2-Chlorophenol-d4	7.78	132	105293	13.70	ng/ul	0.00
13) 4-Methylphenol-d8	8.95	113	120728	13.42	ng/ul	0.00
19) Nitrobenzene-d5	9.44	128	57455	13.90	ng/ul	0.00
22) 2-Nitrophenol-d4	10.15	143	66902	13.56	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.70	165	126176	12.85	ng/ul	0.00
29) 4-Chloroaniline-d4	11.22	131	135900	12.39	ng/ul	0.00
43) Dimethylphthalate-d6	14.27	166	462809	13.47	ng/ul	0.00
46) Acenaphthylene-d8	14.57	160	521048	13.91	ng/ul	0.00
51) 4-Nitrophenol-d4	15.06	143	64054	10.47	ng/ul	0.00
57) Fluorene-d10	15.87	176	419757	12.98	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.07	200	240	0.05	ng/ul	0.09
70) Anthracene-d10	17.72	188	641735	22.77	ng/ul	0.00
76) Pyrene-d10	19.99	212	771372	14.81	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.11	264	802089	14.48	ng/ul	0.00

Target Compounds


						Qvalue
6) Phenol	7.42	94	17873	1.60	ng/ul	95
44) Dimethylphthalate	14.31	163	87999	2.67	ng/ul#	91
77) Pyrene	20.02	202	166408	2.82	ng/ul#	91
80) Benzo(a)anthracene	21.89	228	106827	1.63	ng/ul	96
82) Chrysene	21.96	228	105463	1.72	ng/ul	100
85) Benzo(b)fluoranthene	24.26	252	116181	1.74	ng/ul#	95
86) Benzo(k)fluoranthene	24.26	252	116181	1.84	ng/ul#	93
88) Benzo(a)pyrene	25.18	252	102023	1.58	ng/ul#	79


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG112116\
Data File : BG024878.D
Acq On : 22 Nov 2016 3:36
Operator : UM/SJ
Sample : H5694-20
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JHSS7

Quant Time: Nov 22 06:25:54 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG111416.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 22 01:29:33 2016
Response via : Initial Calibration

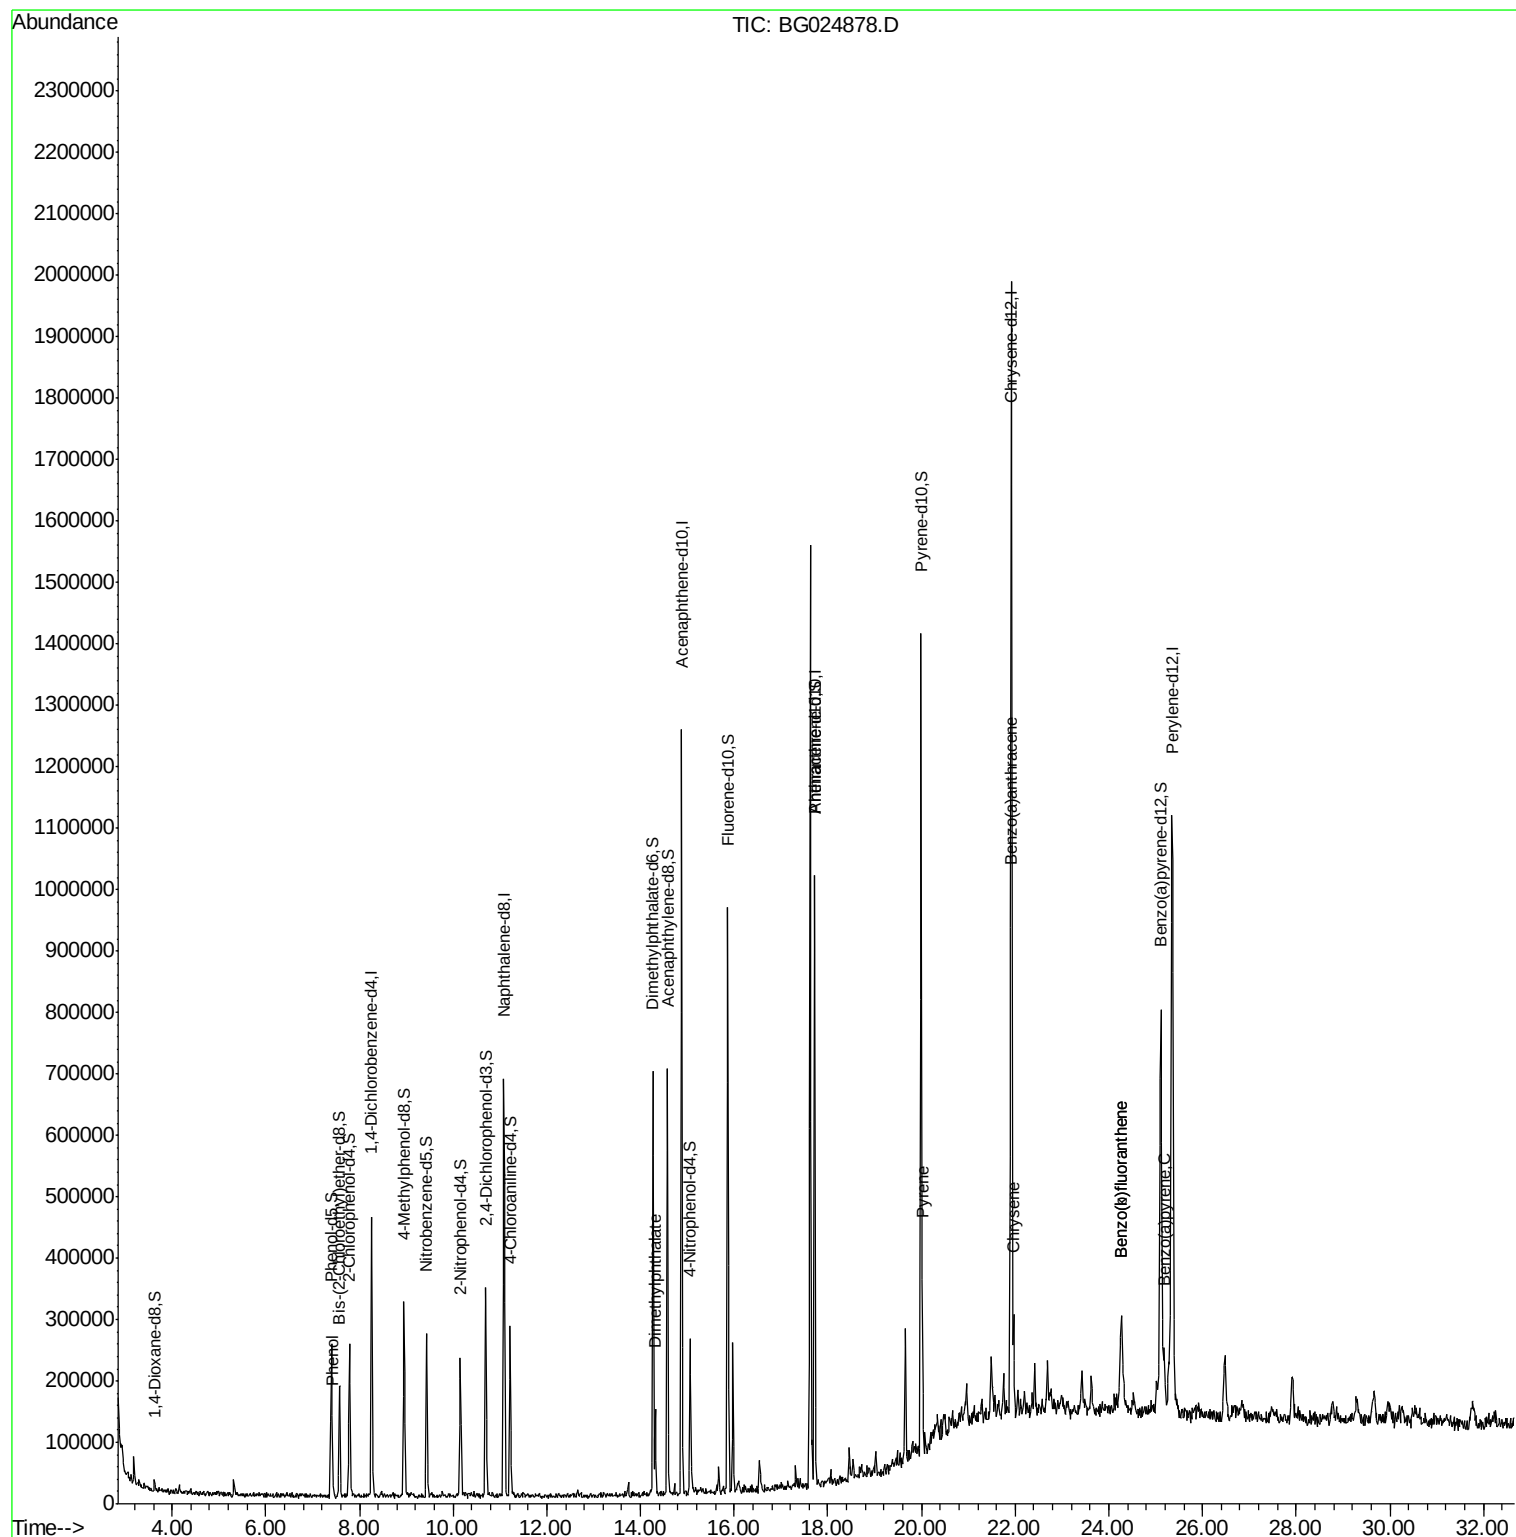

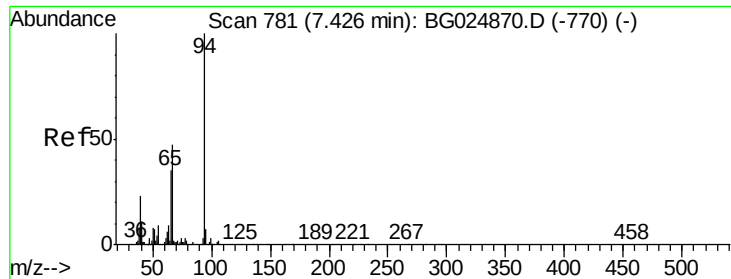

#6

Phenol

Concen: 1.60 ng/ul

RT: 7.42 min Scan# 780

Delta R.T. -0.00 min

Lab File: BG024878.D

Acq: 22 Nov 2016 3:36

Instrument :

BNA_G

ClientSampleId :

JHSS7


Tgt Ion: 94 Resp: 17873

Ion Ratio Lower Upper




94 100

65 28.9 26.8 40.2

66 53.4 44.4 66.6

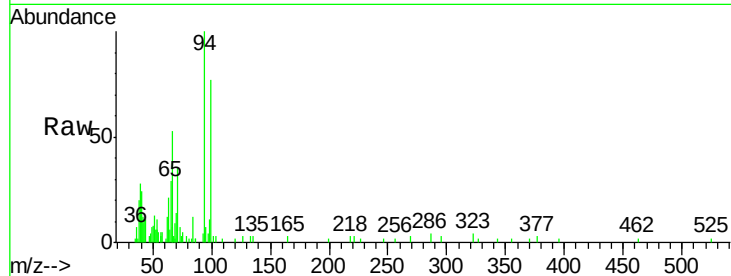

Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC

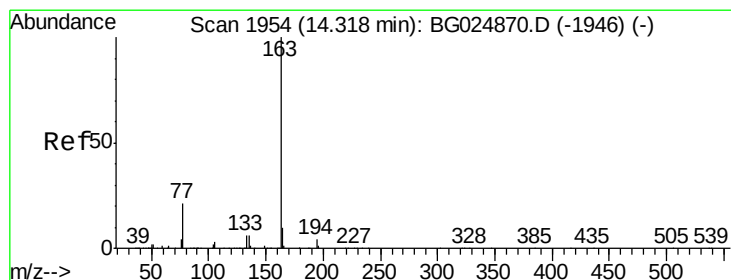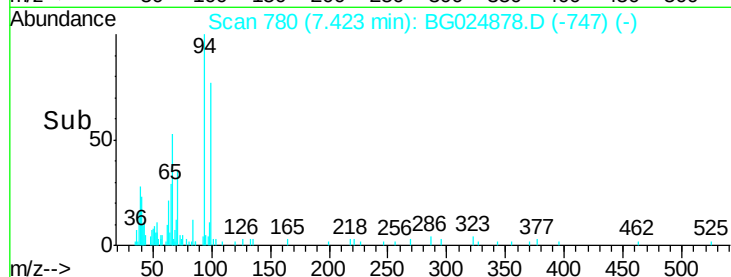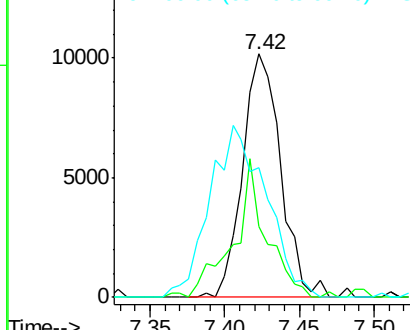

#44

Dimethylphthalate

Concen: 2.67 ng/ul

RT: 14.31 min Scan# 1952

Delta R.T. -0.01 min

Lab File: BG024878.D

Acq: 22 Nov 2016 3:36


Tgt Ion:163 Resp: 87999

Ion Ratio Lower Upper



163 100


194 4.1 3.4 5.0

164 6.6 9.0 13.4#

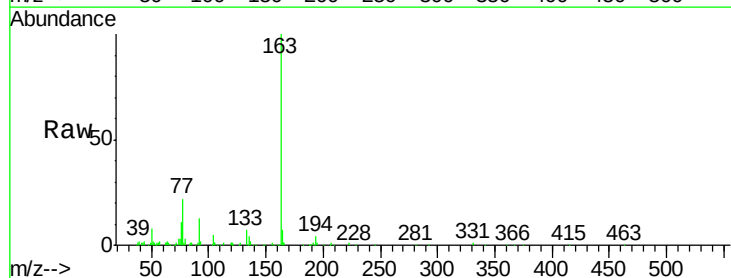

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

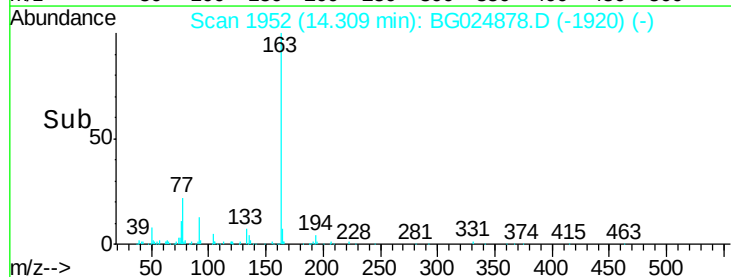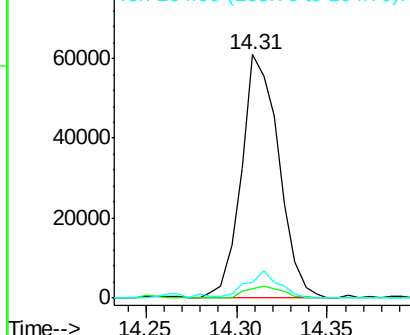

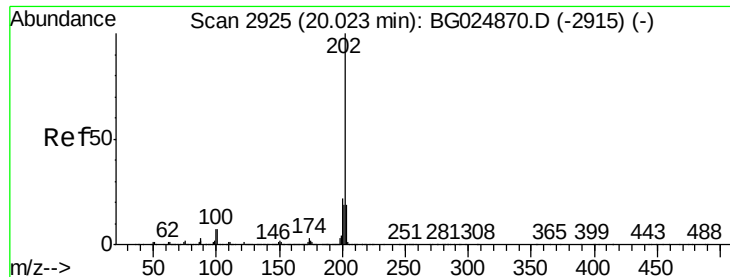

#77

Pyrene

Concen: 2.82 ng/ul

RT: 20.02 min Scan# 2924

Delta R.T. -0.00 min

Lab File: BG024878.D

Acq: 22 Nov 2016 3:36

Instrument :

BNA_G

ClientSampleId :

JHSS7


Tgt Ion:202 Resp: 166408

Ion Ratio Lower Upper

202 100

101 4.8 6.9 10.3#




100 5.4 6.6 10.0#

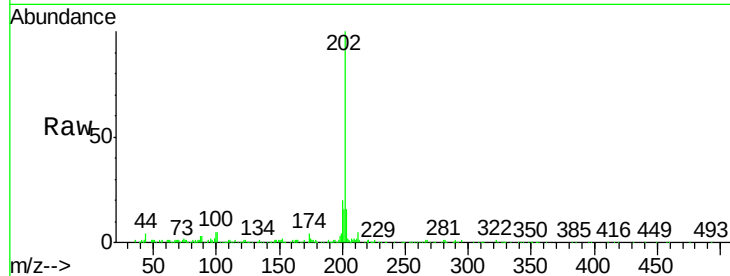

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E

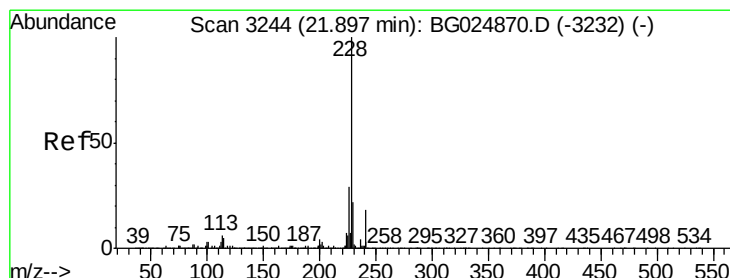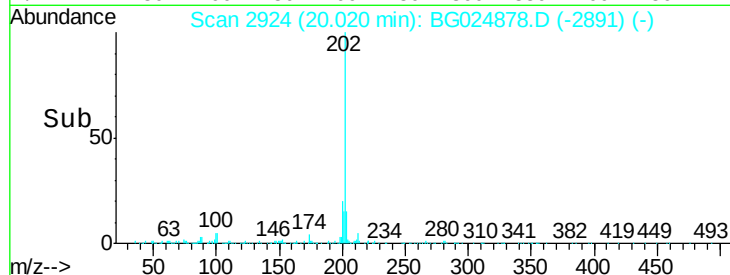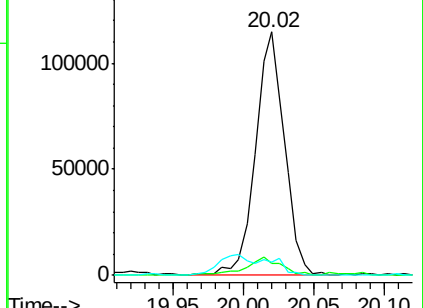

#80

Benzo(a)anthracene

Concen: 1.63 ng/ul

RT: 21.89 min Scan# 3243

Delta R.T. -0.00 min

Lab File: BG024878.D

Acq: 22 Nov 2016 3:36


Tgt Ion:228 Resp: 106827

Ion Ratio Lower Upper

228 100

229 19.4 16.3 24.5



226 24.2 21.9 32.9

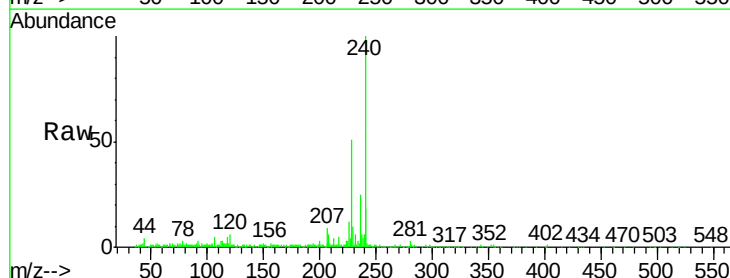


Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

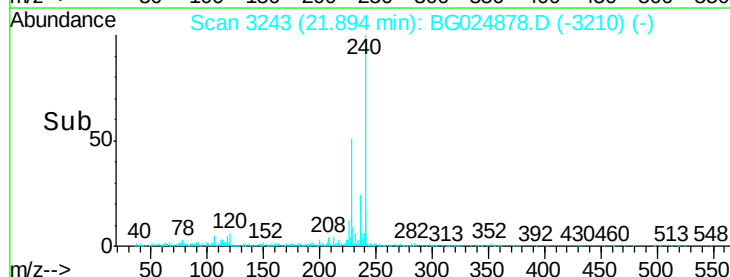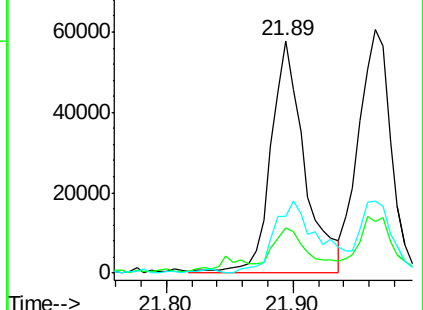

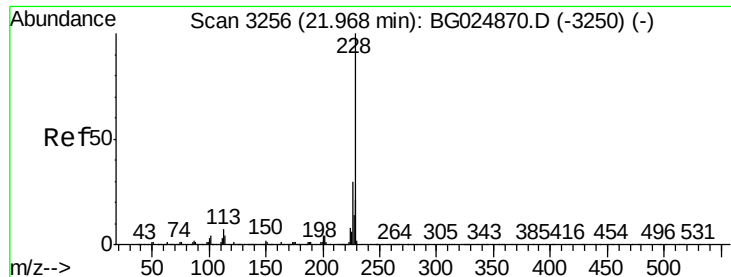

#82

Chrysene

Concen: 1.72 ng/ul

RT: 21.96 min Scan# 3255

Delta R.T. -0.00 min

Lab File: BG024878.D

Acq: 22 Nov 2016 3:36

Instrument :

BNA_G

ClientSampleId :

JHSS7


Tgt Ion:228 Resp: 105463

Ion Ratio Lower Upper

228 100

226 29.7 24.0 36.0




229 21.2 16.9 25.3

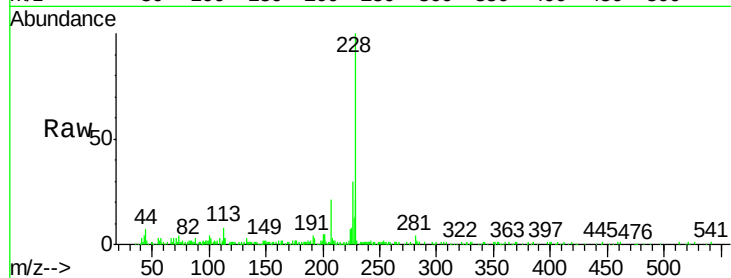

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

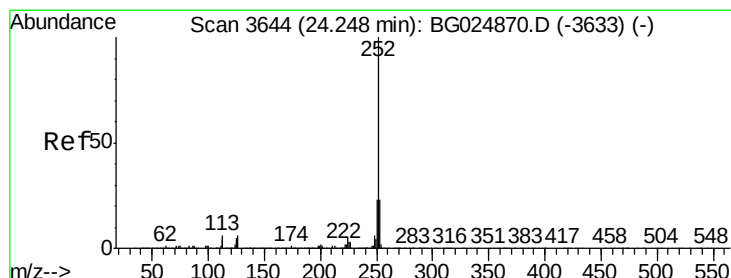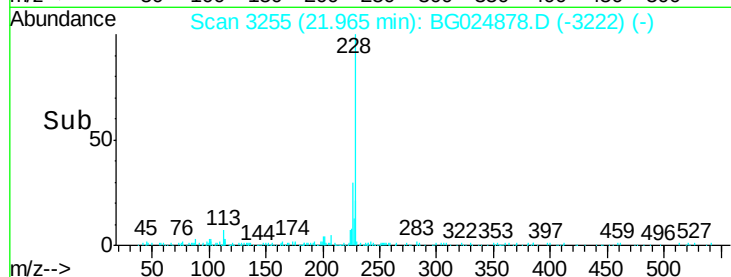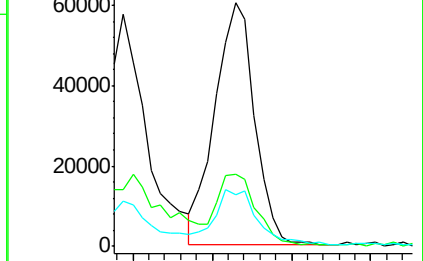

#85

Benzo(b)fluoranthene

Concen: 1.74 ng/ul

RT: 24.26 min Scan# 3645

Delta R.T. 0.01 min

Lab File: BG024878.D

Acq: 22 Nov 2016 3:36


Tgt Ion:252 Resp: 116181

Ion Ratio Lower Upper

252 100

253 20.6 17.7 26.5



125 9.7 4.0 6.0#

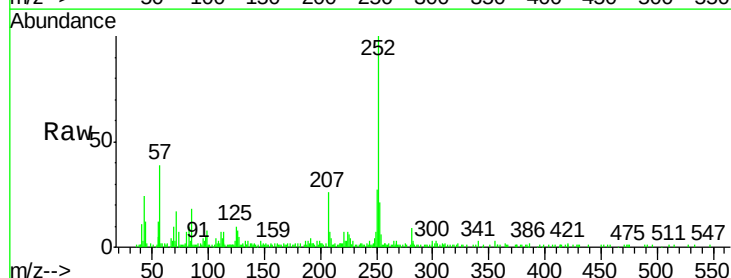


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

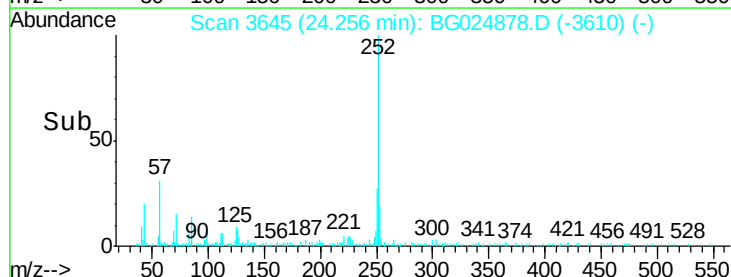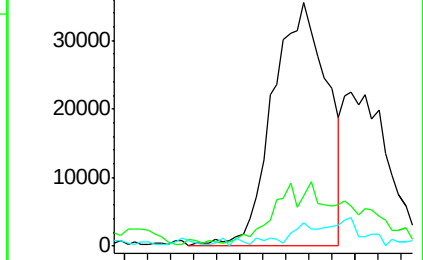

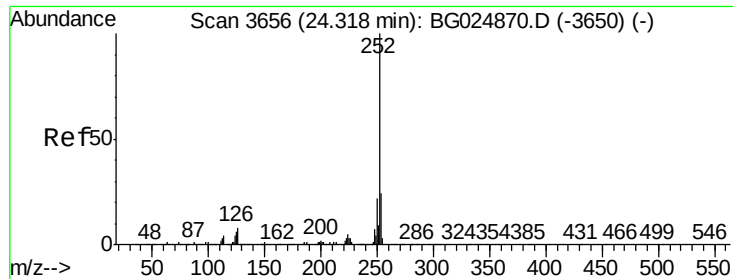

#86

Benzo(k)fluoranthene

Concen: 1.84 ng/ul

RT: 24.26 min Scan# 3645

Delta R.T. -0.06 min

Lab File: BG024878.D

Acq: 22 Nov 2016 3:36





Instrument :

BNA_G

ClientSampleId :

JHSS7

Tgt Ion:	252	Resp:	116181
Ion Ratio	Lower	Upper	
252	100		
253	20.6	18.5	27.7
125	9.7	4.1	6.1#

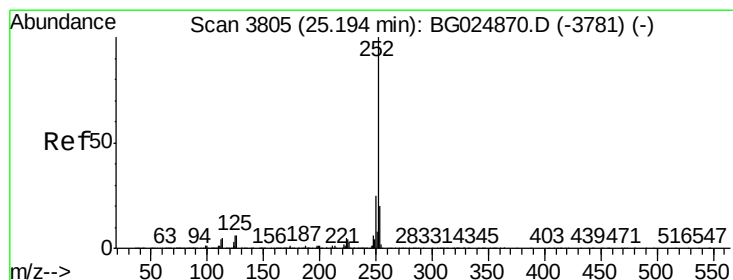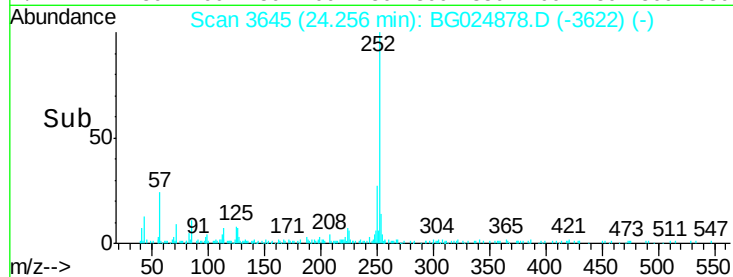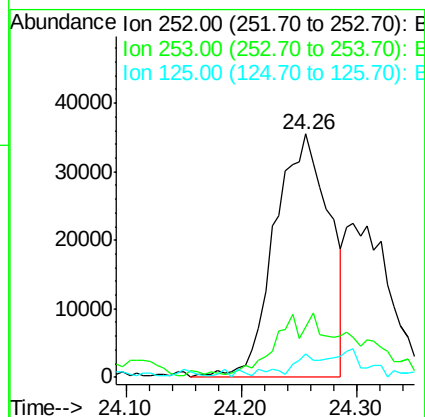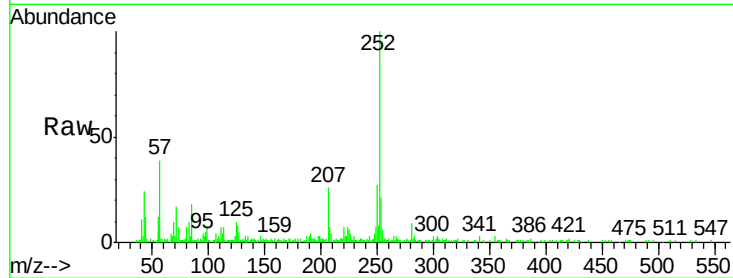

#88

Benzo(a)pyrene

Concen: 1.58 ng/ul

RT: 25.18 min Scan# 3803

Delta R.T. -0.01 min

Lab File: BG024878.D

Acq: 22 Nov 2016 3:36

Tgt Ion:	252	Resp:	102023
Ion Ratio	Lower	Upper	
252	100		
253	34.6	17.8	26.6#
125	7.8	5.4	8.0

