


Data Path : Z:\HPCHEM1\BNA G\DATA\BG112117\
 Data File : BG031151.D
 Acq On : 21 Nov 2017 12:33
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG111017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Nov 10 15:38:25 2017

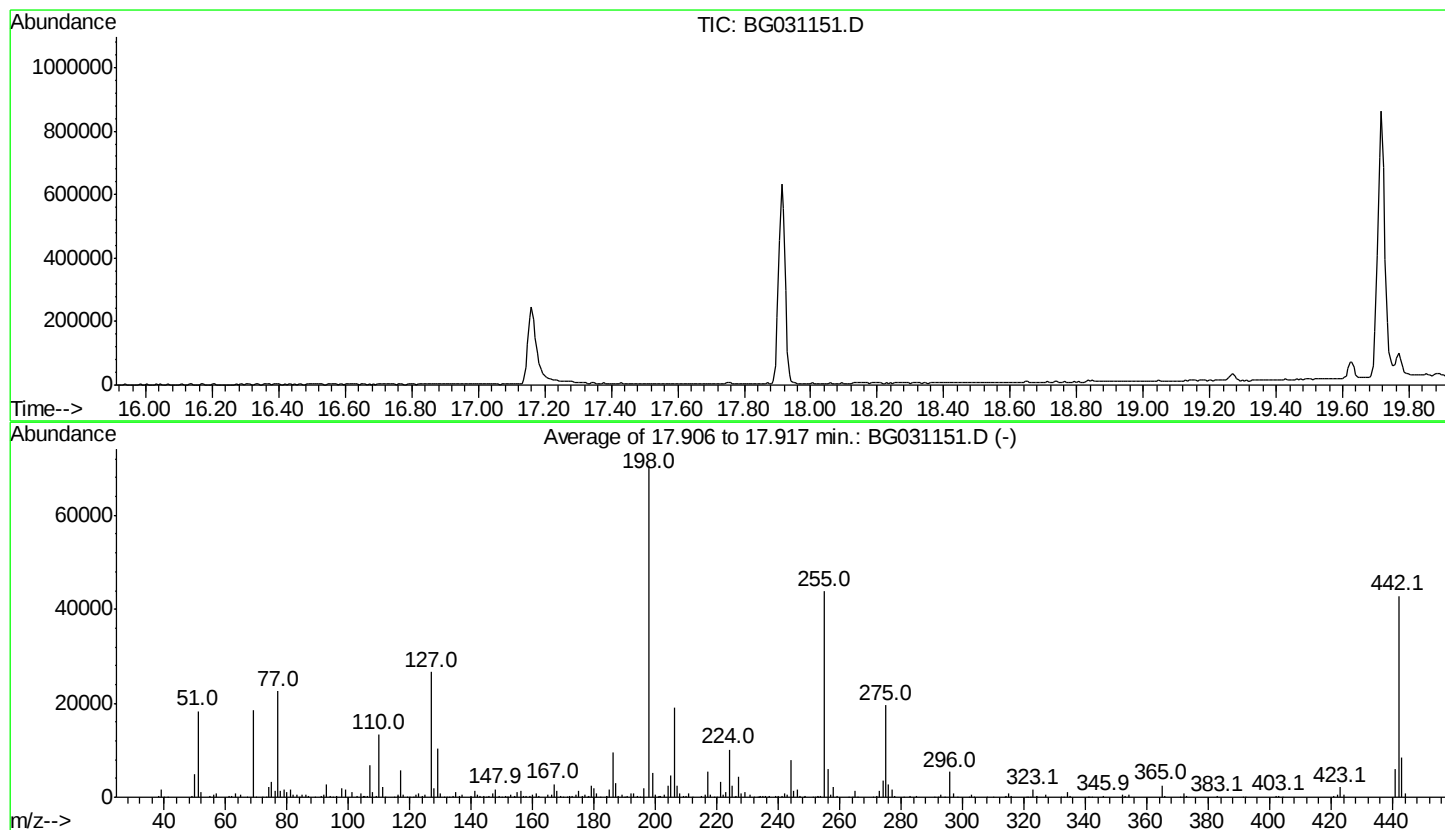

AutoFind: Scans 2488, 2489, 2490; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.9	18309	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	26.4	18644	PASS
70	69	0.00	2	0.2	36	PASS
127	198	10	80	37.8	26669	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	70581	PASS
199	198	5	9	7.2	5105	PASS
275	198	10	60	27.6	19493	PASS
365	198	1	100	3.5	2487	PASS
441	442	0.01	24	14.2	6071	PASS
442	198	50	100	60.7	42816	PASS
443	442	15	24	20.1	8589	PASS