


Data Path : Z:\HPCHEM1\BNA G\DATA\BG112117\
 Data File : BG031168.D
 Acq On : 22 Nov 2017 00:50
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG111017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Nov 10 15:38:25 2017

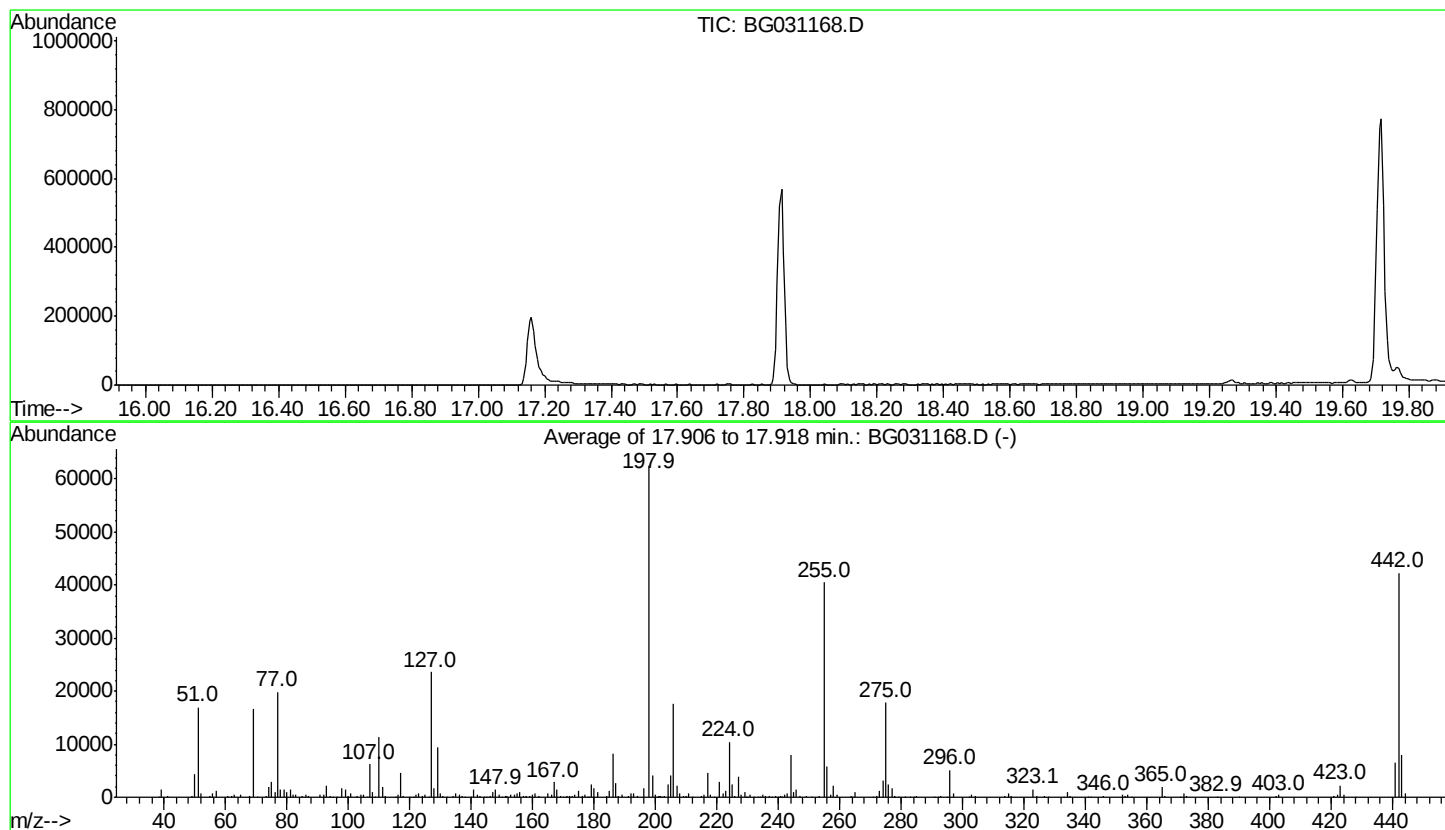

AutoFind: Scans 2488, 2489, 2490; Background Corrected with Scan 2481

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.2	16975	PASS
68	69	0.00	2	0.9	151	PASS
69	198	0.00	100	26.5	16545	PASS
70	69	0.00	2	0.4	65	PASS
127	198	10	80	37.7	23586	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	62493	PASS
199	198	5	9	6.5	4089	PASS
275	198	10	60	28.4	17765	PASS
365	198	1	100	3.2	2012	PASS
441	442	0.01	24	15.3	6459	PASS
442	198	50	100	67.6	42240	PASS
443	442	15	24	18.7	7906	PASS