
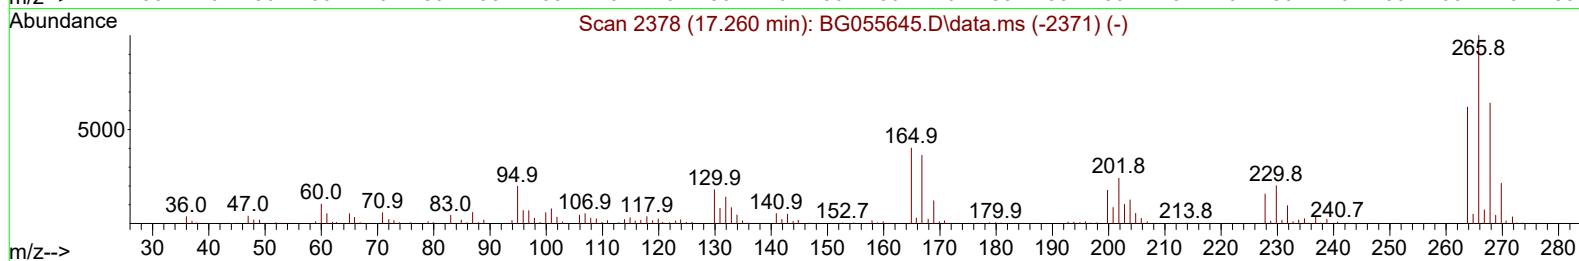
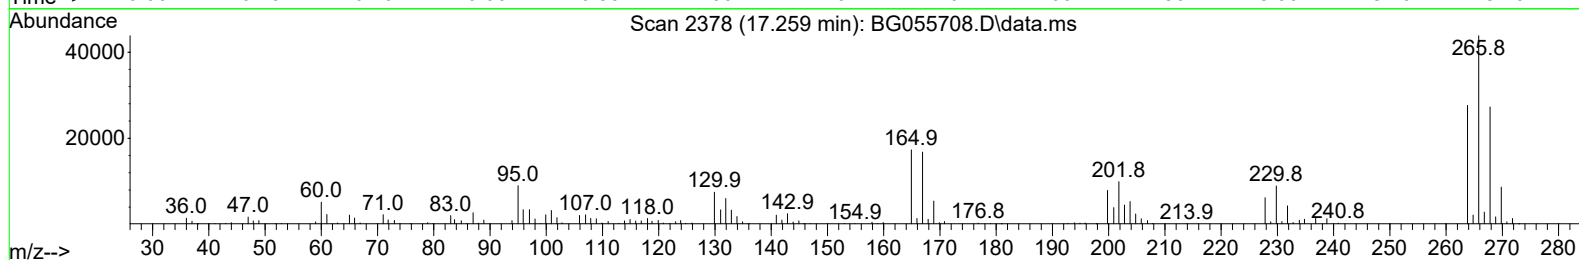


Quant Time: Nov 22 06:13:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 17 02:02:46 2022
Response via : Initial Calibration

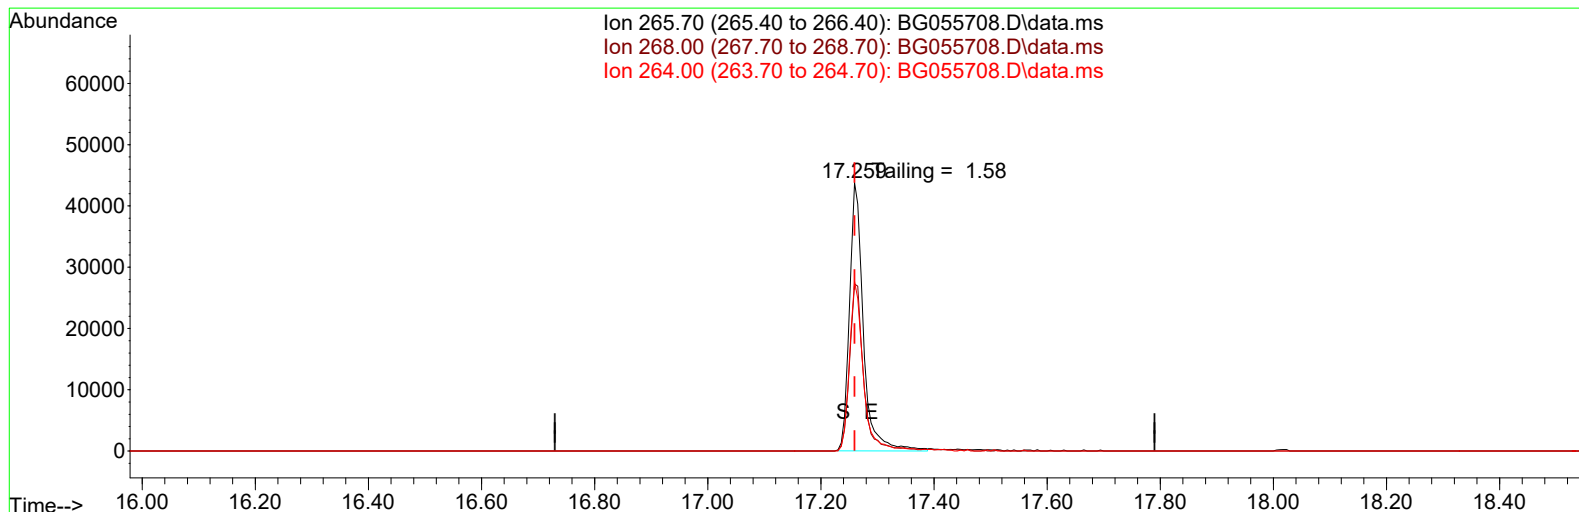

TIC: BG055708.D\data.ms

(70) Pentachlorophenol (C)




17.259min (-0.000) 24483.83 ng

response **75879**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	62.24
264.00	61.90	63.09
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112122\
Data File : BG055708.D
Acq On : 21 Nov 2022 9:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 22 06:13:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 17 02:02:46 2022
Response via : Initial Calibration

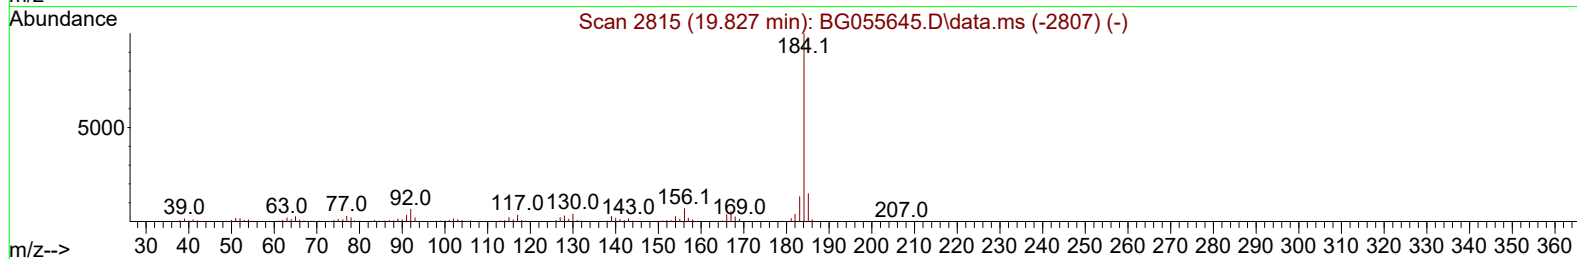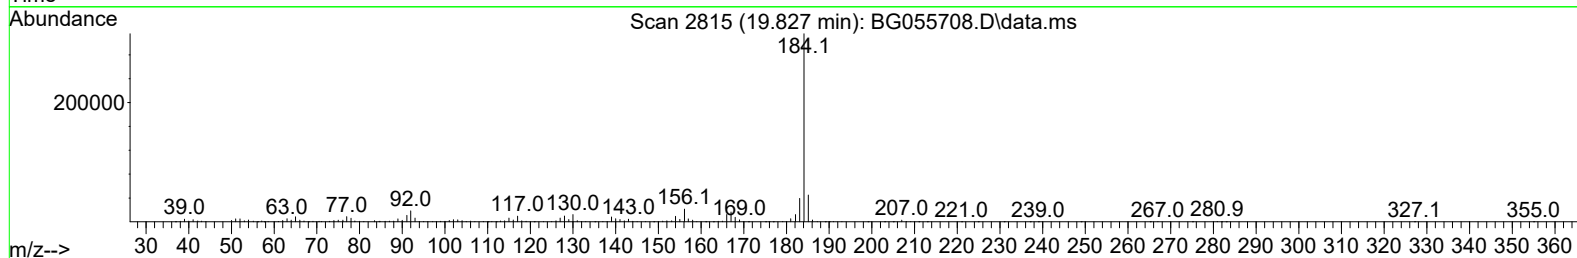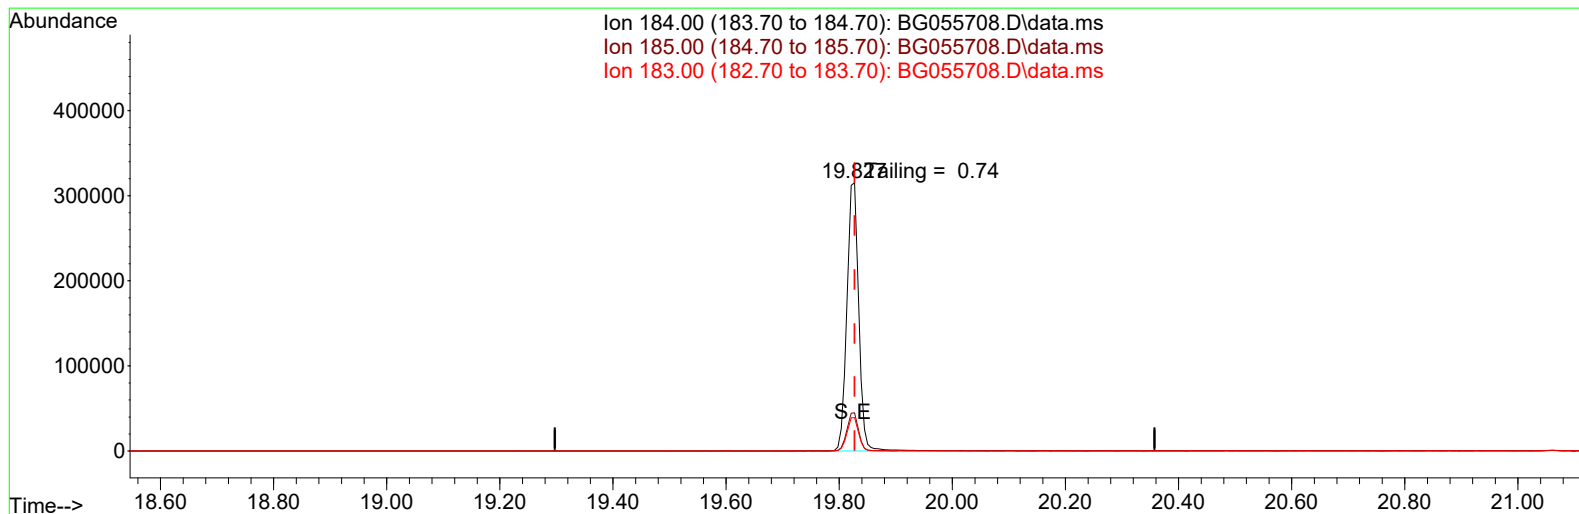

TIC: BG055708.D\data.ms

(77) Benzidine**19.827min (-0.000) 148227.09 ng****response 459507**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.27
183.00	13.20	12.49
0.00	0.00	0.00