
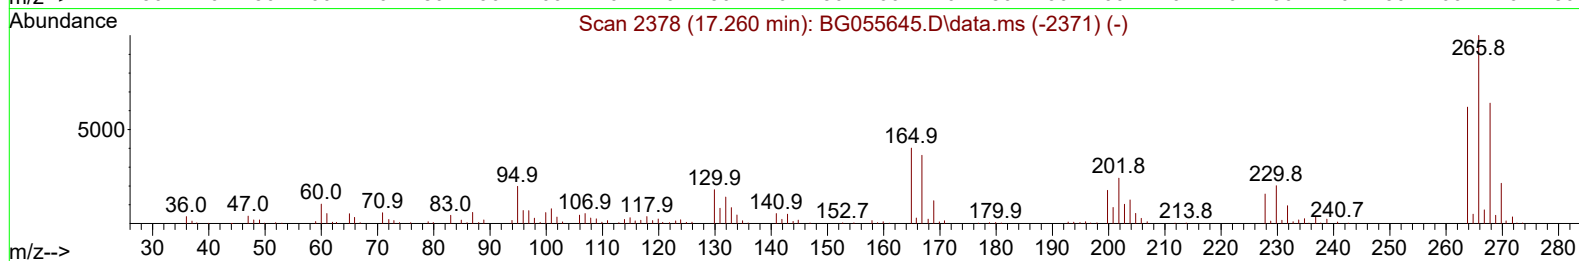
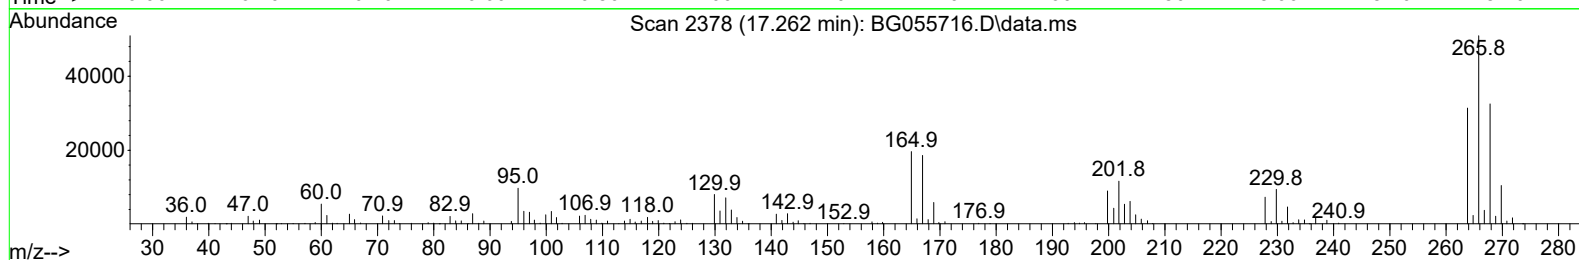


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112122\
Data File : BG055716.D
Acq On : 21 Nov 2022 15:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 22 06:15:17 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 17 02:02:46 2022
Response via : Initial Calibration

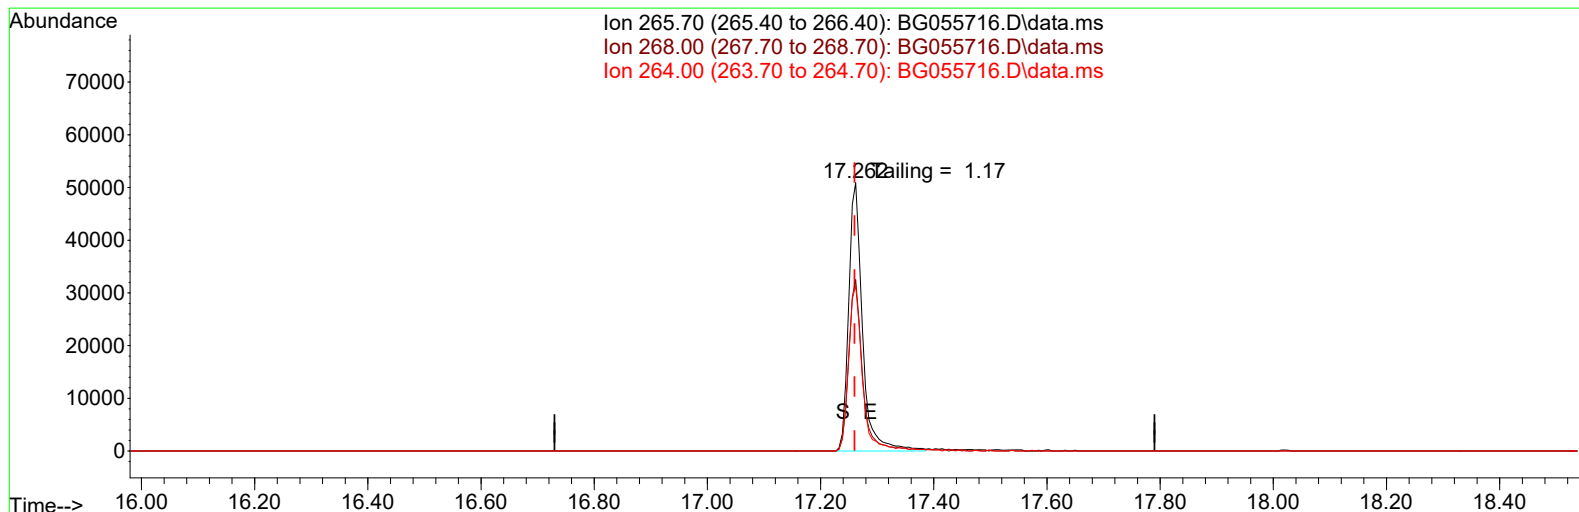

TIC: BG055716.D\data.ms

(70) Pentachlorophenol (C)




17.262min (+ 0.002) 26042.22 ng

response 86948

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	63.89
264.00	61.90	61.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112122\
Data File : BG055716.D
Acq On : 21 Nov 2022 15:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 22 06:15:17 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 17 02:02:46 2022
Response via : Initial Calibration

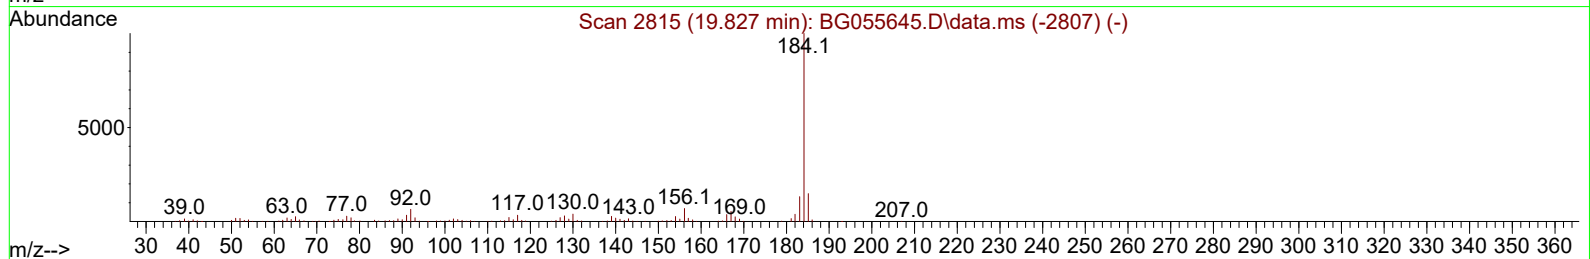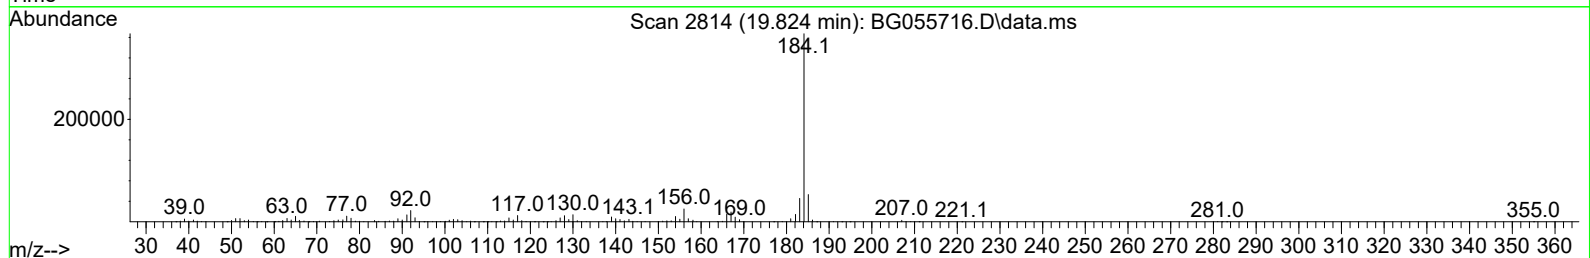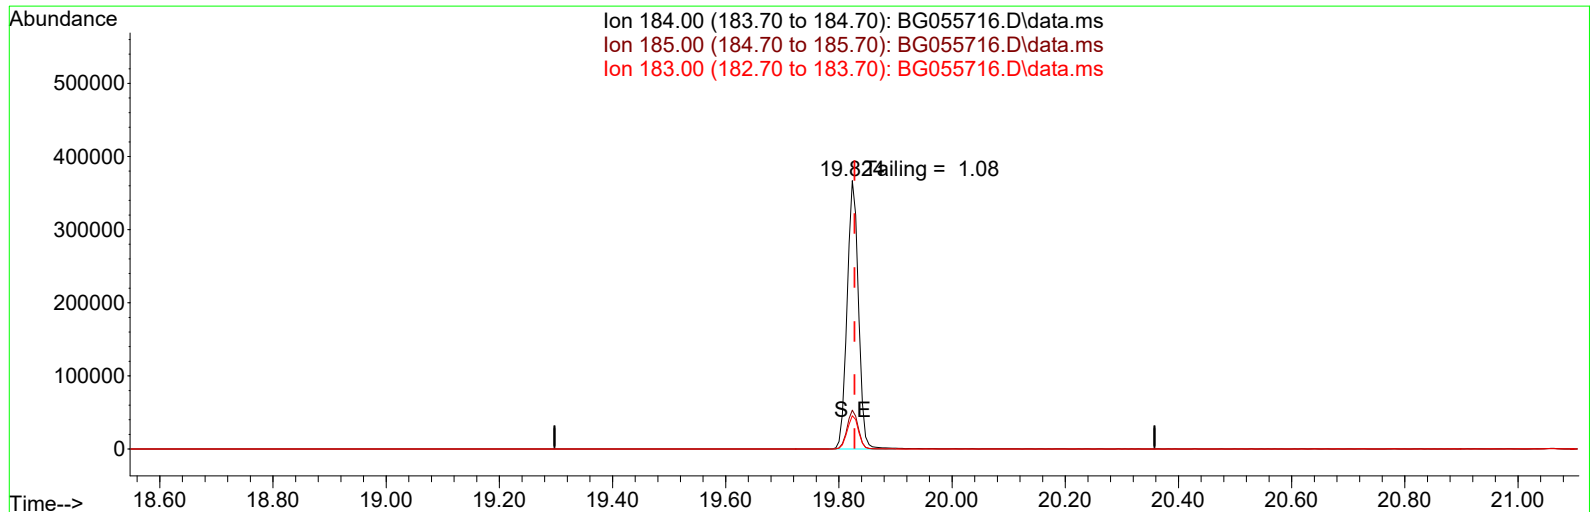

TIC: BG055716.D\data.ms

(77) Benzidine**19.824min (-0.004) 390456.14 ng****response 514881**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.51
183.00	13.20	12.43
0.00	0.00	0.00