

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112122\
 Data File : BG055724.D
 Acq On : 21 Nov 2022 21:08
 Operator : CG/JU
 Sample : N5678-15
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 250FB-BP-BACKFILL-08

Quant Time: Nov 22 02:08:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 17 02:02:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.244	152	34004	20.000	ng	0.00
21) Naphthalene-d8	11.071	136	160088	20.000	ng	-0.01
39) Acenaphthene-d10	14.866	164	124726	20.000	ng	0.00
64) Phenanthrene-d10	17.610	188	285933	20.000	ng	0.00
76) Chrysene-d12	21.905	240	269438	20.000	ng	-0.01
86) Perylene-d12	25.319	264	281881	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.777	112	185561	98.637	ng	0.00
7) Phenol-d6	7.387	99	257236	102.720	ng	0.00
23) Nitrobenzene-d5	9.414	82	158475	52.322	ng	-0.01
42) 2,4,6-Tribromophenol	16.353	330	139071	79.184	ng	0.00
45) 2-Fluorobiphenyl	13.491	172	443350	53.252	ng	0.00
79) Terphenyl-d14	20.195	244	776662	57.654	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112122\
Data File : BG055724.D
Acq On : 21 Nov 2022 21:08
Operator : CG/JU
Sample : N5678-15
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
250FB-BP-BACKFILL-08

Quant Time: Nov 22 02:08:14 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 17 02:02:46 2022
Response via : Initial Calibration




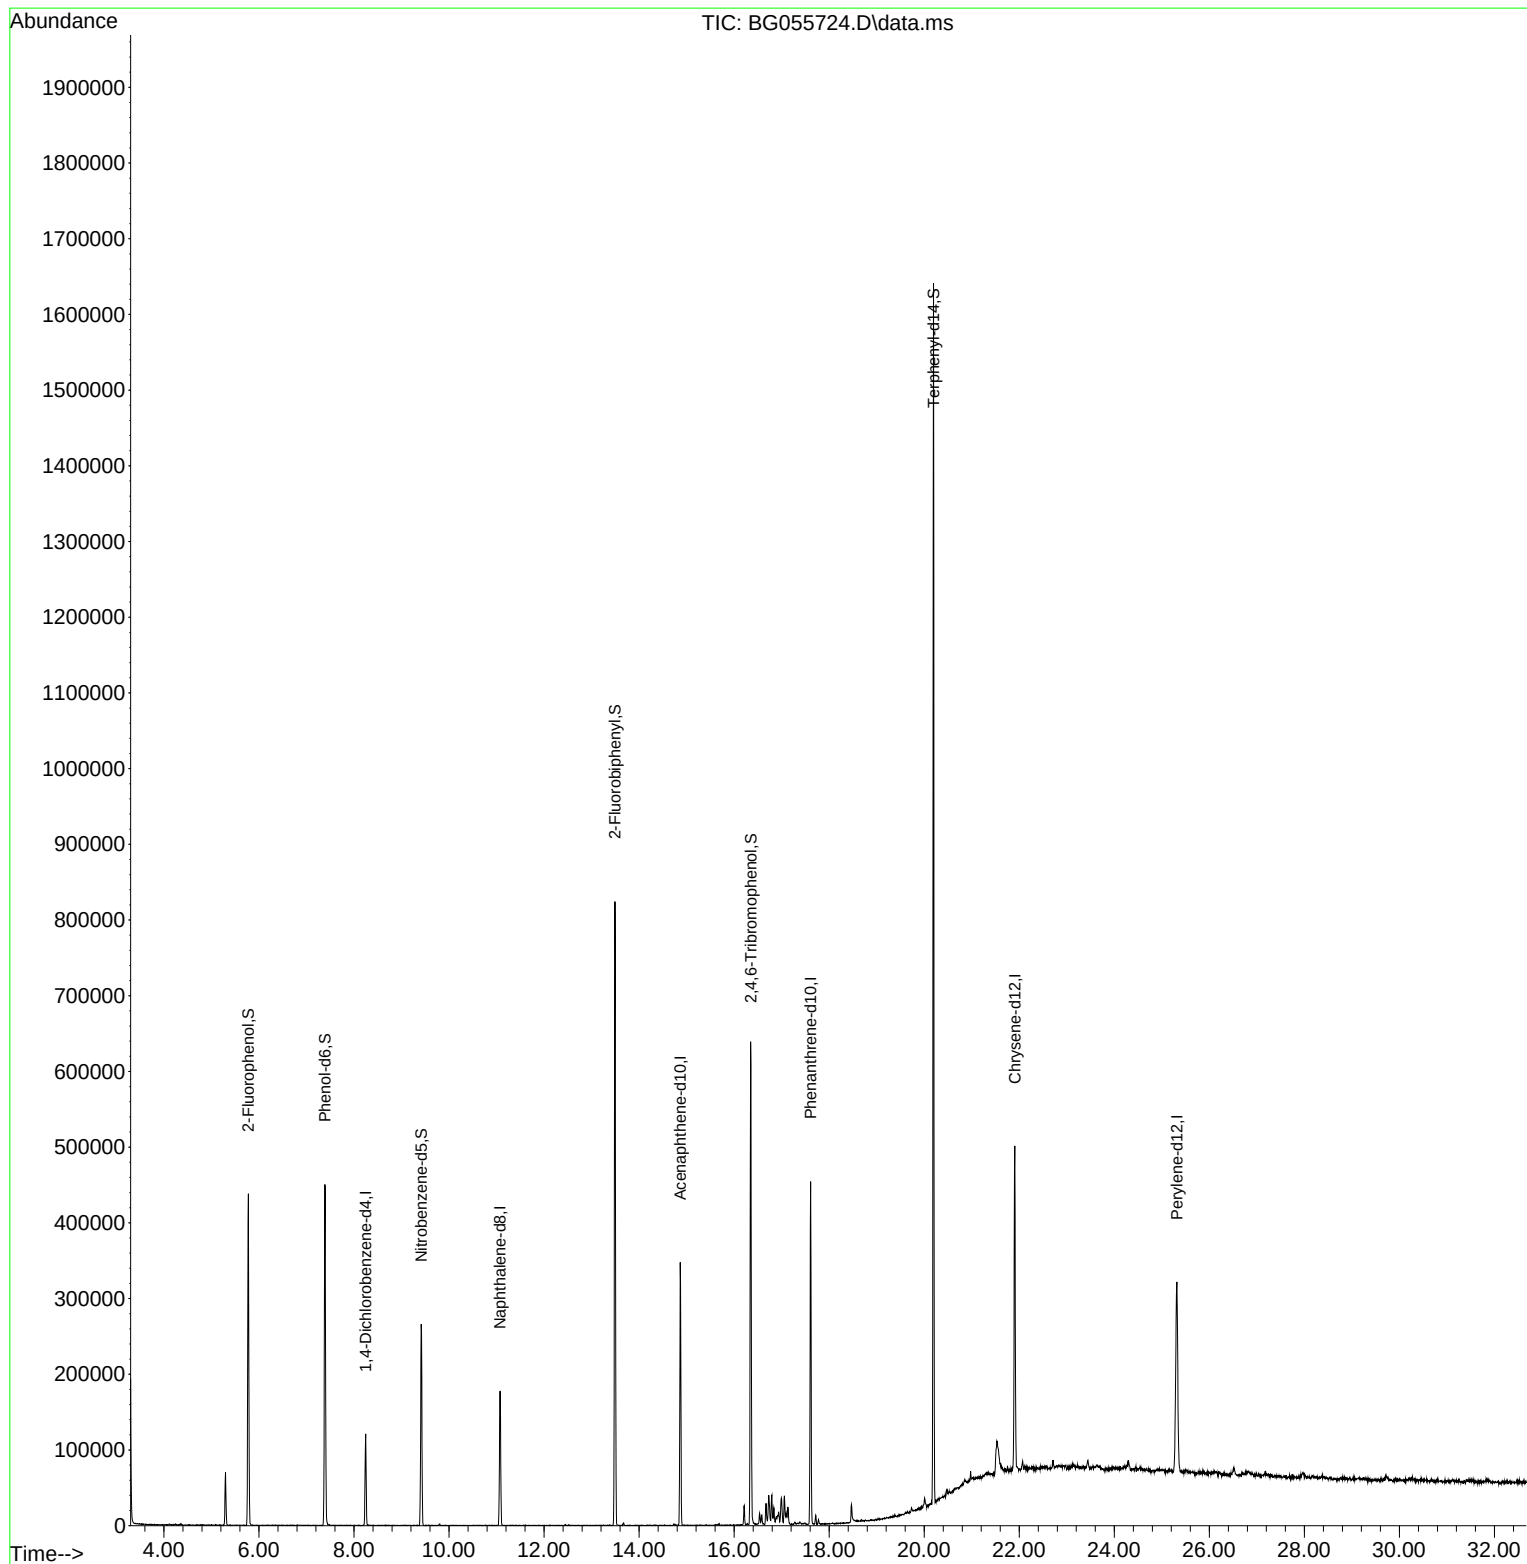


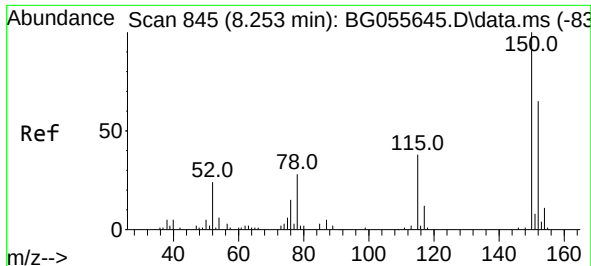

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.244 min Scan# 84
Delta R.T. -0.009 min
Lab File: BG055724.D
Acq: 21 Nov 2022 21:08




Instrument :
BNA_G
ClientSampleId :
250FB-BP-BACKFILL-08


Tgt Ion:152 Resp: 34004
Ion Ratio Lower Upper
152 100
150 154.6 123.0 184.6
115 61.6 47.0 70.4

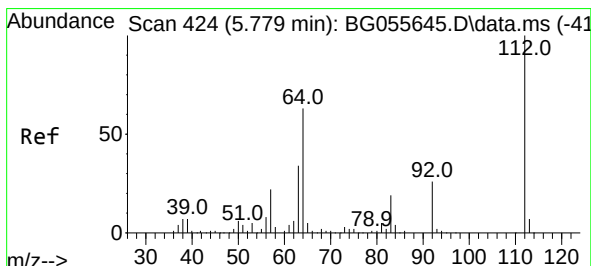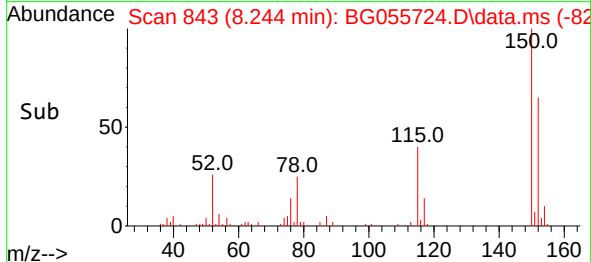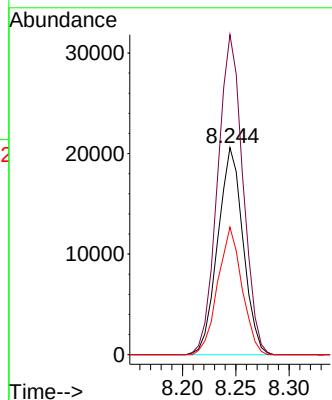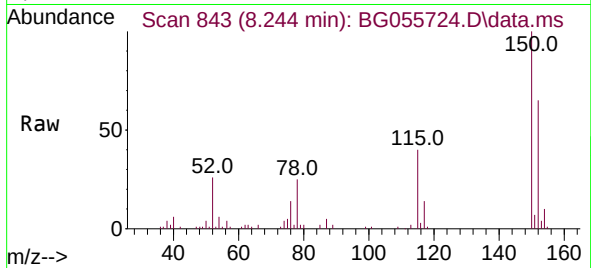

#5
2-Fluorophenol
Concen: 98.637 ng
RT: 5.777 min Scan# 423
Delta R.T. -0.002 min
Lab File: BG055724.D
Acq: 21 Nov 2022 21:08

Tgt Ion:112 Resp: 185561
Ion Ratio Lower Upper
112 100
64 64.0 50.6 76.0
63 33.9 27.5 41.3


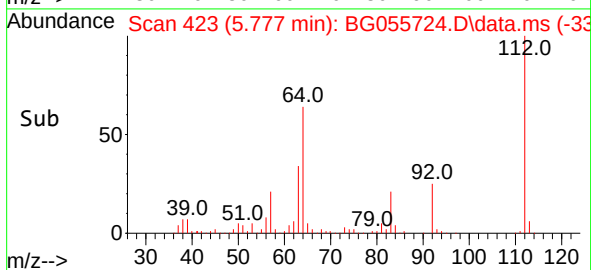
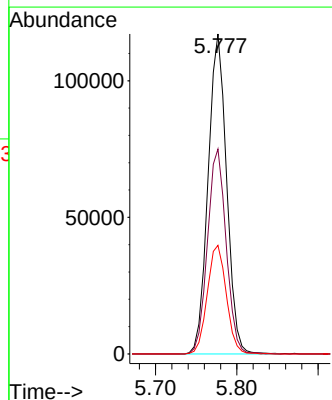
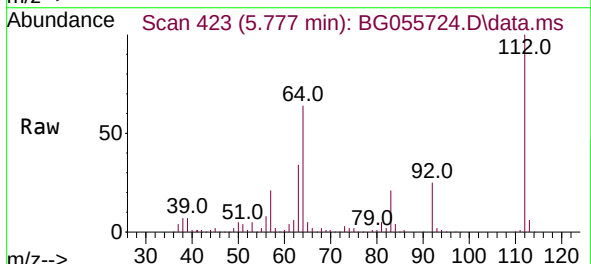


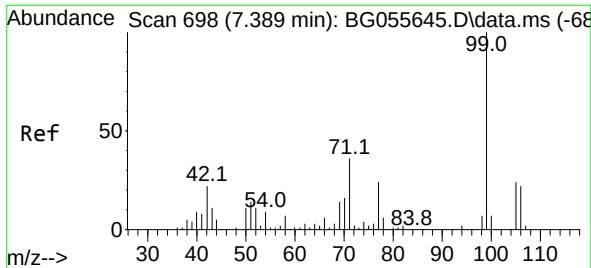

#7
Phenol-d6
Concen: 102.720 ng
RT: 7.387 min Scan# 69
Delta R.T. -0.002 min
Lab File: BG055724.D
Acq: 21 Nov 2022 21:08




Instrument :
BNA_G
ClientSampleId :
250FB-BP-BACKFILL-08


Tgt Ion: 99 Resp: 257236
Ion Ratio Lower Upper
99 100
42 22.2 18.0 27.0
71 36.8 29.0 43.6

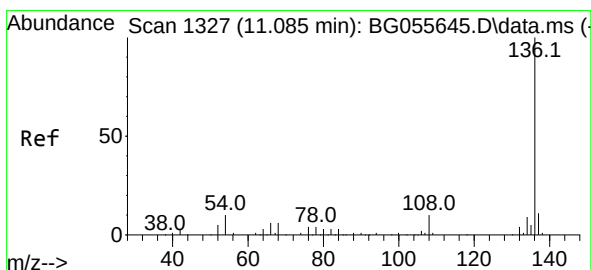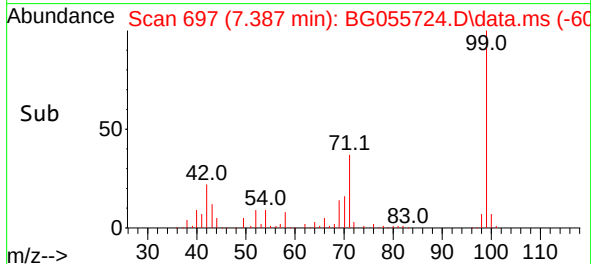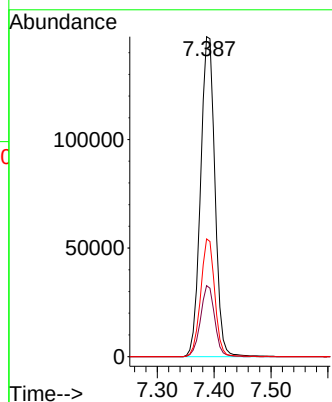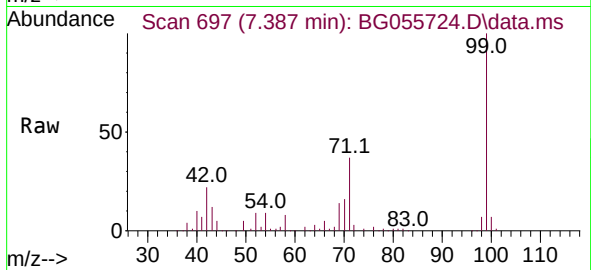

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 11.071 min Scan# 1324
Delta R.T. -0.014 min
Lab File: BG055724.D
Acq: 21 Nov 2022 21:08

Tgt Ion:136 Resp: 160088
Ion Ratio Lower Upper
136 100
137 10.8 9.0 13.6
54 9.3 7.8 11.6
68 5.6 5.0 7.4

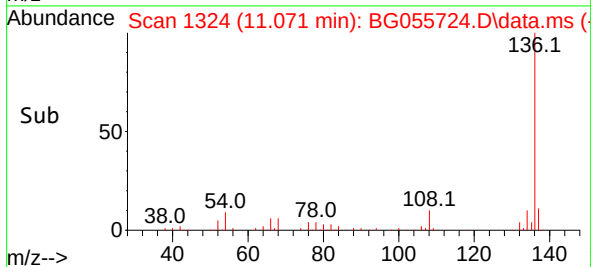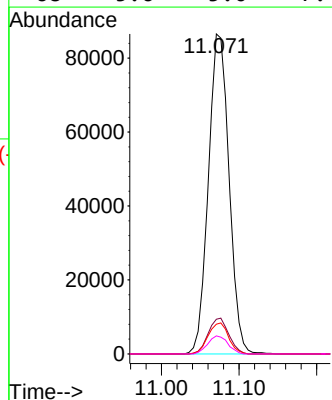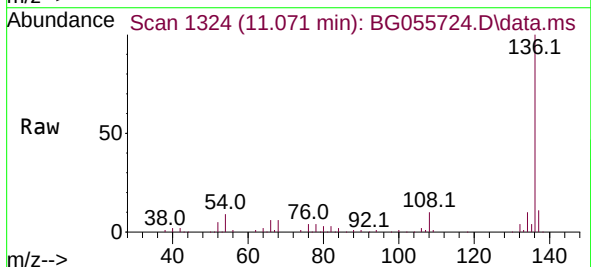

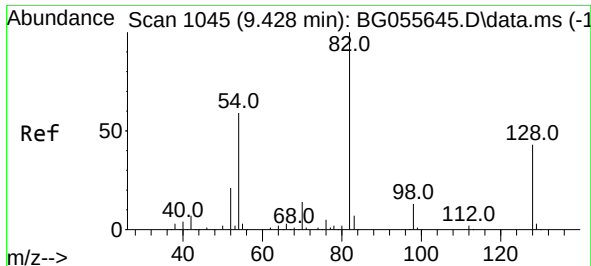

#23

Nitrobenzene-d5

Concen: 52.322 ng

RT: 9.414 min Scan# 1042

Delta R.T. -0.014 min

Lab File: BG055724.D

Acq: 21 Nov 2022 21:08

Instrument :

BNA_G

ClientSampleId :

250FB-BP-BACKFILL-08





Tgt Ion: 82 Resp: 158475

Ion Ratio Lower Upper

82 100

128 42.4 34.1 51.1

54 56.9 47.3 70.9

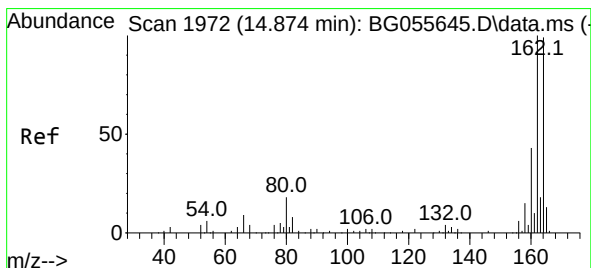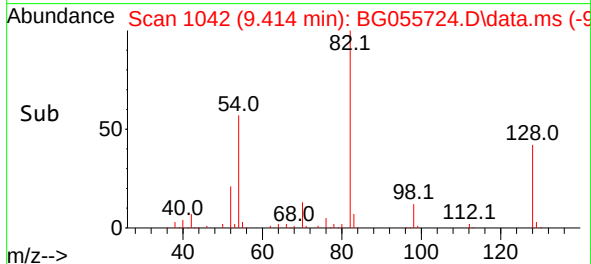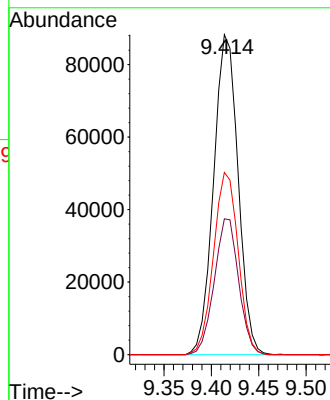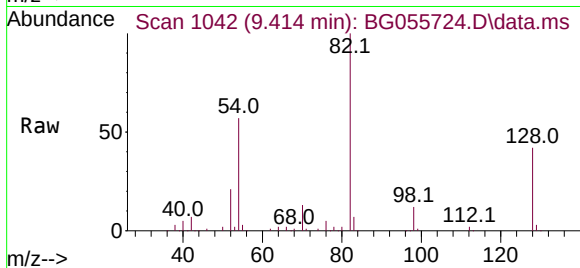

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.866 min Scan# 1970

Delta R.T. -0.008 min

Lab File: BG055724.D

Acq: 21 Nov 2022 21:08




Tgt Ion:164 Resp: 124726


Ion Ratio Lower Upper

164 100

162 101.0 81.1 121.7

160 43.8 34.8 52.2


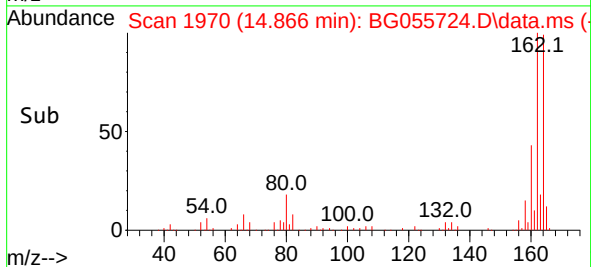
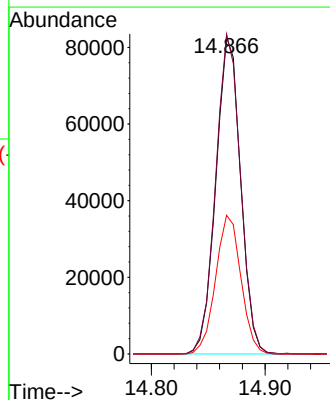
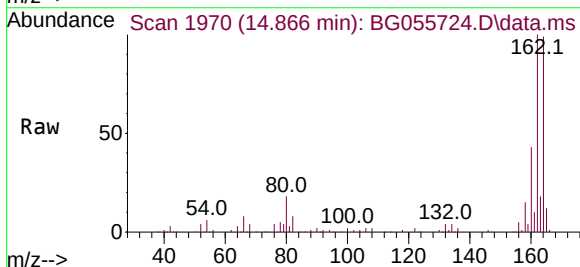


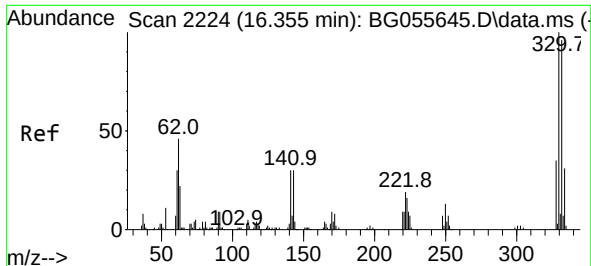

#42
2,4,6-Tribromophenol
Concen: 79.184 ng
RT: 16.353 min Scan# 21
Delta R.T. -0.002 min
Lab File: BG055724.D
Acq: 21 Nov 2022 21:08




Instrument :
BNA_G
ClientSampleId :
250FB-BP-BACKFILL-08


Tgt Ion:330 Resp: 139071
Ion Ratio Lower Upper
330 100
332 96.8 77.8 116.8
141 30.3 23.9 35.9

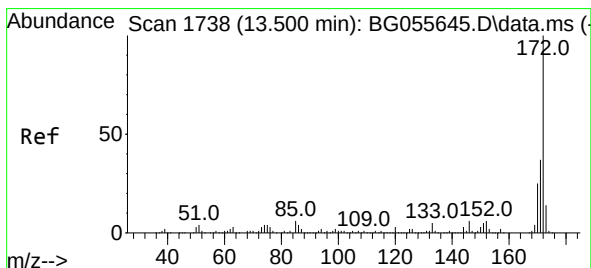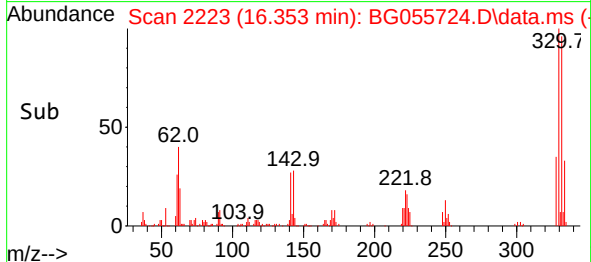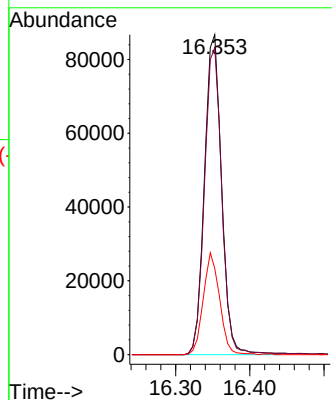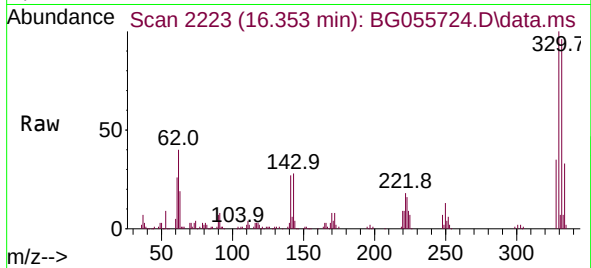

#45
2-Fluorobiphenyl
Concen: 53.252 ng
RT: 13.491 min Scan# 1736
Delta R.T. -0.008 min
Lab File: BG055724.D
Acq: 21 Nov 2022 21:08

Tgt Ion:172 Resp: 443350
Ion Ratio Lower Upper
172 100
171 36.7 29.8 44.6
170 24.5 20.2 30.4


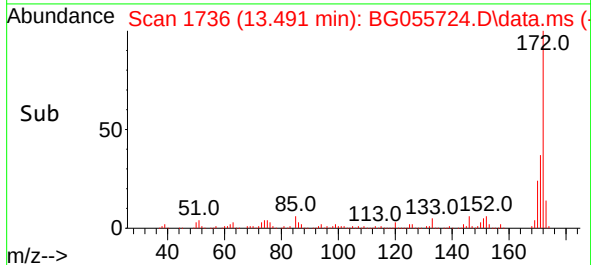
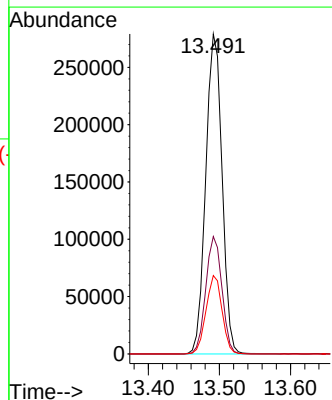
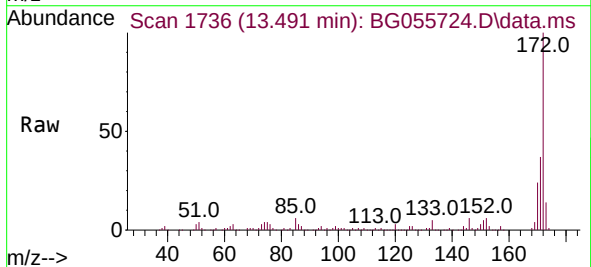


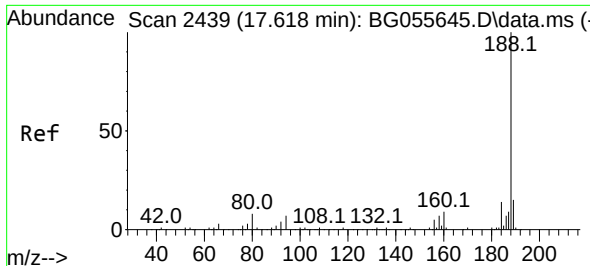

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.610 min Scan# 2439
Delta R.T. -0.008 min
Lab File: BG055724.D
Acq: 21 Nov 2022 21:08




Instrument :
BNA_G
ClientSampleId :
250FB-BP-BACKFILL-08


Tgt Ion:188 Resp: 285933
Ion Ratio Lower Upper
188 100
94 7.1 5.4 8.2
80 8.0 6.6 10.0

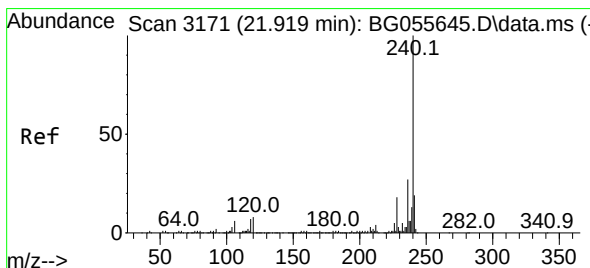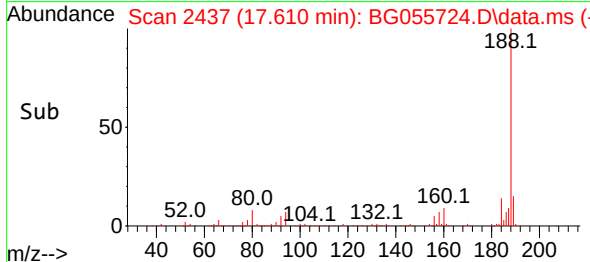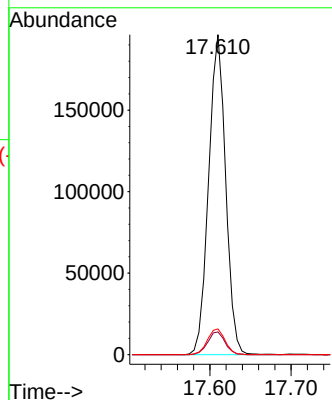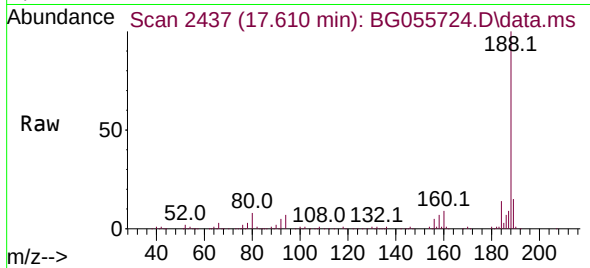

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.905 min Scan# 3168
Delta R.T. -0.014 min
Lab File: BG055724.D
Acq: 21 Nov 2022 21:08

Tgt Ion:240 Resp: 269438
Ion Ratio Lower Upper
240 100
120 7.8 6.3 9.5
236 26.8 21.9 32.9


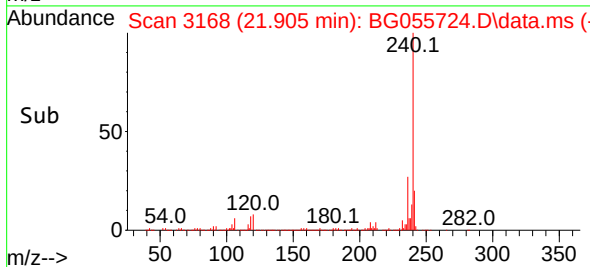
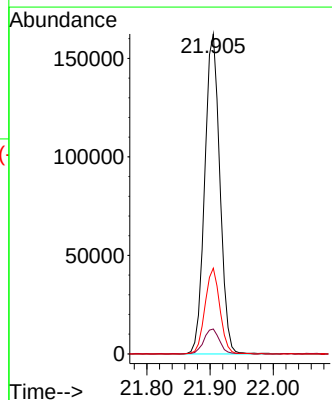
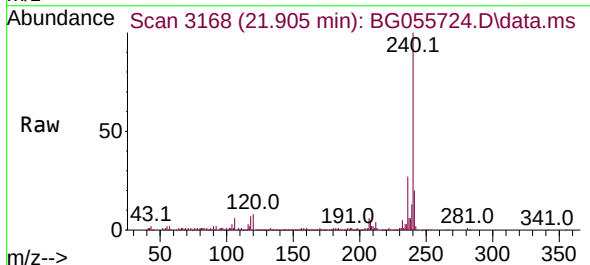


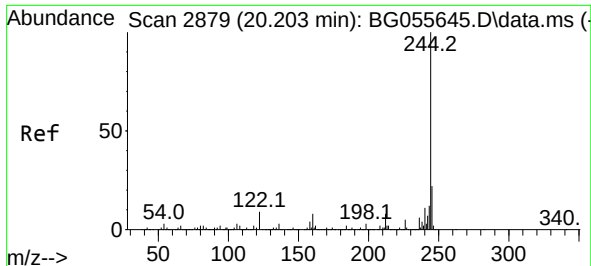

#79
 Terphenyl-d14
 Concen: 57.654 ng
 RT: 20.195 min Scan# 21
 Delta R.T. -0.008 min
 Lab File: BG055724.D
 Acq: 21 Nov 2022 21:08

Instrument :
 BNA_G
 ClientSampleId :
 250FB-BP-BACKFILL-08

Tgt Ion:244 Resp: 776662
 Ion Ratio Lower Upper
 244 100
 212 7.5 6.3 9.5
 122 8.4 6.9 10.3

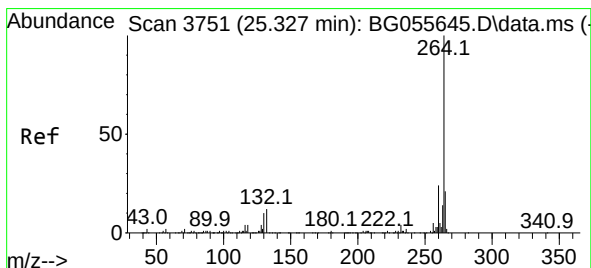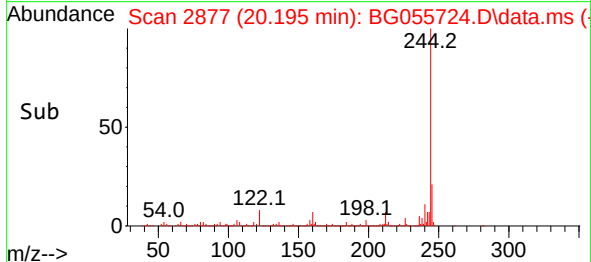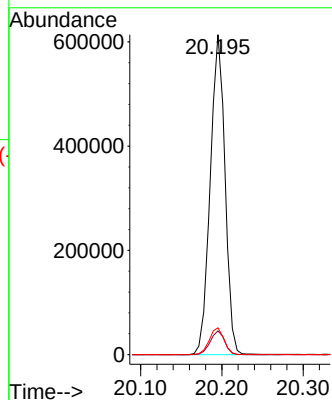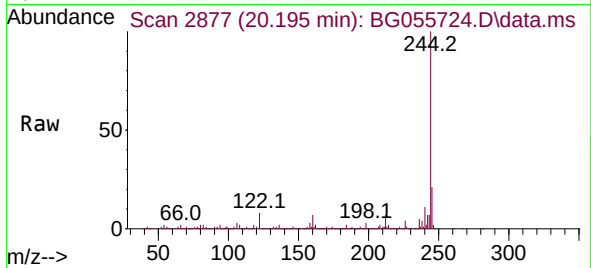

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 25.319 min Scan# 3749
 Delta R.T. -0.008 min
 Lab File: BG055724.D
 Acq: 21 Nov 2022 21:08

Tgt Ion:264 Resp: 281881
 Ion Ratio Lower Upper
 264 100
 260 24.4 19.5 29.3
 265 21.8 17.1 25.7

