

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112122\
 Data File : BG055712.D
 Acq On : 21 Nov 2022 12:41
 Operator : CG/JU
 Sample : N5678-19
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 250FB-BP-BACKFILL-10

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG055712.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.296	337	342	349	rBV	71589	112873	5.72%	0.666%
2	5.778	416	424	435	rBV	499478	816688	41.36%	4.820%
3	7.394	691	699	710	rBV	496815	859403	43.52%	5.073%
4	8.246	835	844	851	rBV	122858	205919	10.43%	1.215%
5	9.421	1036	1044	1051	rBV	286036	521631	26.42%	3.079%
6	11.078	1319	1326	1335	rBV	168845	302500	15.32%	1.785%
7	13.493	1731	1737	1744	rBV	772057	1238369	62.71%	7.309%
8	14.867	1965	1971	1982	rVB	279784	454937	23.04%	2.685%
9	16.213	2196	2200	2206	rVB4	12330	21493	1.09%	0.127%
10	16.354	2217	2224	2234	rBV	714472	1156331	58.56%	6.825%
11	17.611	2432	2438	2443	rBV	375203	578711	29.31%	3.416%
12	18.023	2501	2508	2514	rBV	86651	244665	12.39%	1.444%
13	18.463	2576	2583	2608	rVB2	507724	1718881	87.05%	10.145%
14	19.251	2711	2717	2725	rVB	88198	200906	10.17%	1.186%
15	19.726	2790	2798	2816	rVB	625580	1857739	94.08%	10.965%
16	20.161	2866	2872	2874	rBV	214999	349469	17.70%	2.063%
17	20.197	2874	2878	2884	rVB	1512910	1974693	100.00%	11.655%
18	20.943	2999	3005	3015	rVB	288841	530556	26.87%	3.132%
19	21.754	3136	3143	3150	rVB	282824	579064	29.32%	3.418%
20	21.906	3164	3169	3176	rVB2	356139	594167	30.09%	3.507%
21	22.664	3292	3298	3311	rVB	277822	675017	34.18%	3.984%
22	23.734	3473	3480	3491	rVB	217503	584878	29.62%	3.452%
23	24.979	3686	3692	3706	rVB2	192328	622044	31.50%	3.672%
24	25.320	3743	3750	3763	rVB2	240451	741408	37.55%	4.376%




Sum of corrected areas: 16942342

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112122\
Data File : BG055712.D
Acq On : 21 Nov 2022 12:41
Operator : CG/JU
Sample : N5678-19
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
250FB-BP-BACKFILL-10

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

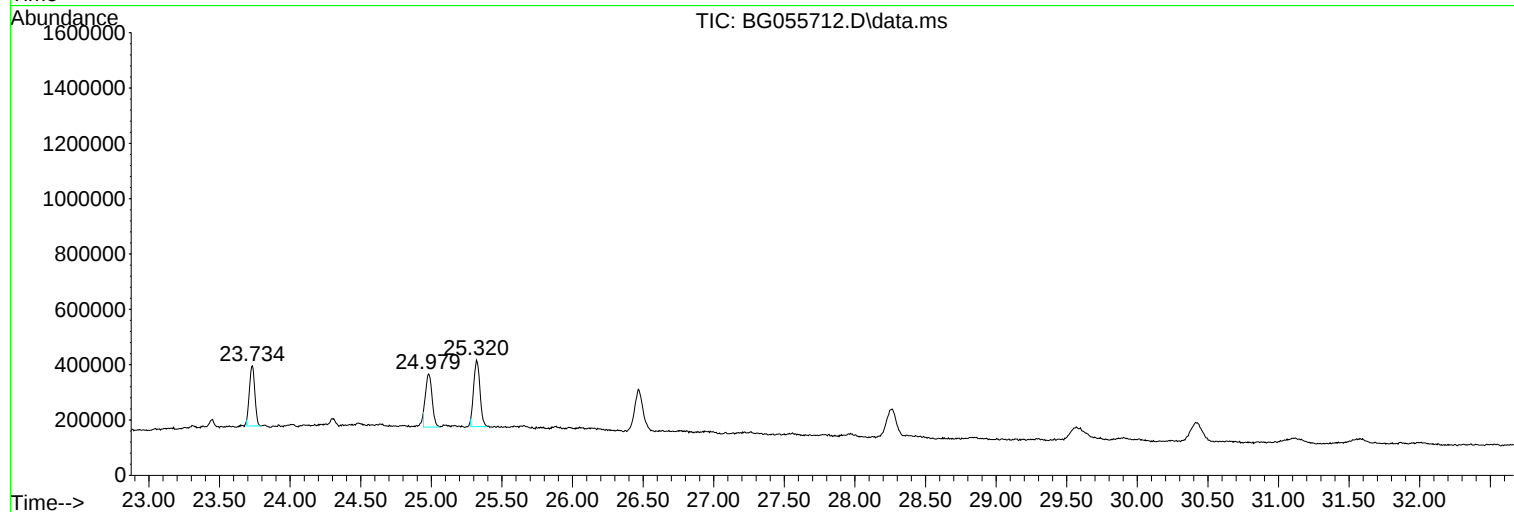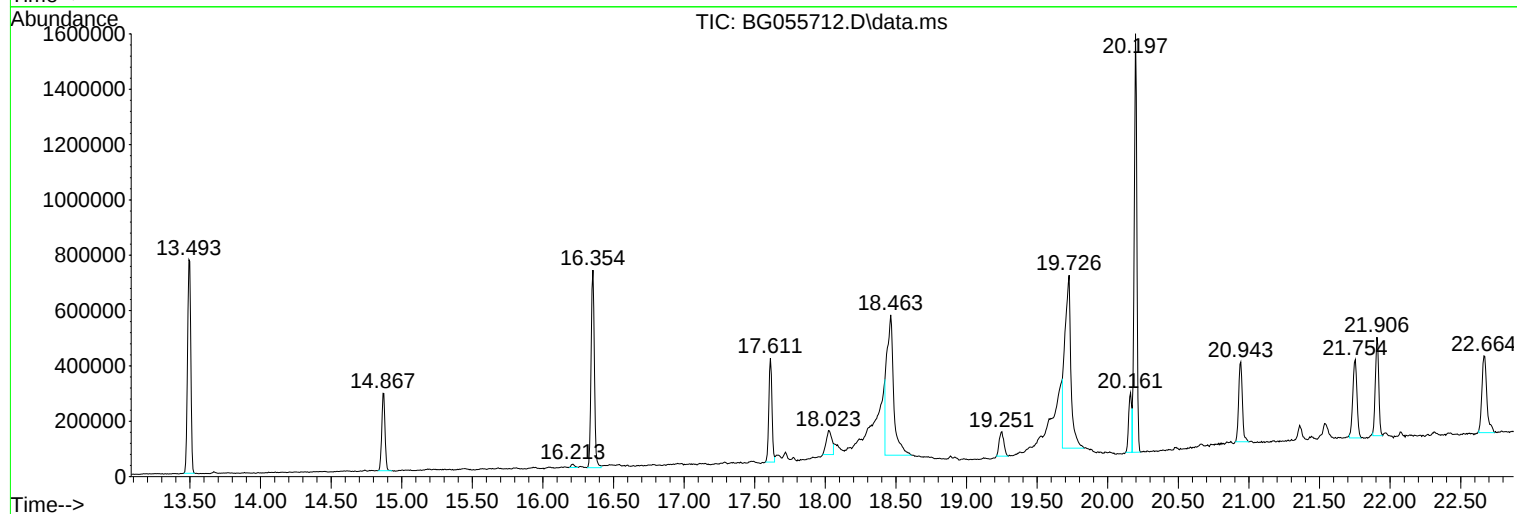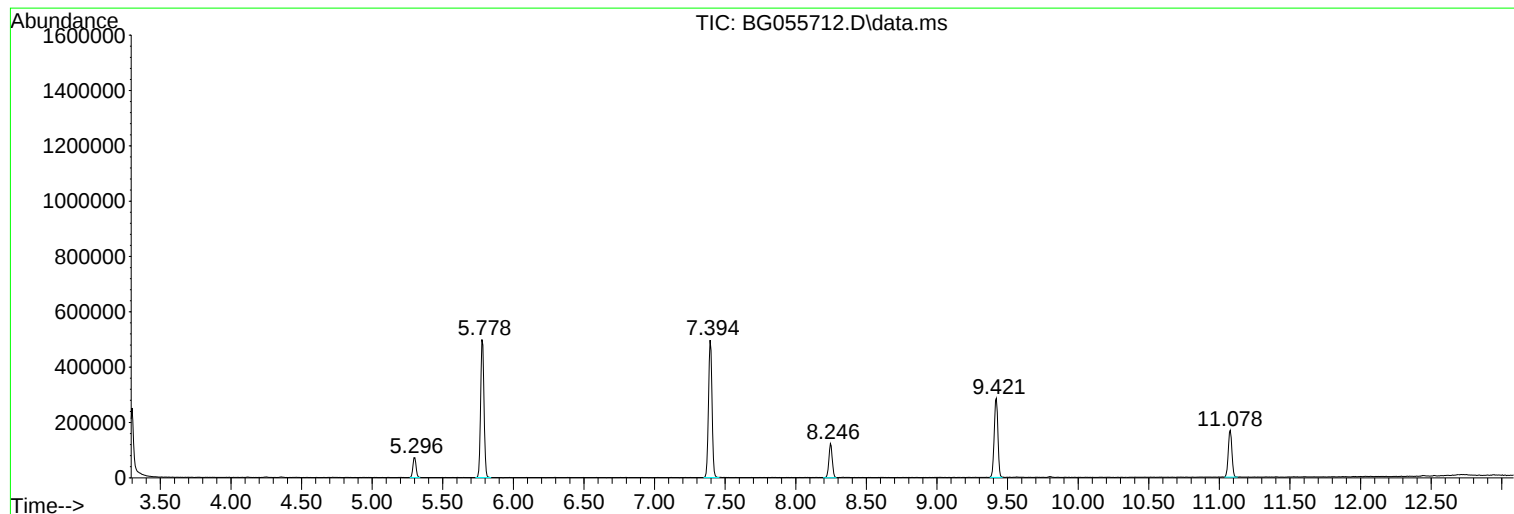

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112122\
Data File : BG055712.D
Acq On : 21 Nov 2022 12:41
Operator : CG/JU
Sample : N5678-19
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
250FB-BP-BACKFILL-10

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112122\
Data File : BG055712.D
Acq On : 21 Nov 2022 12:41
Operator : CG/JU
Sample : N5678-19
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
250FB-BP-BACKFILL-10

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------