

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112122\
 Data File : BG055713.D
 Acq On : 21 Nov 2022 13:22
 Operator : CG/JU
 Sample : N5678-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 250FB-BP-BACKFILL-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG055713.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.297	336	342	351	rVB	91568	139830	5.79%	1.247%
2	5.779	417	424	439	rVB	577466	924757	38.31%	8.246%
3	7.394	691	699	717	rVB	588522	999474	41.41%	8.912%
4	8.246	837	844	850	rBV	119121	200026	8.29%	1.784%
5	9.416	1035	1043	1052	rBV	338260	606750	25.14%	5.410%
6	11.072	1318	1325	1333	rBV	166652	302041	12.51%	2.693%
7	13.493	1730	1737	1745	rVB	1023159	1571076	65.09%	14.008%
8	14.868	1964	1971	1980	rBV	299412	463545	19.21%	4.133%
9	16.213	2194	2200	2205	rBV	36180	53547	2.22%	0.477%
10	16.355	2217	2224	2232	rBV	872756	1395142	57.80%	12.440%
11	17.612	2430	2438	2445	rBV	395813	604736	25.05%	5.392%
12	19.727	2795	2798	2813	rVB8	29525	82101	3.40%	0.732%
13	20.197	2872	2878	2884	rBV	1860054	2413648	100.00%	21.521%
14	21.907	3163	3169	3181	rVB2	366246	632916	26.22%	5.643%
15	25.320	3742	3750	3774	rVB2	233934	825692	34.21%	7.362%




Sum of corrected areas: 11215281

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112122\
Data File : BG055713.D
Acq On : 21 Nov 2022 13:22
Operator : CG/JU
Sample : N5678-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
250FB-BP-BACKFILL-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

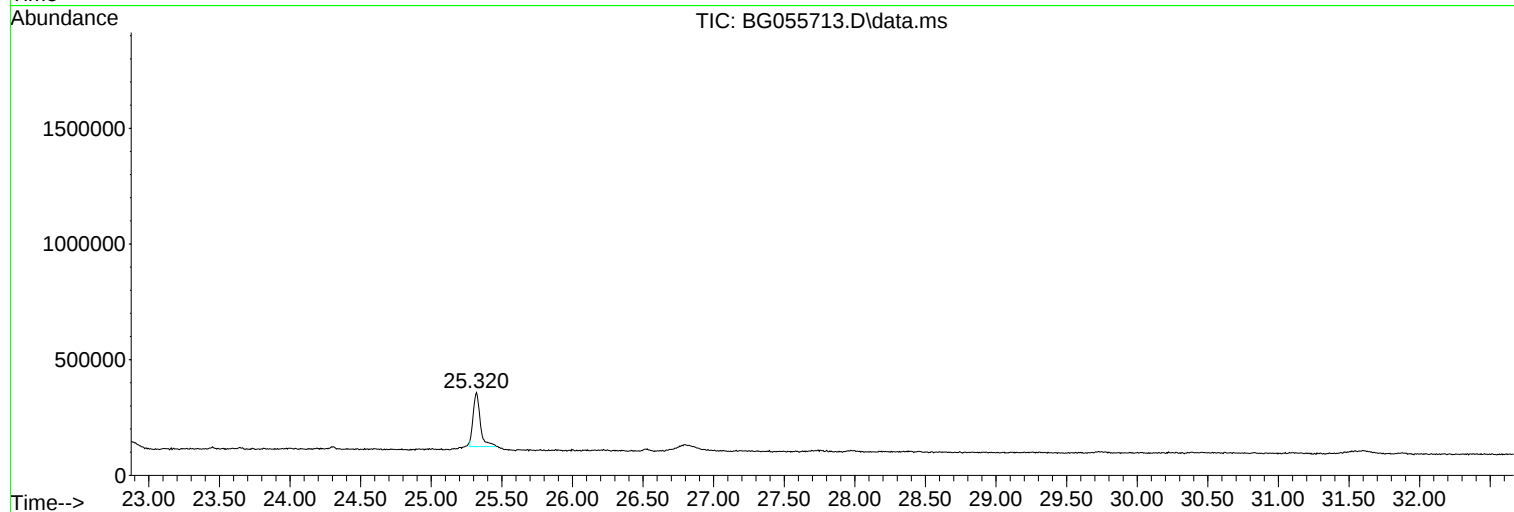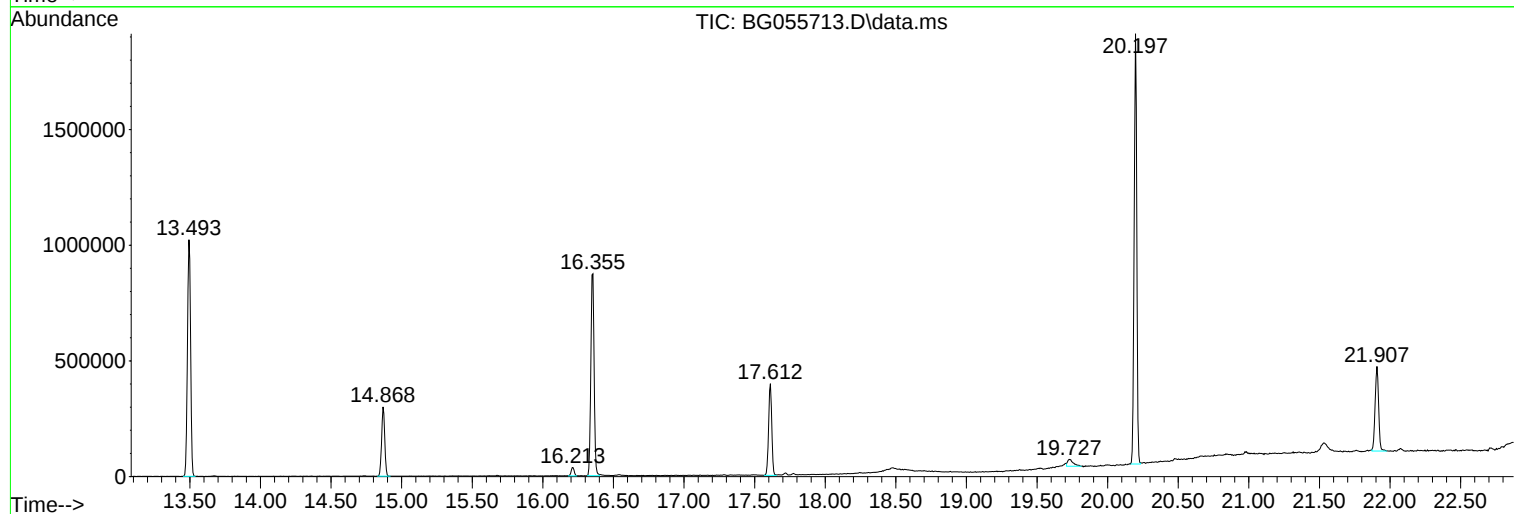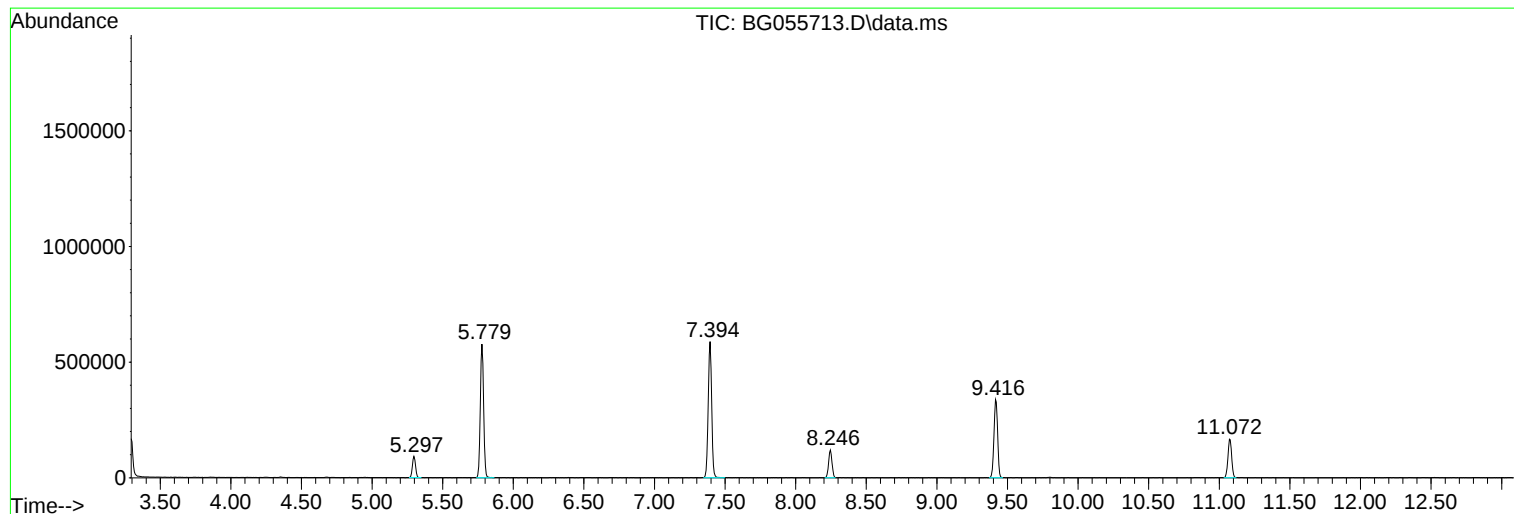

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112122\
Data File : BG055713.D
Acq On : 21 Nov 2022 13:22
Operator : CG/JU
Sample : N5678-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
250FB-BP-BACKFILL-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112122\
Data File : BG055713.D
Acq On : 21 Nov 2022 13:22
Operator : CG/JU
Sample : N5678-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
250FB-BP-BACKFILL-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------