

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112122\
 Data File : BG055724.D
 Acq On : 21 Nov 2022 21:08
 Operator : CG/JU
 Sample : N5678-15
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 250FB-BP-BACKFILL-08

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG055724.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.295	335	341	352	rBV	70000	105996	5.22%	1.043%
2	5.777	416	423	436	rVB	438118	697996	34.36%	6.872%
3	7.387	689	697	714	rBV	450518	791862	38.98%	7.796%
4	8.244	836	843	849	rBV	120961	197193	9.71%	1.941%
5	9.414	1035	1042	1051	rBV	265839	476867	23.48%	4.695%
6	11.071	1316	1324	1337	rVB	177302	327638	16.13%	3.225%
7	13.491	1728	1736	1745	rBV	824271	1282699	63.15%	12.628%
8	14.866	1964	1970	1978	rVB	347343	527047	25.95%	5.189%
9	16.212	2193	2199	2205	rVB	25836	37537	1.85%	0.370%
10	16.347	2216	2222	2232	rBV	637878	1010688	49.76%	9.950%
11	16.535	2246	2254	2258	rBV2	14599	21713	1.07%	0.214%
12	16.670	2272	2277	2282	rBV	28349	44644	2.20%	0.440%
13	16.729	2282	2287	2294	rVV2	37740	76489	3.77%	0.753%
14	16.793	2294	2298	2302	rVV	36999	56730	2.79%	0.558%
15	16.834	2302	2305	2310	rVB	19497	25706	1.27%	0.253%
16	16.993	2326	2332	2339	rVB4	32512	63943	3.15%	0.629%
17	17.058	2339	2343	2347	rBV	35298	52540	2.59%	0.517%
18	17.128	2352	2355	2365	rVB3	22856	40838	2.01%	0.402%
19	17.610	2428	2437	2445	rBV	452807	662040	32.59%	6.518%
20	18.468	2578	2583	2593	rBV2	23615	44412	2.19%	0.437%
21	20.195	2871	2877	2883	rBV	1613310	2031229	100.00%	19.997%
22	21.529	3098	3104	3115	rBV6	35116	126243	6.22%	1.243%
23	21.905	3162	3168	3175	rVB	424197	697872	34.36%	6.870%
24	25.319	3739	3749	3760	rVB	250113	757860	37.31%	7.461%




Sum of corrected areas: 10157782

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112122\
Data File : BG055724.D
Acq On : 21 Nov 2022 21:08
Operator : CG/JU
Sample : N5678-15
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
250FB-BP-BACKFILL-08

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

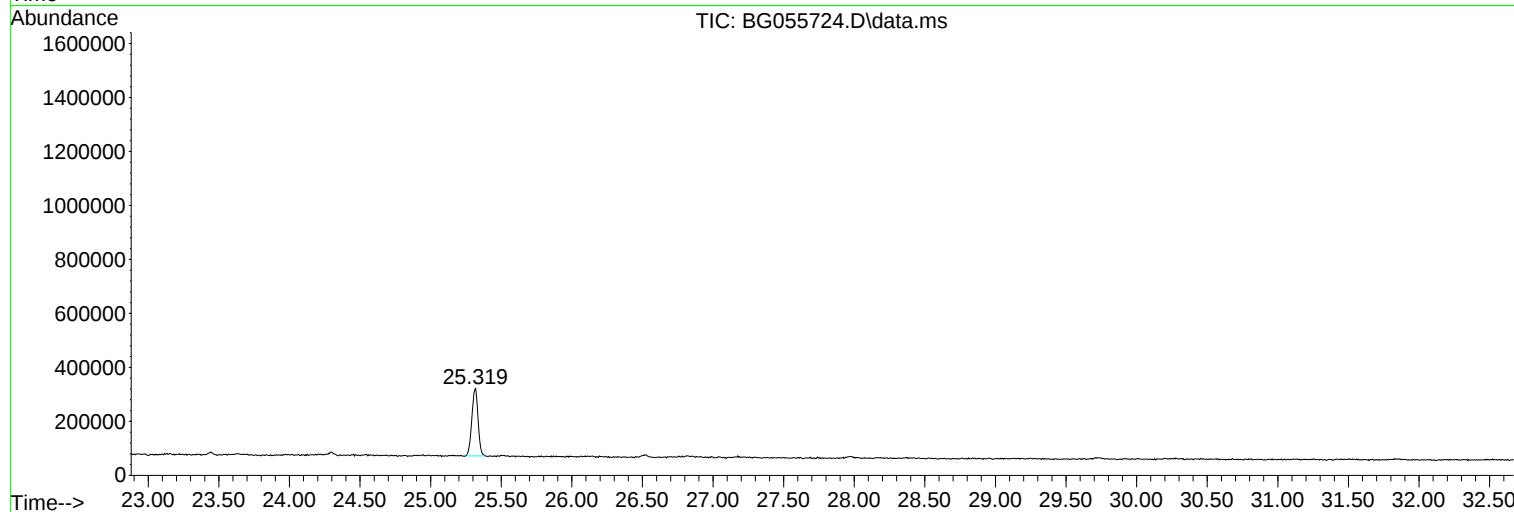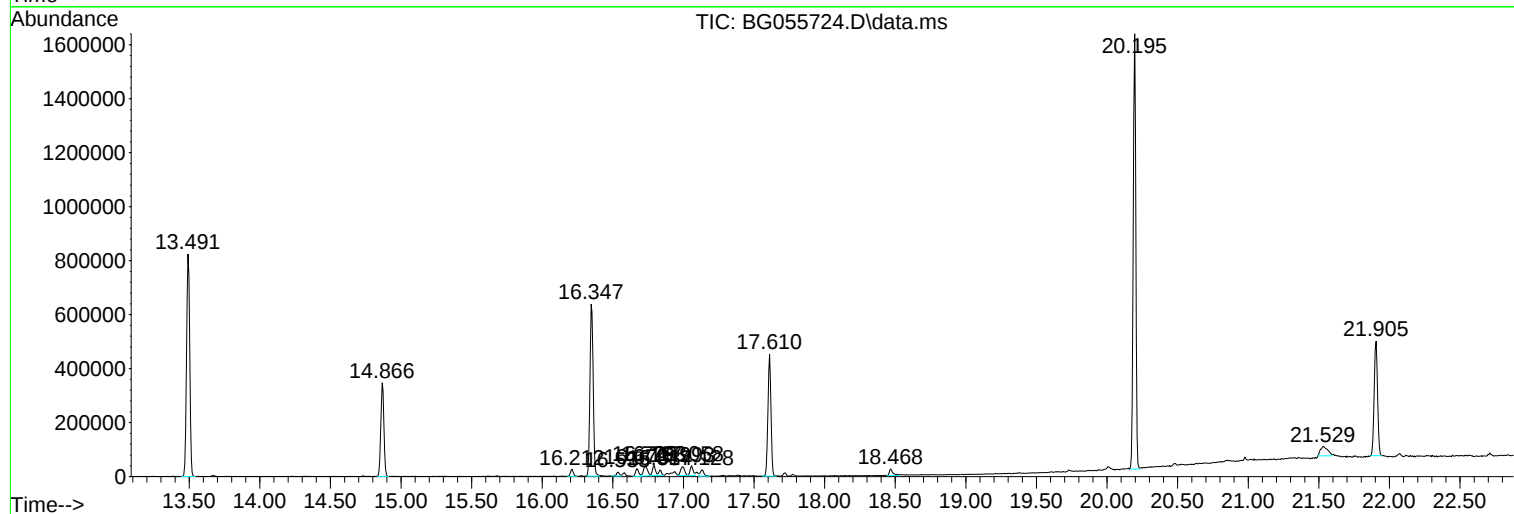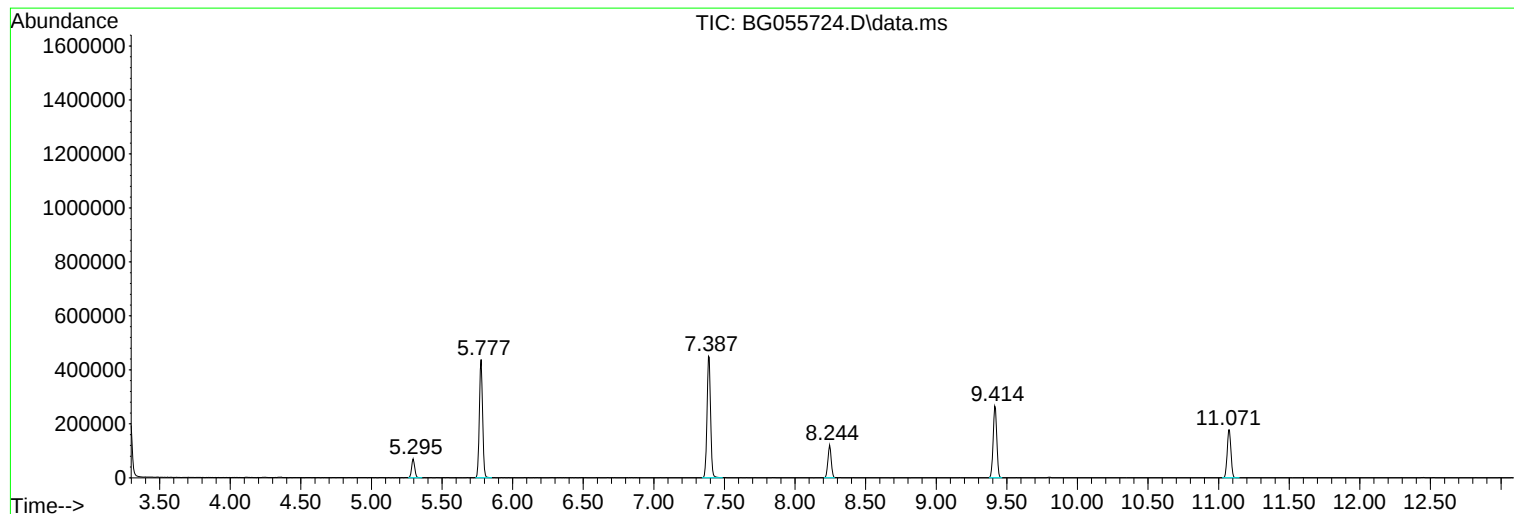

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112122\
Data File : BG055724.D
Acq On : 21 Nov 2022 21:08
Operator : CG/JU
Sample : N5678-15
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
250FB-BP-BACKFILL-08

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112122\
Data File : BG055724.D
Acq On : 21 Nov 2022 21:08
Operator : CG/JU
Sample : N5678-15
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
250FB-BP-BACKFILL-08

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------