

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112122\
 Data File : BG055726.D
 Acq On : 21 Nov 2022 22:30
 Operator : CG/JU
 Sample : N5678-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 250FB-BP-BACKFILL-04

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG055726.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.298	335	342	350	rBV	88303	138237	4.90%	1.072%
2	5.774	416	423	433	rBV	602949	976724	34.65%	7.573%
3	7.389	690	698	715	rBV	656978	1115811	39.58%	8.651%
4	8.241	836	843	850	rBV	119154	202299	7.18%	1.569%
5	9.416	1035	1043	1052	rVB	388677	691624	24.53%	5.363%
6	11.073	1317	1325	1337	rVB	187852	339785	12.05%	2.635%
7	13.494	1729	1737	1744	rBV	1216106	1903022	67.51%	14.755%
8	14.869	1963	1971	1978	rBV	352712	547730	19.43%	4.247%
9	16.208	2192	2199	2206	rVB	33078	46651	1.65%	0.362%
10	16.349	2216	2223	2234	rBV	990518	1535593	54.47%	11.906%
11	16.537	2246	2255	2261	rVB2	23460	40565	1.44%	0.315%
12	17.607	2431	2437	2444	rBV	467817	677781	24.04%	5.255%
13	18.465	2578	2583	2593	rBV	100261	174563	6.19%	1.353%
14	19.728	2794	2798	2805	rBV3	36014	60406	2.14%	0.468%
15	20.198	2872	2878	2884	rBV	2035619	2818961	100.00%	21.857%
16	21.537	3098	3106	3119	rBV7	41685	175810	6.24%	1.363%
17	21.902	3162	3168	3177	rVB2	413025	695911	24.69%	5.396%
18	25.309	3739	3748	3762	rVB2	257171	755857	26.81%	5.861%




Sum of corrected areas: 12897330

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112122\
Data File : BG055726.D
Acq On : 21 Nov 2022 22:30
Operator : CG/JU
Sample : N5678-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
250FB-BP-BACKFILL-04

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

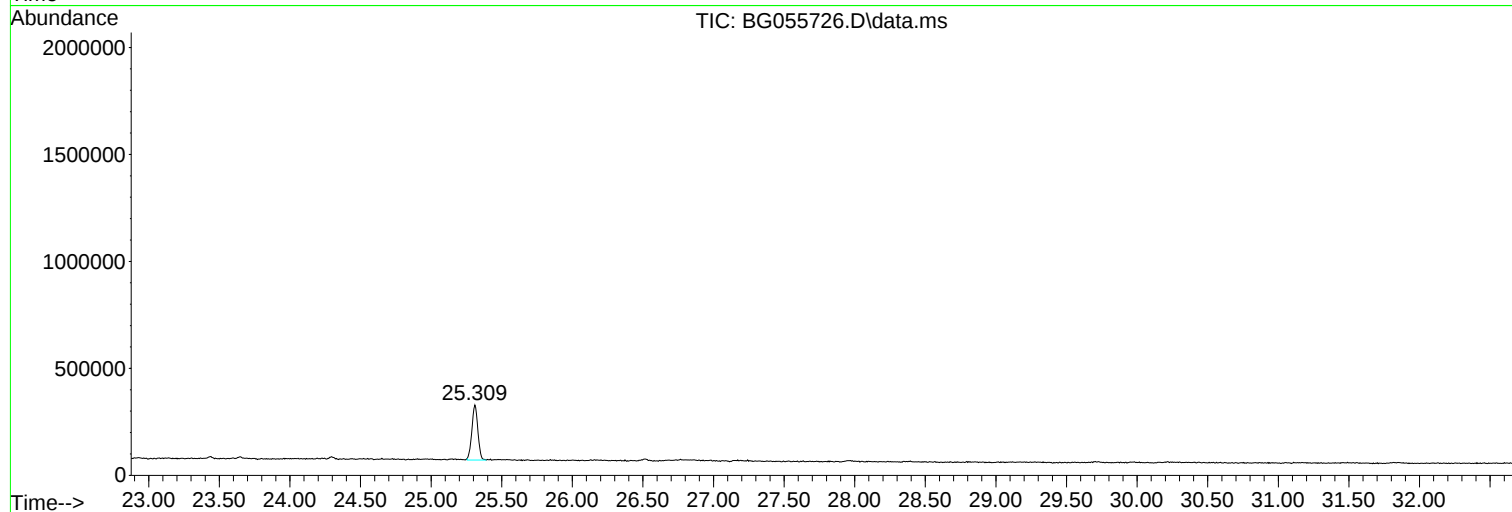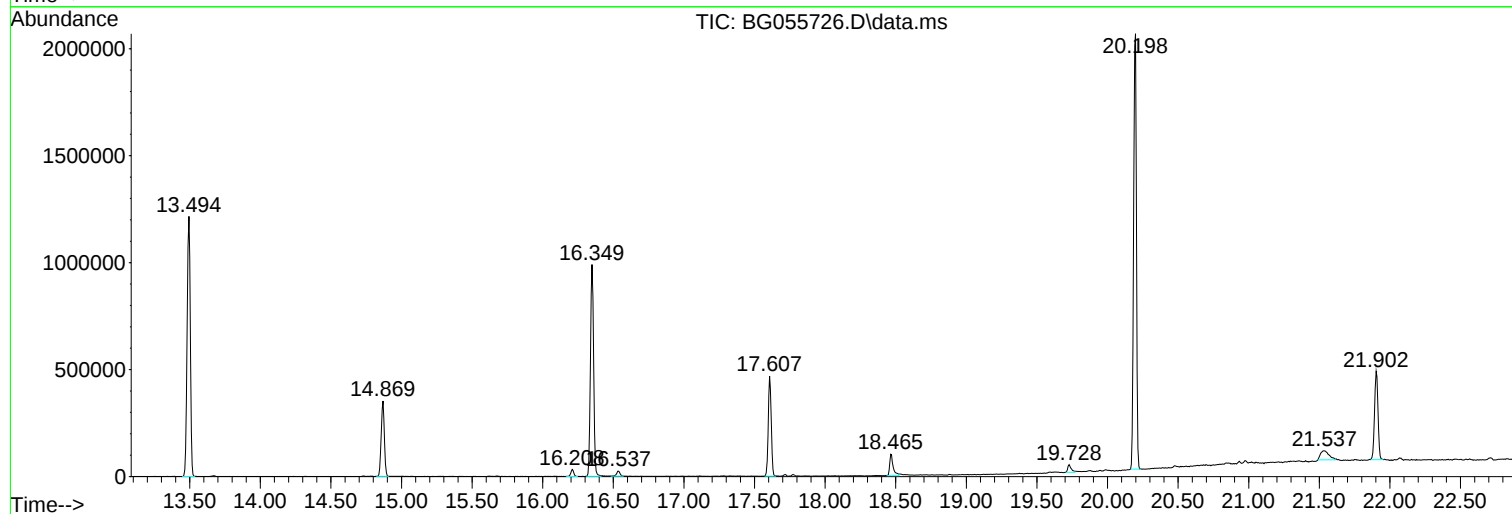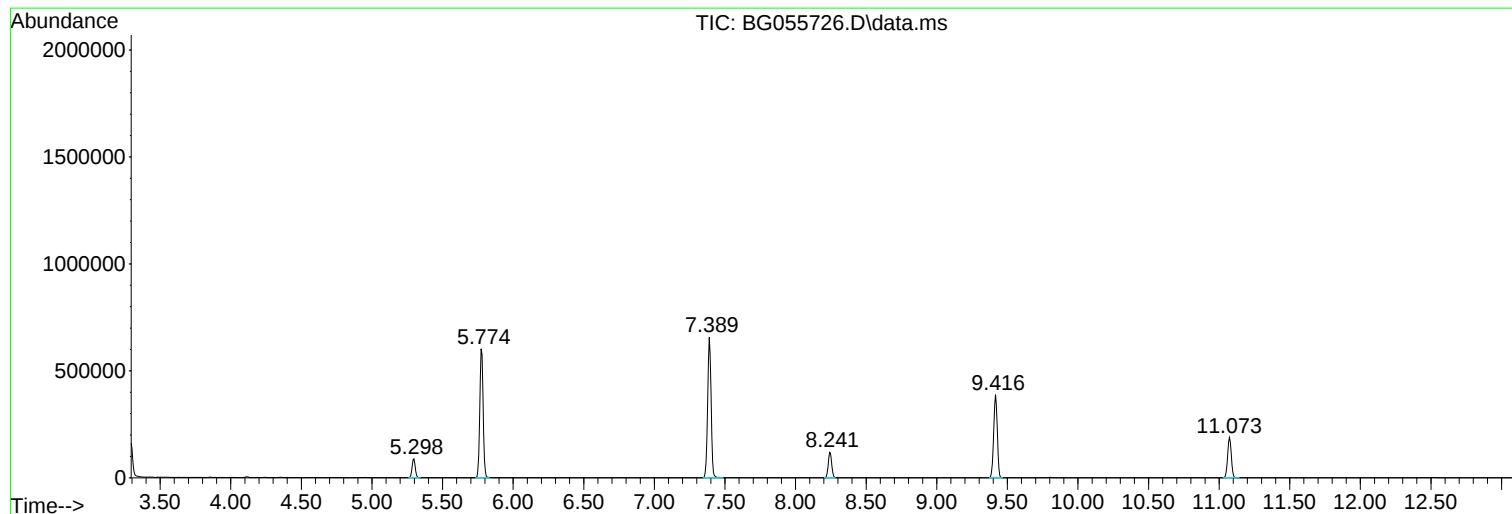

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112122\
Data File : BG055726.D
Acq On : 21 Nov 2022 22:30
Operator : CG/JU
Sample : N5678-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
250FB-BP-BACKFILL-04

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112122\
Data File : BG055726.D
Acq On : 21 Nov 2022 22:30
Operator : CG/JU
Sample : N5678-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
250FB-BP-BACKFILL-04

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------