

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112122\
 Data File : BG055727.D
 Acq On : 21 Nov 2022 23:11
 Operator : CG/JU
 Sample : N5678-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 250FB-BP-BACKFILL-05

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG055727.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.298	336	342	353	rVB	61353	96585	4.79%	0.988%
2	5.774	416	423	436	rBV	415035	664722	32.96%	6.802%
3	7.389	690	698	710	rBV	445888	768138	38.09%	7.860%
4	8.241	836	843	850	rBV	121754	205954	10.21%	2.107%
5	9.417	1035	1043	1055	rVB	275712	485891	24.09%	4.972%
6	11.073	1317	1325	1336	rBV	193444	341829	16.95%	3.498%
7	13.494	1730	1737	1747	rVB	840368	1324129	65.66%	13.549%
8	14.869	1964	1971	1978	rVB	336498	540098	26.78%	5.527%
9	16.209	2194	2199	2206	rVB2	15220	21506	1.07%	0.220%
10	16.350	2216	2223	2232	rBV	693438	1047032	51.92%	10.714%
11	17.607	2430	2437	2446	rBV	452072	661695	32.81%	6.771%
12	17.713	2451	2455	2460	rBV2	17127	21924	1.09%	0.224%
13	18.465	2579	2583	2593	rBV2	60721	105078	5.21%	1.075%
14	19.728	2795	2798	2804	rBV7	17323	31835	1.58%	0.326%
15	20.192	2871	2877	2883	rBV	1548595	2016616	100.00%	20.635%
16	21.902	3162	3168	3175	rVB2	411890	696665	34.55%	7.129%
17	25.310	3738	3748	3760	rVB2	243198	743011	36.84%	7.603%




Sum of corrected areas: 9772708

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112122\
Data File : BG055727.D
Acq On : 21 Nov 2022 23:11
Operator : CG/JU
Sample : N5678-09
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
250FB-BP-BACKFILL-05

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

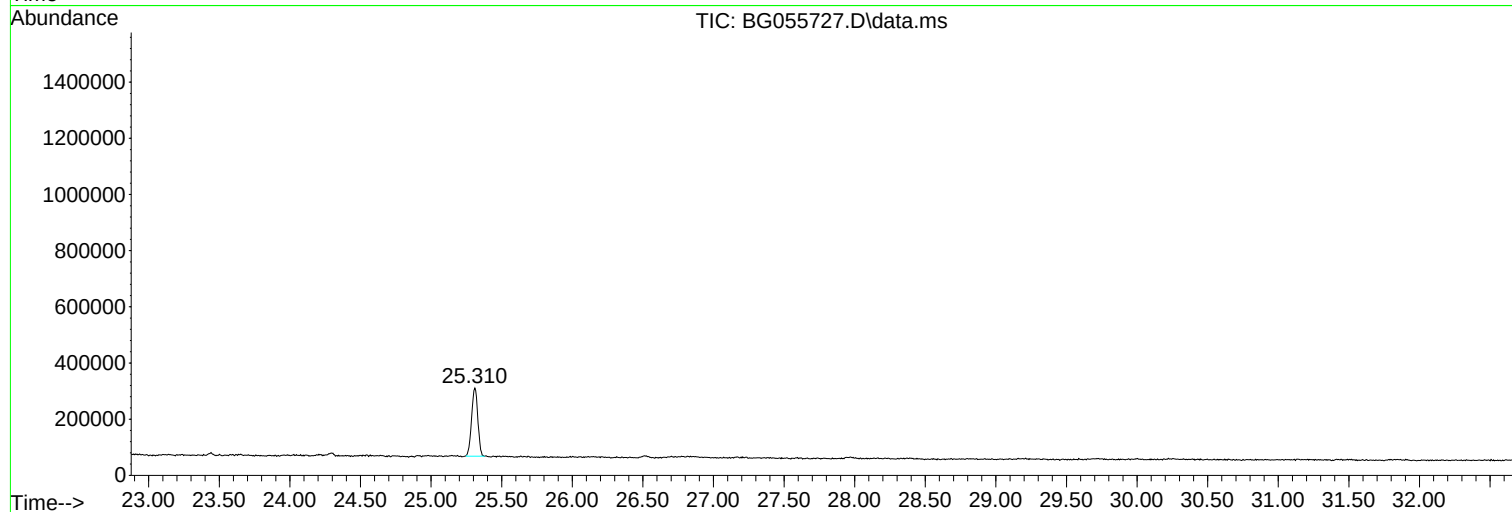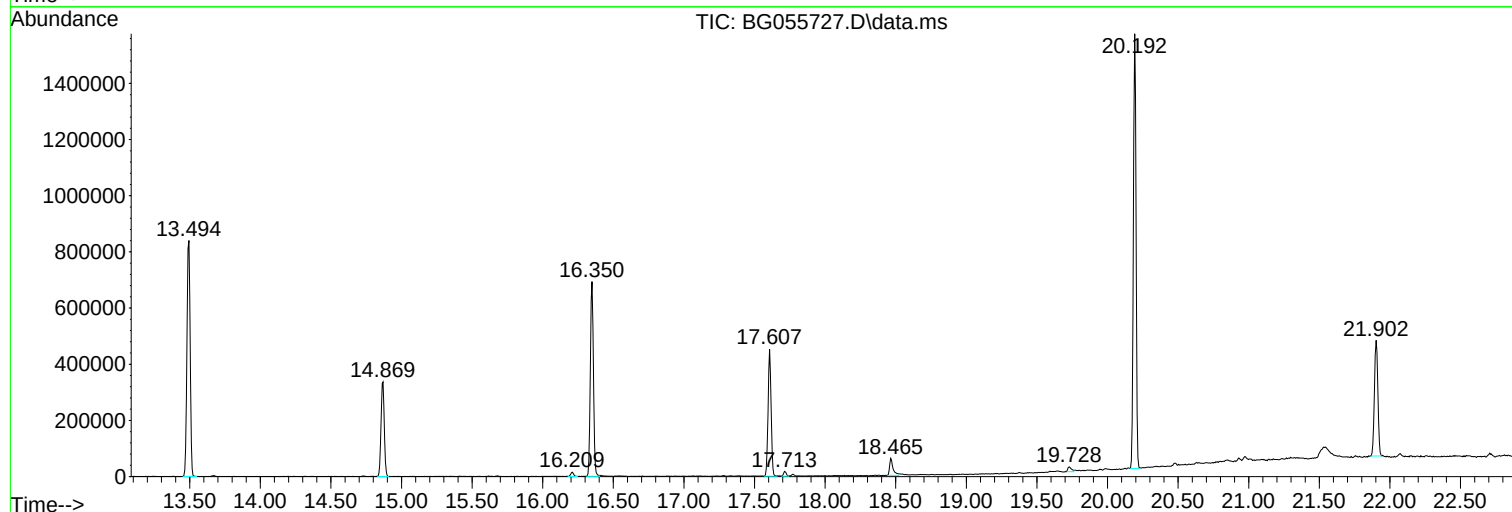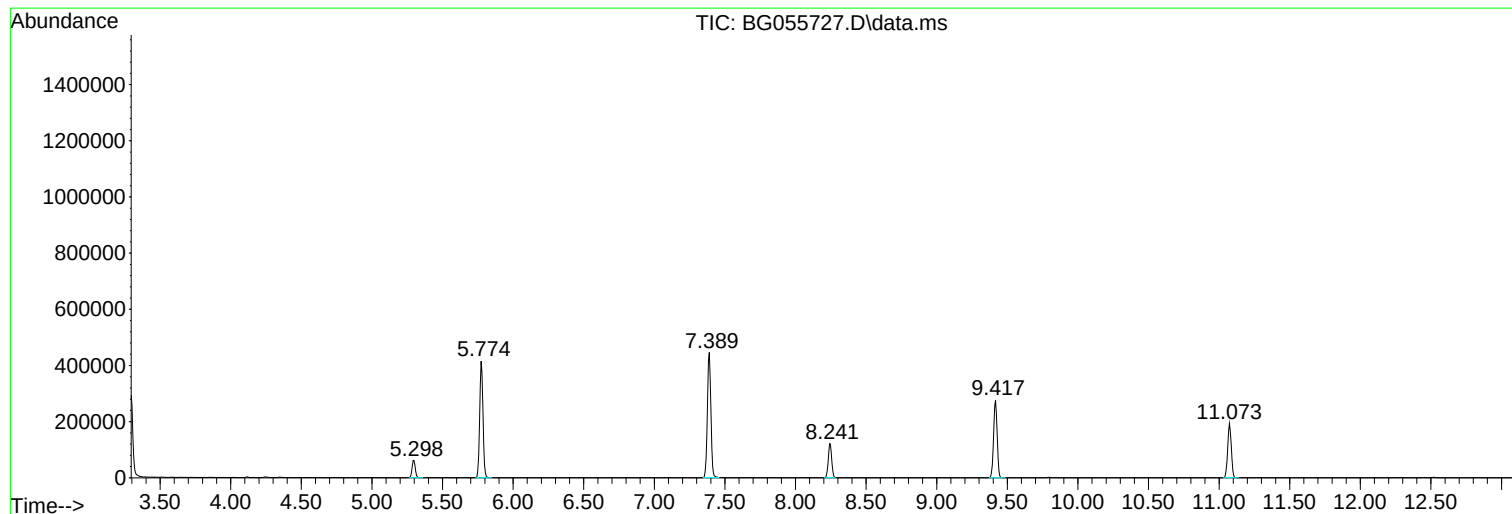

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112122\
Data File : BG055727.D
Acq On : 21 Nov 2022 23:11
Operator : CG/JU
Sample : N5678-09
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
250FB-BP-BACKFILL-05

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112122\
Data File : BG055727.D
Acq On : 21 Nov 2022 23:11
Operator : CG/JU
Sample : N5678-09
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
250FB-BP-BACKFILL-05

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------