


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112122\
Data File : BG055708.D
Acq On : 21 Nov 2022 9:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Nov 17 02:02:46 2022

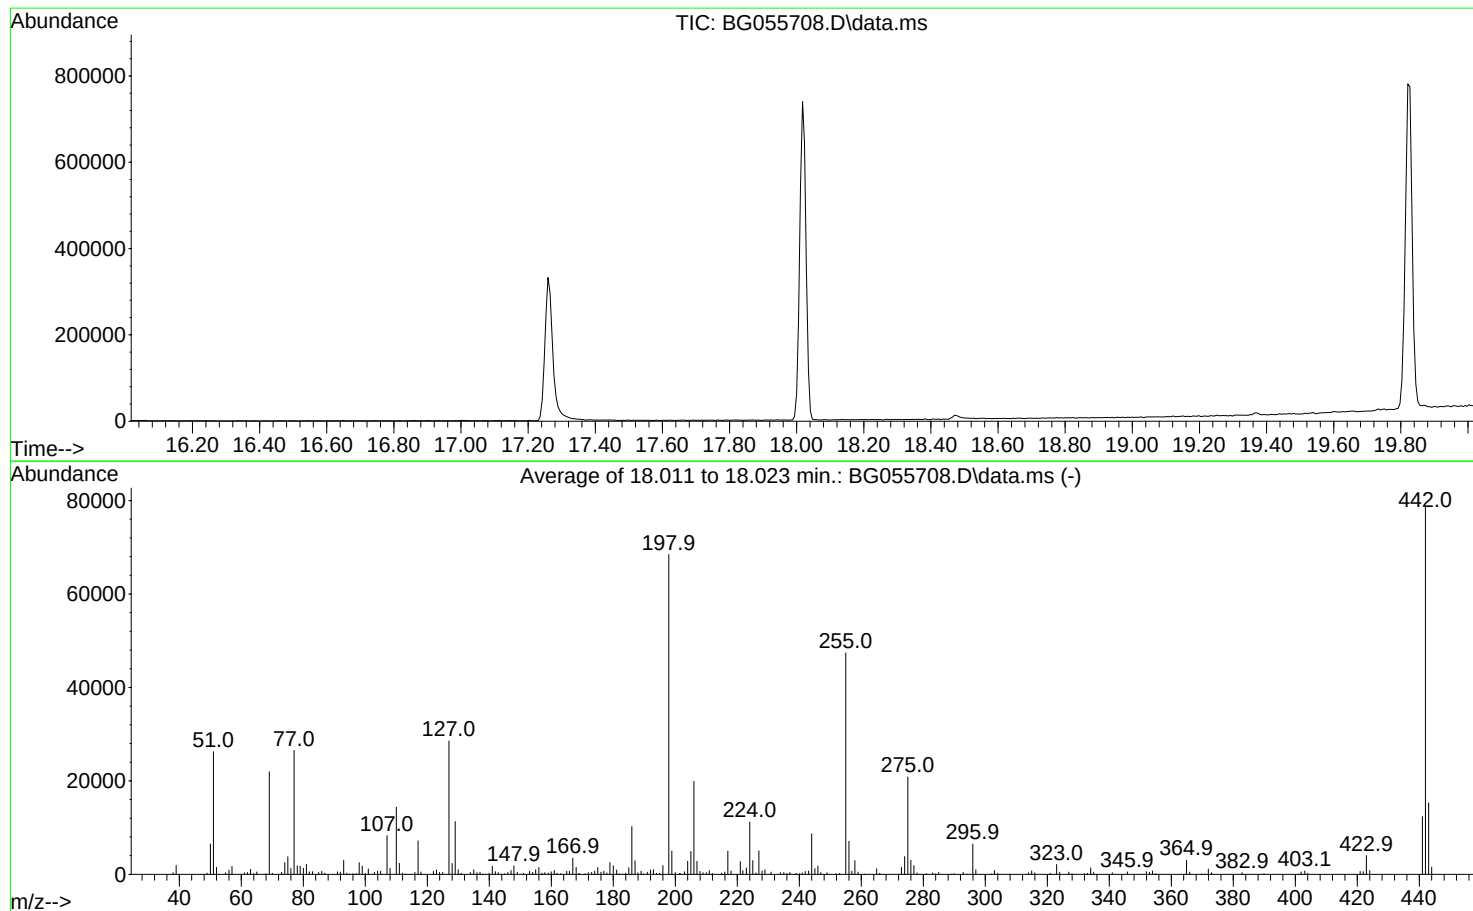




AutoFind: Scans 2506, 2507, 2508; Background Corrected with Scan 2500

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.4	26261	PASS
68	69	0.00	2	0.6	139	PASS
69	198	0.00	100	32.0	21928	PASS
70	69	0.00	2	0.9	208	PASS
127	198	10	80	41.7	28539	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	68432	PASS
199	198	5	9	7.3	4968	PASS
275	198	10	60	30.4	20802	PASS
365	198	1	100	4.4	2987	PASS
441	198	0.01	100	18.1	12353	PASS
442	442	50	100	100.0	78741	PASS
443	442	15	24	19.4	15306	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112122\
Data File : BG055708.D
Acq On : 21 Nov 2022 9:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 22 06:13:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 17 02:02:46 2022
Response via : Initial Calibration

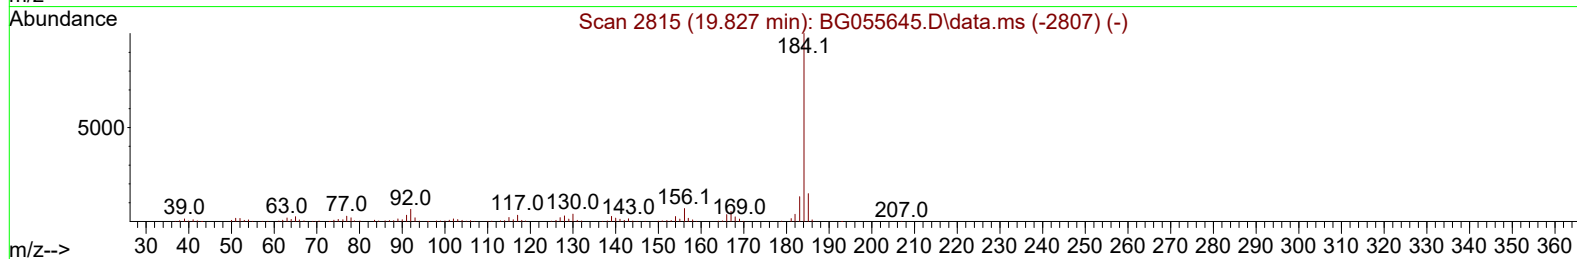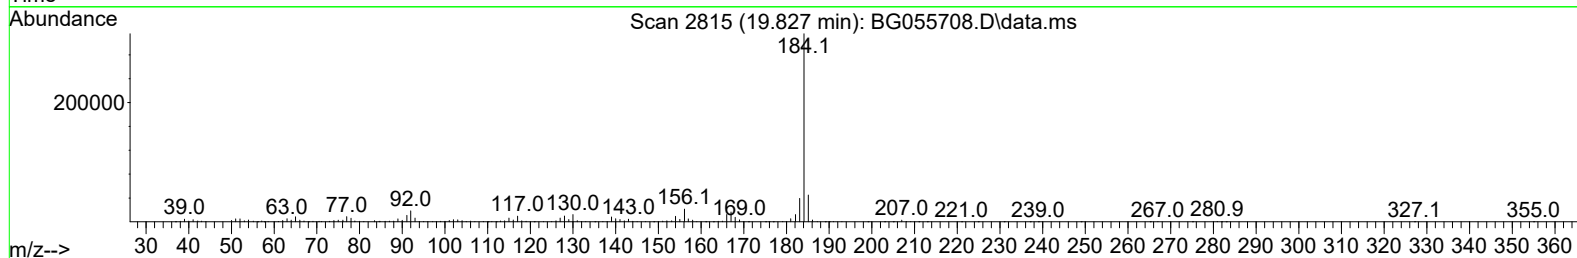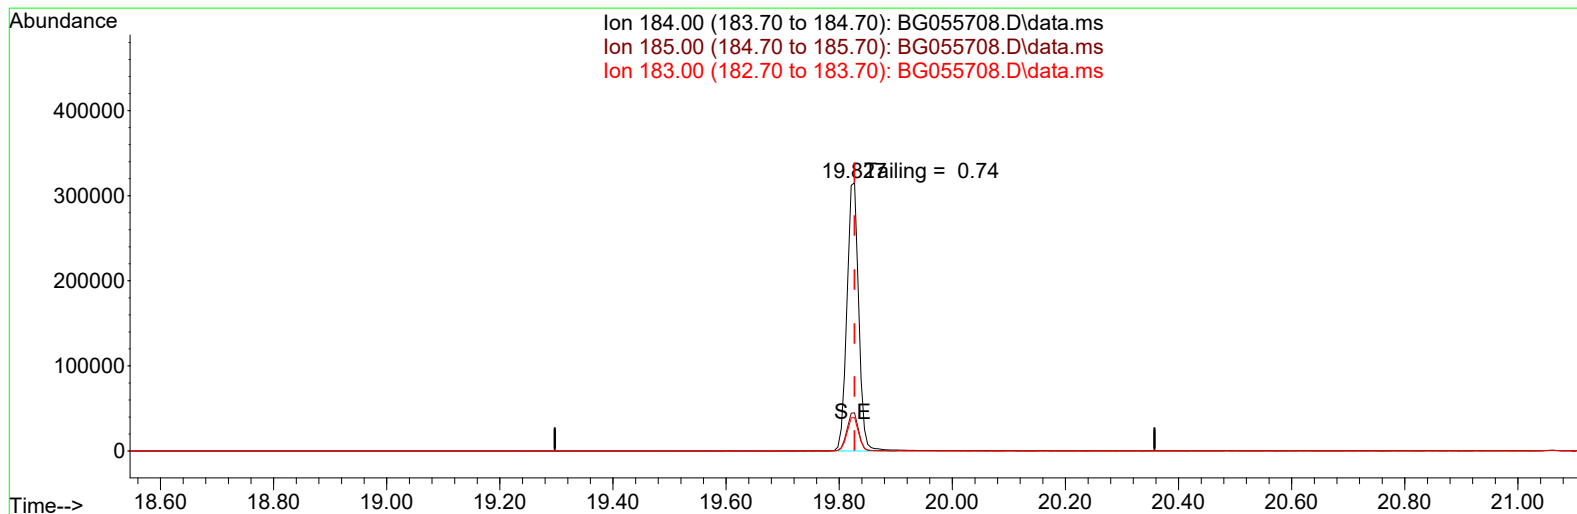

TIC: BG055708.D\data.ms

(77) Benzidine

19.827min (-0.000) 148227.09 ng

response 459507

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.27
183.00	13.20	12.49
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/21/2022	BNA_G	BG055708.D
Compound Name	Response	Retention Time
DDT	210251	21.061
DDD	5792	20.608
DDE	372	20.103
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6164	216415	2.85

Instrument :
BNA_G
ClientSampleId :
DFTPP