


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112122\
 Data File : BG055716.D
 Acq On : 21 Nov 2022 15:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Nov 17 02:02:46 2022

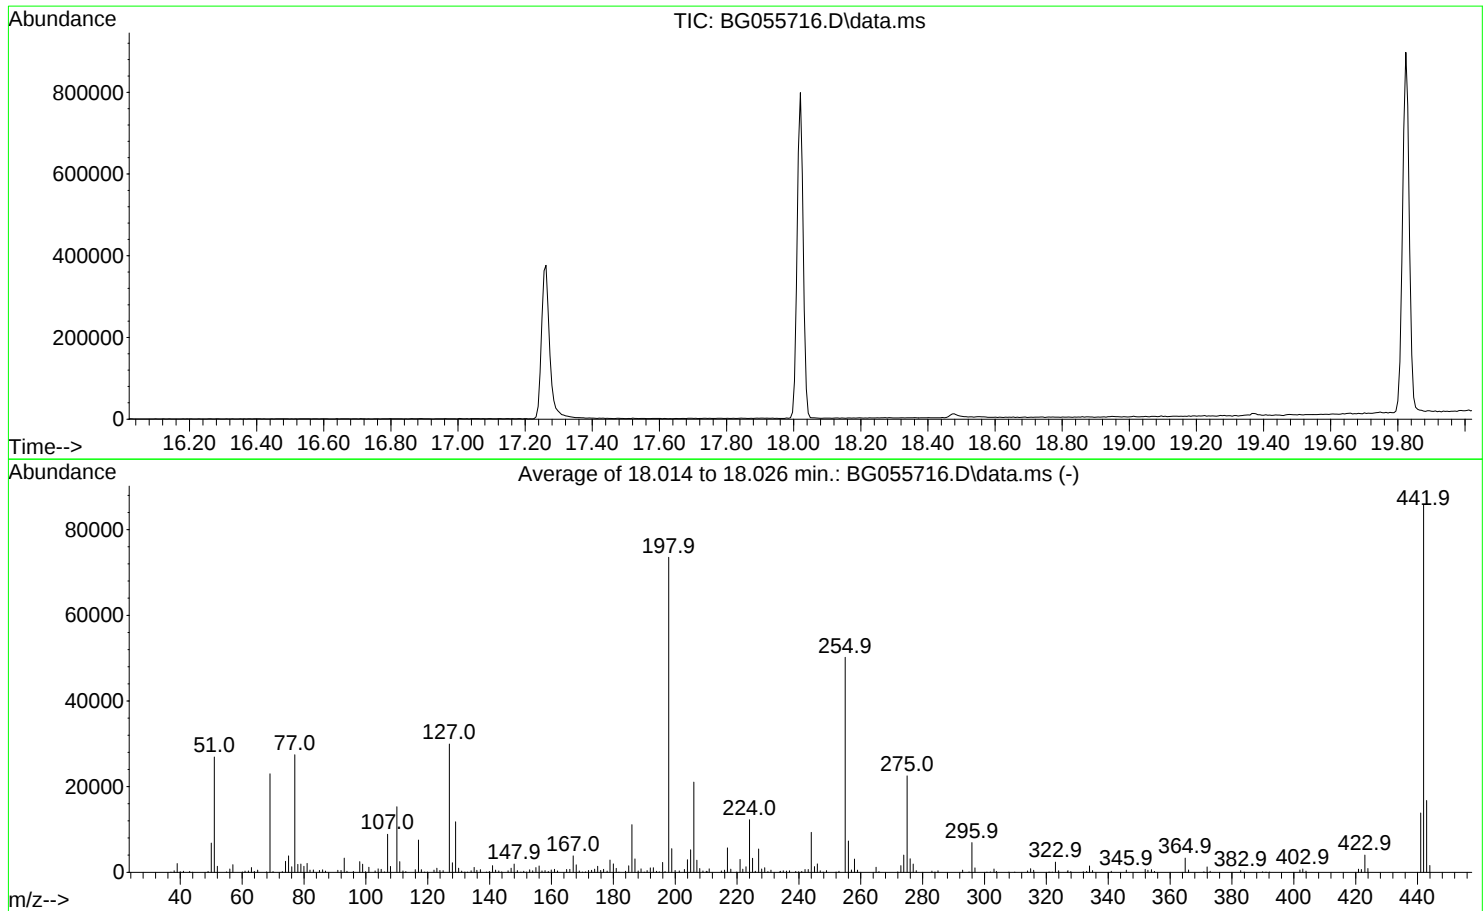




AutoFind: Scans 2506, 2507, 2508; Background Corrected with Scan 2499

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.6	26933	PASS
68	69	0.00	2	0.4	101	PASS
69	198	0.00	100	31.3	23011	PASS
70	69	0.00	2	0.7	159	PASS
127	198	10	80	40.7	29955	PASS
197	198	0.00	2	0.2	159	PASS
198	198	100	100	100.0	73533	PASS
199	198	5	9	7.5	5512	PASS
275	198	10	60	30.6	22525	PASS
365	198	1	100	4.5	3300	PASS
441	198	0.01	100	18.8	13835	PASS
442	442	50	100	100.0	85893	PASS
443	442	15	24	19.5	16754	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112122\
 Data File : BG055716.D
 Acq On : 21 Nov 2022 15:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Nov 22 06:15:17 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 17 02:02:46 2022
 Response via : Initial Calibration

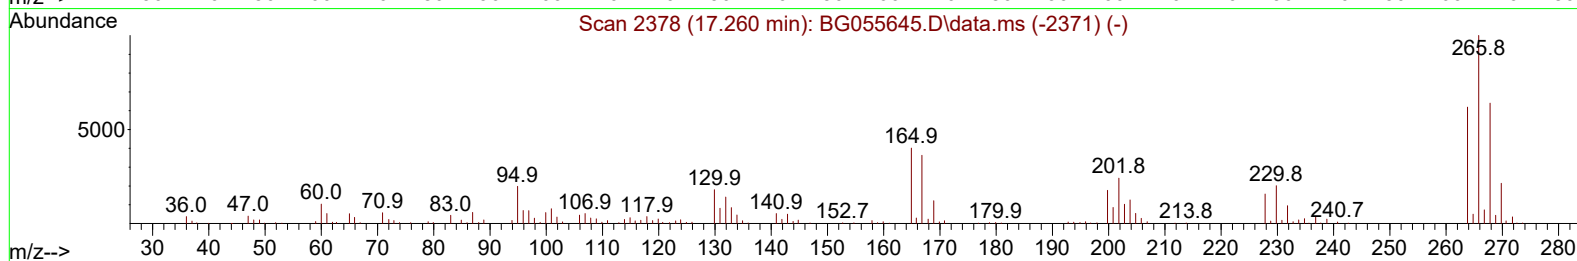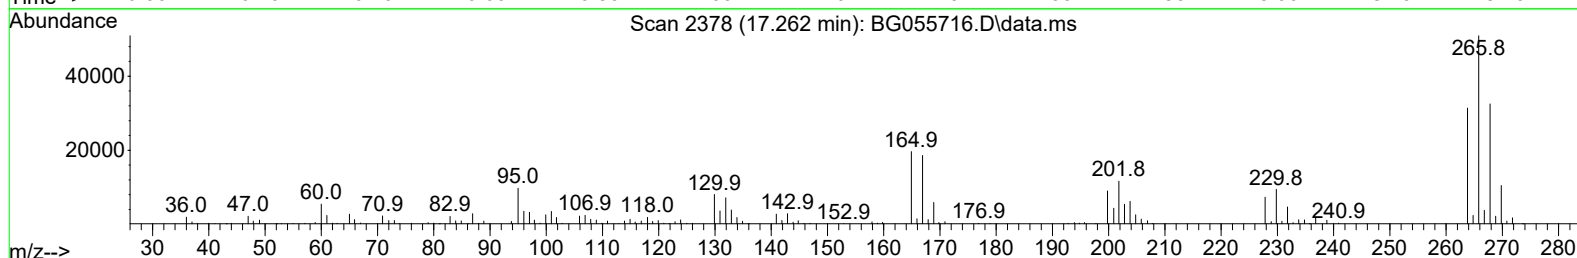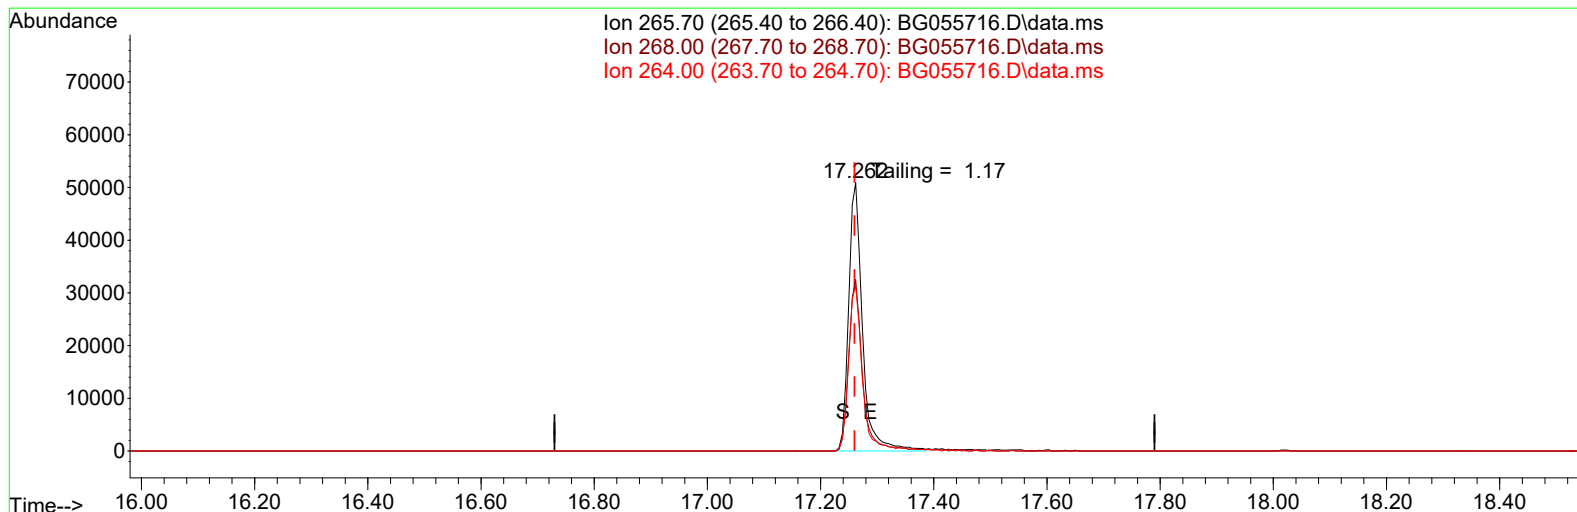

TIC: BG055716.D\data.ms

(70) Pentachlorophenol (C)

17.262min (+ 0.002) 26042.22 ng




response 86948

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	63.89
264.00	61.90	61.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112122\
Data File : BG055716.D
Acq On : 21 Nov 2022 15:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 22 06:15:17 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 17 02:02:46 2022
Response via : Initial Calibration

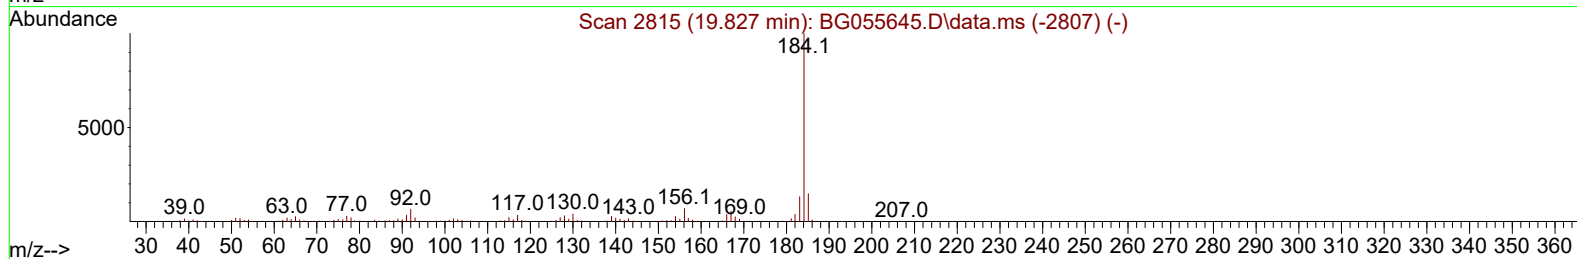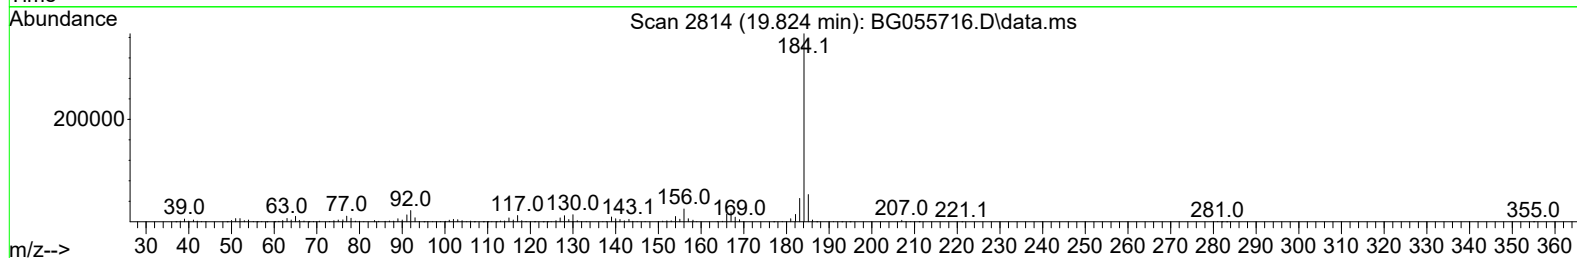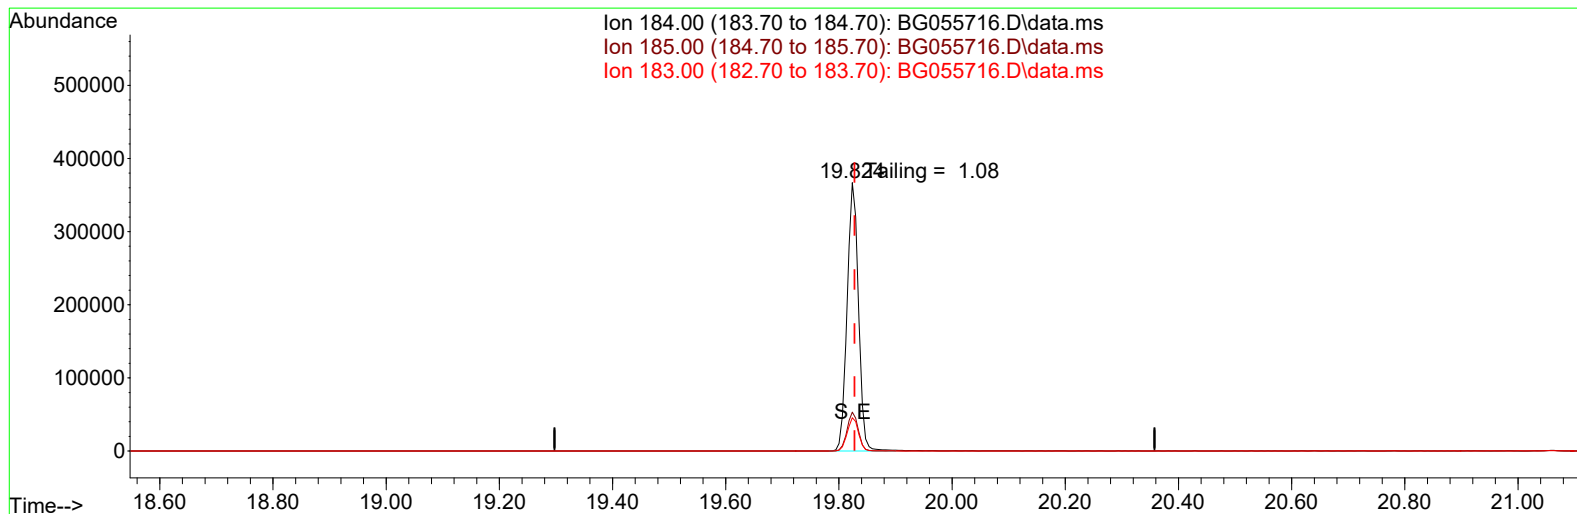

TIC: BG055716.D\data.ms

(77) Benzidine

19.824min (-0.004) 390456.14 ng

response 514881

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.51
183.00	13.20	12.43
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/21/2022	BNA_G	<u>BG055716.D</u>
Compound Name	Response	Retention Time
DDT	244365	21.058
DDD	5169	20.658
DDE	276	20.106
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5445	249810	2.18

Instrument :
BNA_G
ClientSampleId :
DFTPP