

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112124\
 Data File : BG063504.D
 Acq On : 21 Nov 2024 11:06
 Operator : RC/JU
 Sample : PB165140BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK140

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063504.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.298	33	36	43	rVB2	27845	47575	1.54%	0.160%
2	3.704	100	105	113	rBV	295937	514527	16.64%	1.727%
3	4.115	173	175	177	rBV	4544	4575	0.15%	0.015%
4	5.843	467	469	472	rVB3	5578	4798	0.16%	0.016%
5	6.383	556	561	566	rBV3	4094	7978	0.26%	0.027%
6	6.448	569	572	575	rBV3	4705	5301	0.17%	0.018%
7	6.859	641	642	645	rVB3	5639	4665	0.15%	0.016%
8	6.894	645	648	649	rBV	3496	4331	0.14%	0.015%
9	7.006	661	667	676	rBV	379921	637886	20.62%	2.141%
10	7.165	688	694	702	rVB	280272	464807	15.03%	1.560%
11	7.364	722	728	738	rBV	361410	619991	20.05%	2.081%
12	7.828	800	807	814	rBV	358323	593808	19.20%	1.993%
13	7.881	814	816	821	rVB5	5264	8620	0.28%	0.029%
14	8.240	875	877	883	rVB	3588	5066	0.16%	0.017%
15	8.451	910	913	915	rBV3	4167	4834	0.16%	0.016%
16	8.539	921	928	938	rBV	463348	810060	26.19%	2.719%
17	8.733	959	961	966	rVB4	3483	4737	0.15%	0.016%
18	8.986	997	1004	1012	rBV2	361393	634526	20.52%	2.130%
19	9.709	1120	1127	1136	rBV	314160	577306	18.67%	1.938%
20	10.249	1211	1219	1231	rBV	456910	853827	27.61%	2.866%
21	10.384	1240	1242	1247	rVB4	3664	5939	0.19%	0.020%
22	10.561	1267	1272	1274	rBV4	3761	4309	0.14%	0.014%
23	10.619	1274	1282	1289	rBV	496800	845281	27.33%	2.837%
24	10.760	1298	1306	1317	rBV	424993	835442	27.01%	2.804%
25	11.019	1347	1350	1352	rBV2	5039	5547	0.18%	0.019%
26	11.166	1372	1375	1380	rVB2	3730	4903	0.16%	0.016%
27	11.230	1384	1386	1391	rVB3	4190	5686	0.18%	0.019%
28	11.471	1423	1427	1429	rVB2	3841	4335	0.14%	0.015%
29	11.624	1449	1453	1456	rBV4	4993	6073	0.20%	0.020%
30	12.106	1534	1535	1538	rBV	4341	4456	0.14%	0.015%
31	12.288	1563	1566	1568	rVB	4181	4712	0.15%	0.016%
32	12.922	1671	1674	1676	rBV	3517	4582	0.15%	0.015%
33	13.874	1830	1836	1847	rVB	881589	1344500	43.47%	4.513%
34	14.162	1876	1885	1898	rBV	1030924	1576236	50.96%	5.291%
35	14.350	1914	1917	1920	rVB3	4331	6382	0.21%	0.021%
36	14.474	1931	1938	1946	rBV	831017	1294771	41.86%	4.346%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112124\
 Data File : BG063504.D
 Acq On : 21 Nov 2024 11:06
 Operator : RC/JU
 Sample : PB165140BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK140

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
 Title : SVOA CALIBRATION

37	14.691	1969	1975	1986	rBV2	230708	476391	15.40%	1.599%
38	15.026	2031	2032	2037	rVB4	4513	5896	0.19%	0.020%
39	15.467	2101	2107	2115	rBV	1373114	2024324	65.45%	6.795%
40	15.596	2124	2129	2138	rBV	323014	520737	16.84%	1.748%
41	15.713	2147	2149	2152	rVB3	8733	8984	0.29%	0.030%
42	15.796	2161	2163	2167	rVB3	3645	4786	0.15%	0.016%
43	16.424	2268	2270	2273	rBV	4386	4701	0.15%	0.016%
44	16.900	2350	2351	2357	rVB2	5612	6686	0.22%	0.022%
45	16.965	2360	2362	2366	rVB2	5901	6513	0.21%	0.022%
46	17.000	2366	2368	2369	rBV2	4840	4352	0.14%	0.015%
47	17.223	2399	2406	2413	rBV	1151459	1718701	55.57%	5.769%
48	17.323	2417	2423	2435	rVV	1625444	2387925	77.21%	8.016%
49	17.617	2470	2473	2474	rBV	6085	4885	0.16%	0.016%
50	17.764	2496	2498	2502	rVB3	5084	5202	0.17%	0.017%
51	17.793	2502	2503	2506	rBV2	5405	4891	0.16%	0.016%
52	17.946	2526	2529	2532	rVB2	5358	5689	0.18%	0.019%
53	18.199	2568	2572	2573	rBV2	5084	4567	0.15%	0.015%
54	18.616	2640	2643	2646	rBV4	4714	4490	0.15%	0.015%
55	18.774	2669	2670	2674	rBV4	6832	7883	0.25%	0.026%
56	19.192	2736	2741	2748	rVV3	22548	36659	1.19%	0.123%
57	19.262	2748	2753	2758	rVB2	20635	36946	1.19%	0.124%
58	19.562	2801	2804	2806	rBV4	8494	10524	0.34%	0.035%
59	19.626	2808	2815	2823	rVV	2230010	3081166	99.62%	10.343%
60	19.897	2859	2861	2862	rBV2	5841	4872	0.16%	0.016%
61	21.483	3125	3131	3143	rBV2	1370923	2219393	71.76%	7.450%
62	24.315	3604	3613	3626	rVB2	1242844	3092890	100.00%	10.382%
63	24.527	3639	3649	3662	rVB	856560	2338651	75.61%	7.850%




Sum of corrected areas: 29791076

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112124\
Data File : BG063504.D
Acq On : 21 Nov 2024 11:06
Operator : RC/JU
Sample : PB165140BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK140

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

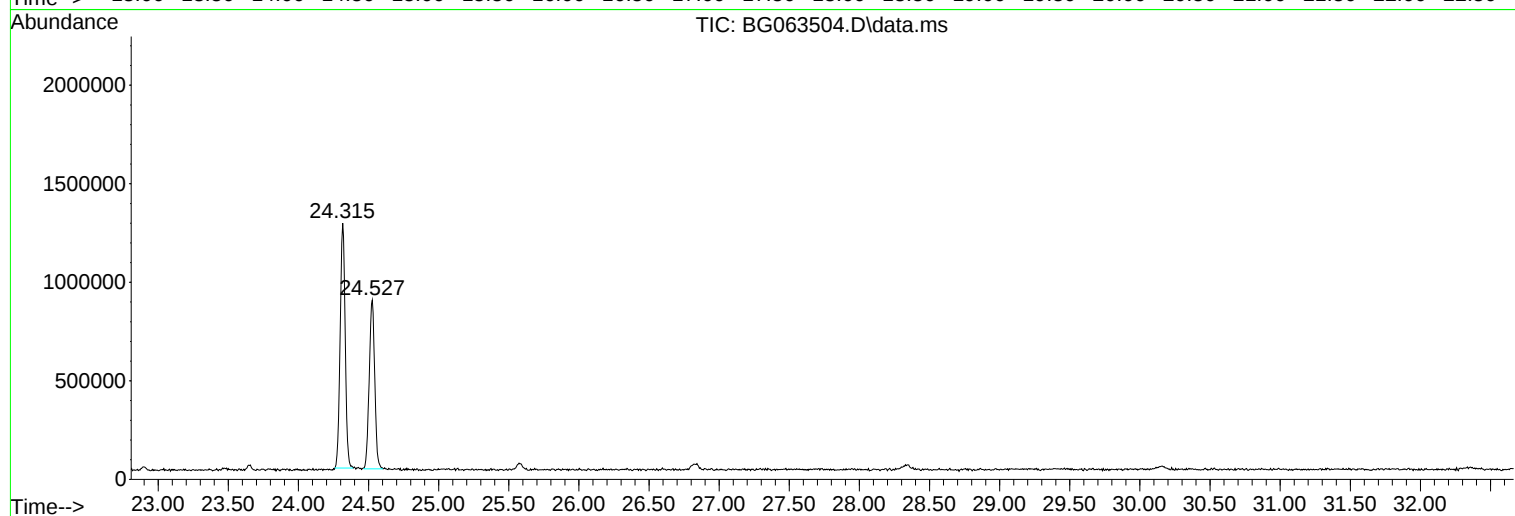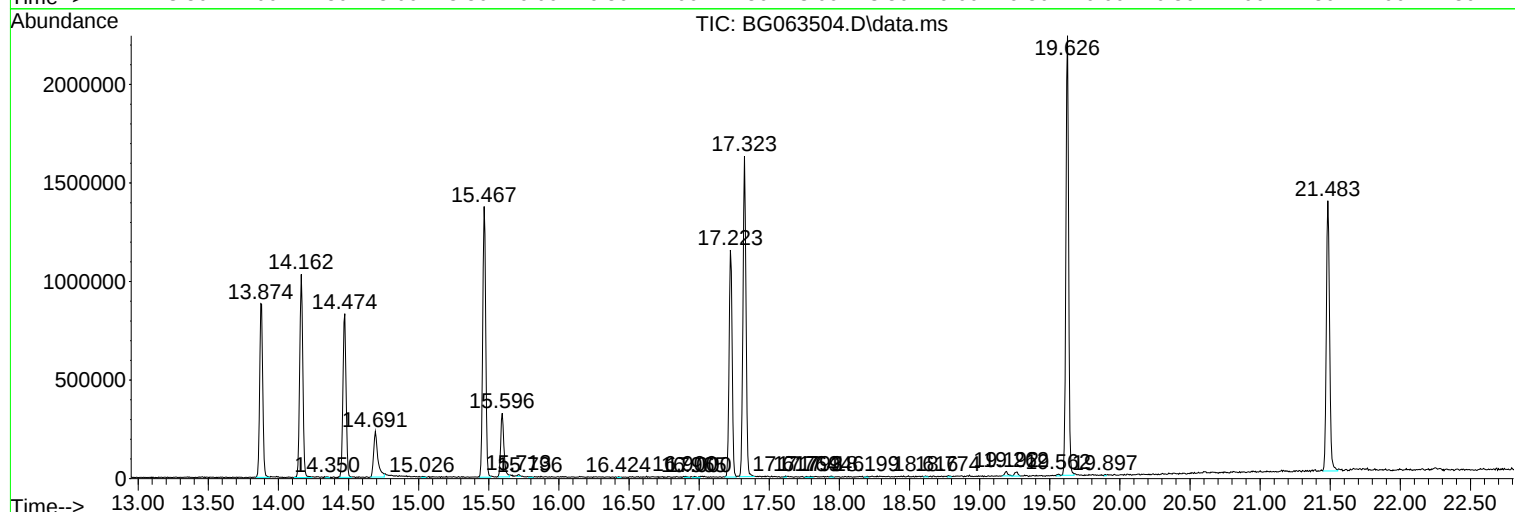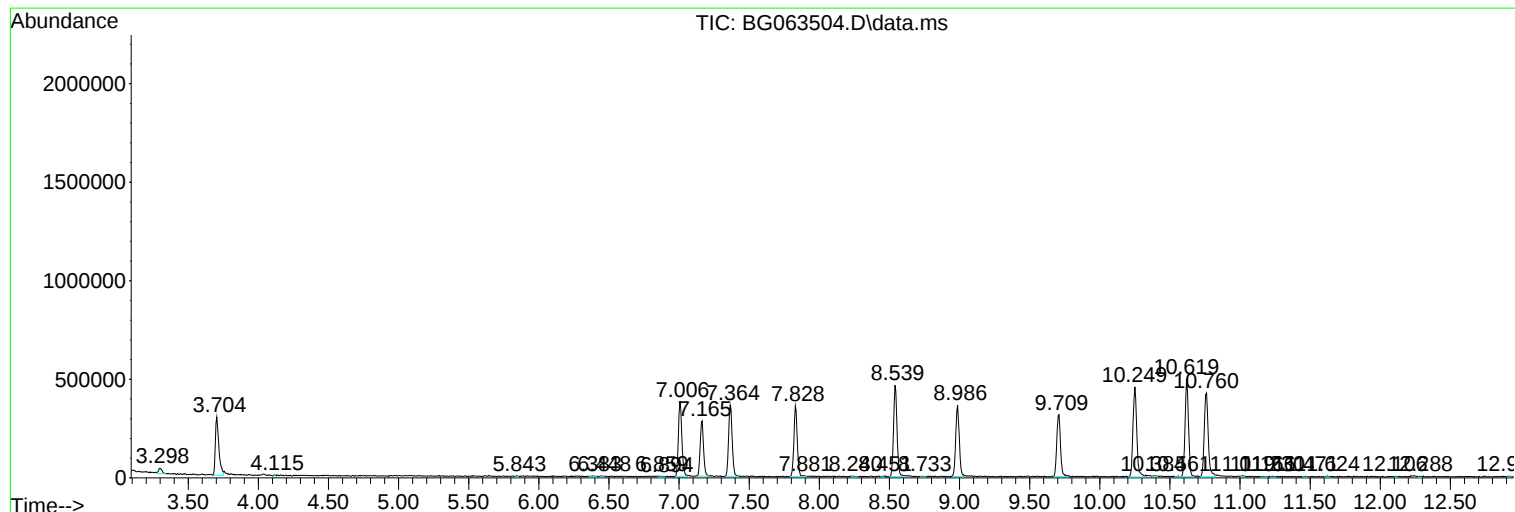

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112124\
Data File : BG063504.D
Acq On : 21 Nov 2024 11:06
Operator : RC/JU
Sample : PB165140BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK140

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112124\
Data File : BG063504.D
Acq On : 21 Nov 2024 11:06
Operator : RC/JU
Sample : PB165140BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK140

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc