

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112124\
Data File : BG063508.D
Acq On : 21 Nov 2024 16:52
Operator : RC/JU
Sample : PB165141BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK141

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
Title : SVOA CALIBRATION

Signal : TIC: BG063508.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.294	32	35	39	rBV3	24187	35119	0.96%	0.112%
2	3.512	70	72	76	rVB2	6396	5842	0.16%	0.019%
3	3.700	100	104	117	rBV	314357	540026	14.74%	1.720%
4	3.893	134	137	140	rBV3	4452	6497	0.18%	0.021%
5	4.029	158	160	162	rBV2	5164	5444	0.15%	0.017%
6	4.587	251	255	259	rBV5	3609	6551	0.18%	0.021%
7	4.969	316	320	324	rBV3	4797	8230	0.22%	0.026%
8	5.668	436	439	442	rBV3	3965	5908	0.16%	0.019%
9	5.774	454	457	459	rVB2	4953	5253	0.14%	0.017%
10	5.797	459	461	464	rBV3	4689	5229	0.14%	0.017%
11	7.002	659	666	674	rBV	405940	736317	20.10%	2.346%
12	7.160	683	693	703	rBV	329617	547104	14.93%	1.743%
13	7.366	720	728	736	rBV	419599	722089	19.71%	2.300%
14	7.830	798	807	816	rBV	302312	517236	14.12%	1.648%
15	8.541	921	928	941	rBV	492226	886957	24.21%	2.826%
16	8.864	979	983	985	rBV2	3773	4935	0.13%	0.016%
17	8.982	995	1003	1012	rBV	392268	720711	19.67%	2.296%
18	9.193	1033	1039	1040	rBV4	3405	6234	0.17%	0.020%
19	9.704	1118	1126	1140	rBV2	359326	643093	17.55%	2.049%
20	10.245	1211	1218	1231	rBV	493695	936242	25.55%	2.983%
21	10.533	1264	1267	1270	rVB3	3333	5031	0.14%	0.016%
22	10.621	1272	1282	1290	rVV	411493	759399	20.73%	2.419%
23	10.756	1299	1305	1314	rBV	455048	874854	23.88%	2.787%
24	11.402	1412	1415	1417	rBV	4974	7145	0.19%	0.023%
25	13.488	1766	1770	1772	rVB2	3652	5343	0.15%	0.017%
26	13.876	1830	1836	1846	rBV	1002307	1496342	40.84%	4.767%
27	13.993	1855	1856	1860	rBV	4613	5137	0.14%	0.016%
28	14.164	1878	1885	1893	rBV	1121368	1731042	47.24%	5.514%
29	14.475	1931	1938	1945	rBV	709716	1111676	30.34%	3.541%
30	14.693	1968	1975	1985	rBV2	280869	572745	15.63%	1.825%
31	15.022	2030	2031	2036	rVB2	6766	6470	0.18%	0.021%
32	15.210	2061	2063	2067	rVB2	5880	7109	0.19%	0.023%
33	15.468	2101	2107	2114	rBV	1485583	2265850	61.84%	7.218%
34	15.597	2123	2129	2137	rBV	400708	639042	17.44%	2.036%
35	15.703	2145	2147	2148	rBV2	6928	6656	0.18%	0.021%
36	16.255	2237	2241	2246	rBV4	3823	5723	0.16%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112124\
 Data File : BG063508.D
 Acq On : 21 Nov 2024 16:52
 Operator : RC/JU
 Sample : PB165141BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK141

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
 Title : SVOA CALIBRATION

37	16.720	2317	2320	2323	rBV4	5266	7826	0.21%	0.025%
38	17.225	2400	2406	2414	rBV	988275	1483582	40.49%	4.726%
39	17.325	2417	2423	2431	rBV	1810977	2693102	73.50%	8.579%
40	17.789	2500	2502	2504	rVB2	5556	5059	0.14%	0.016%
41	17.812	2504	2506	2507	rBV	5215	5209	0.14%	0.017%
42	17.901	2518	2521	2523	rBV	7879	5485	0.15%	0.017%
43	18.194	2569	2571	2574	rVB3	6405	5560	0.15%	0.018%
44	18.958	2699	2701	2704	rBV4	4291	4959	0.14%	0.016%
45	19.193	2736	2741	2746	rBV2	28418	40578	1.11%	0.129%
46	19.264	2748	2753	2758	rBV2	23145	43155	1.18%	0.137%
47	19.557	2800	2803	2805	rBV4	6039	6901	0.19%	0.022%
48	19.628	2808	2815	2828	rBV	2549170	3513357	95.88%	11.192%
49	19.857	2853	2854	2860	rVB3	6430	6339	0.17%	0.020%
50	20.227	2915	2917	2920	rBV4	6674	7654	0.21%	0.024%
51	20.474	2957	2959	2960	rBV2	7228	4877	0.13%	0.016%
52	21.485	3125	3131	3143	rVB	1152251	1885819	51.47%	6.008%
53	22.601	3318	3321	3328	rVB3	71184	108196	2.95%	0.345%
54	24.322	3604	3614	3628	rBV2	1429345	3664152	100.00%	11.673%
55	24.528	3640	3649	3663	rVB	747884	2054418	56.07%	6.545%




Sum of corrected areas: 31390809

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112124\
Data File : BG063508.D
Acq On : 21 Nov 2024 16:52
Operator : RC/JU
Sample : PB165141BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK141

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

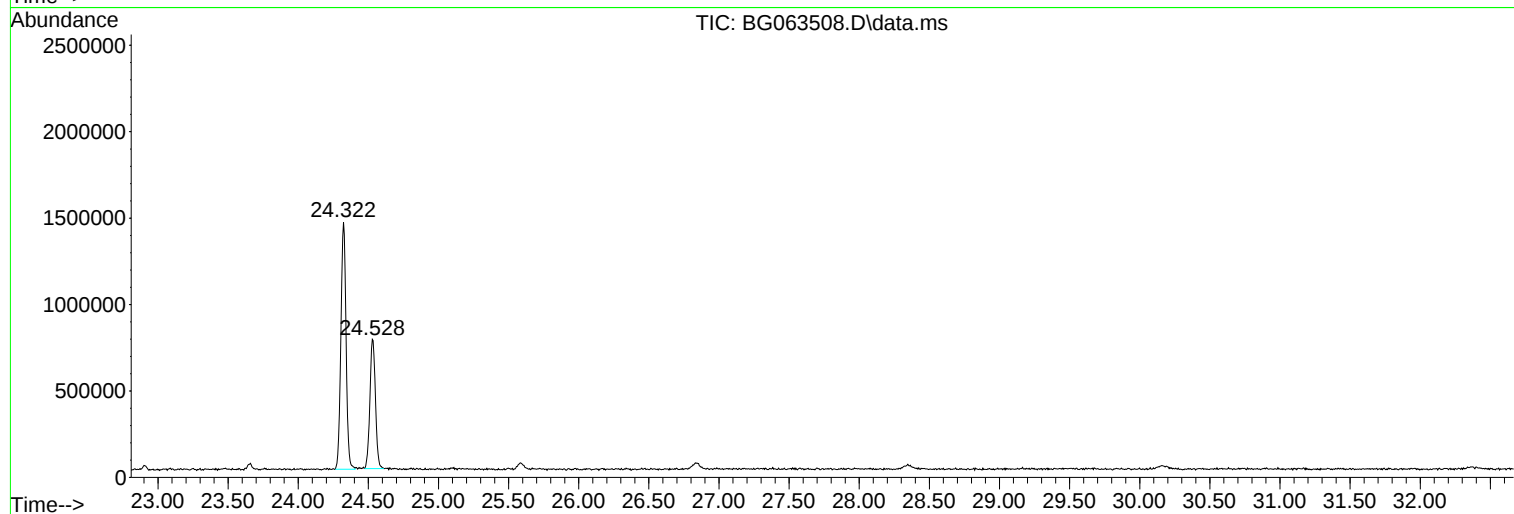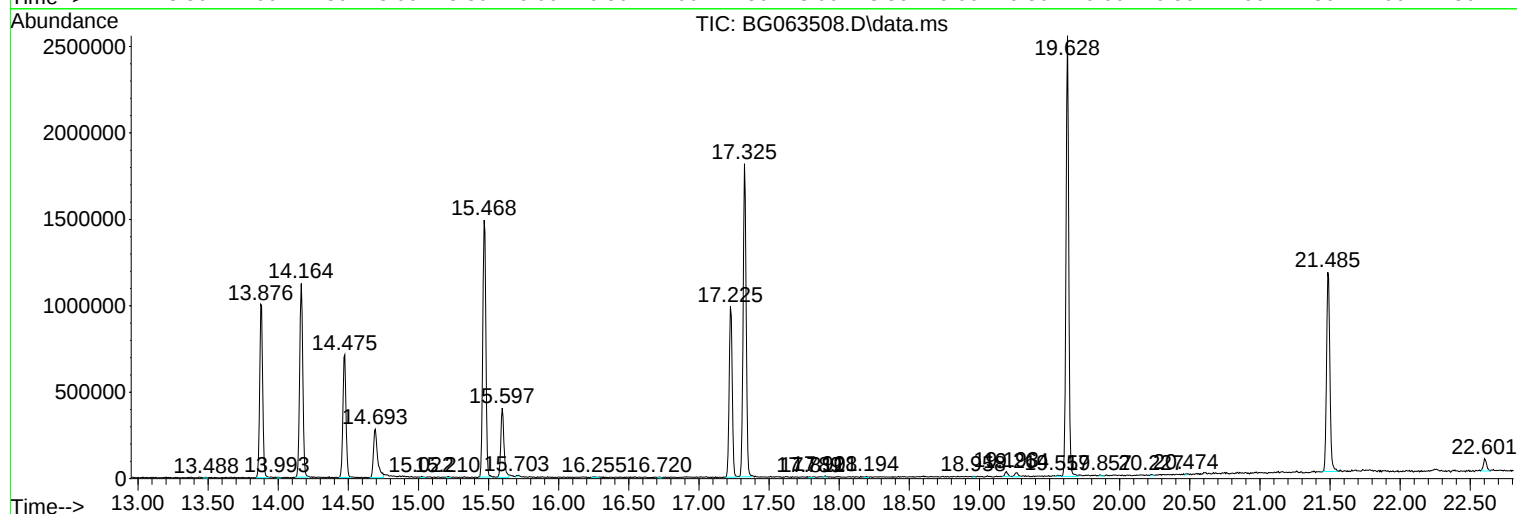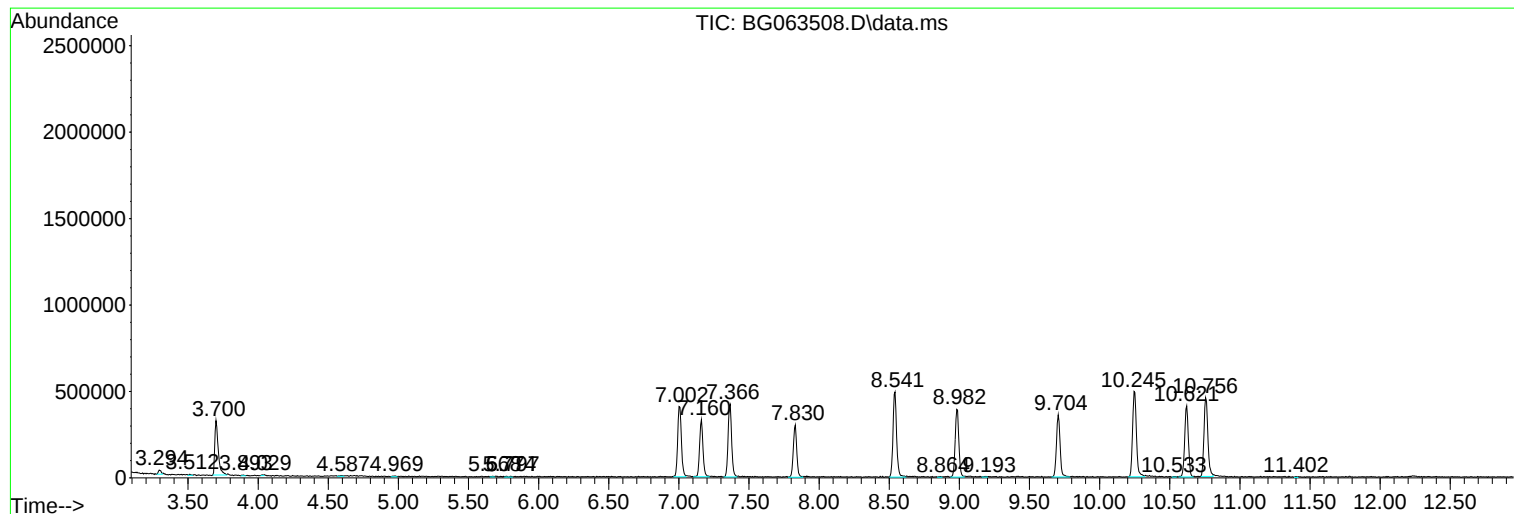

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112124\
Data File : BG063508.D
Acq On : 21 Nov 2024 16:52
Operator : RC/JU
Sample : PB165141BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK141

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112124\
Data File : BG063508.D
Acq On : 21 Nov 2024 16:52
Operator : RC/JU
Sample : PB165141BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK141

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------