


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG112215\
Data File : BG019777.D
Acq On : 22 Nov 2015 11:18
Operator : UM/NP
Sample : DFTPP33
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP33

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG111615.M
Title : SVOA CALIBRATION
Last Update : Mon Nov 23 04:11:25 2015

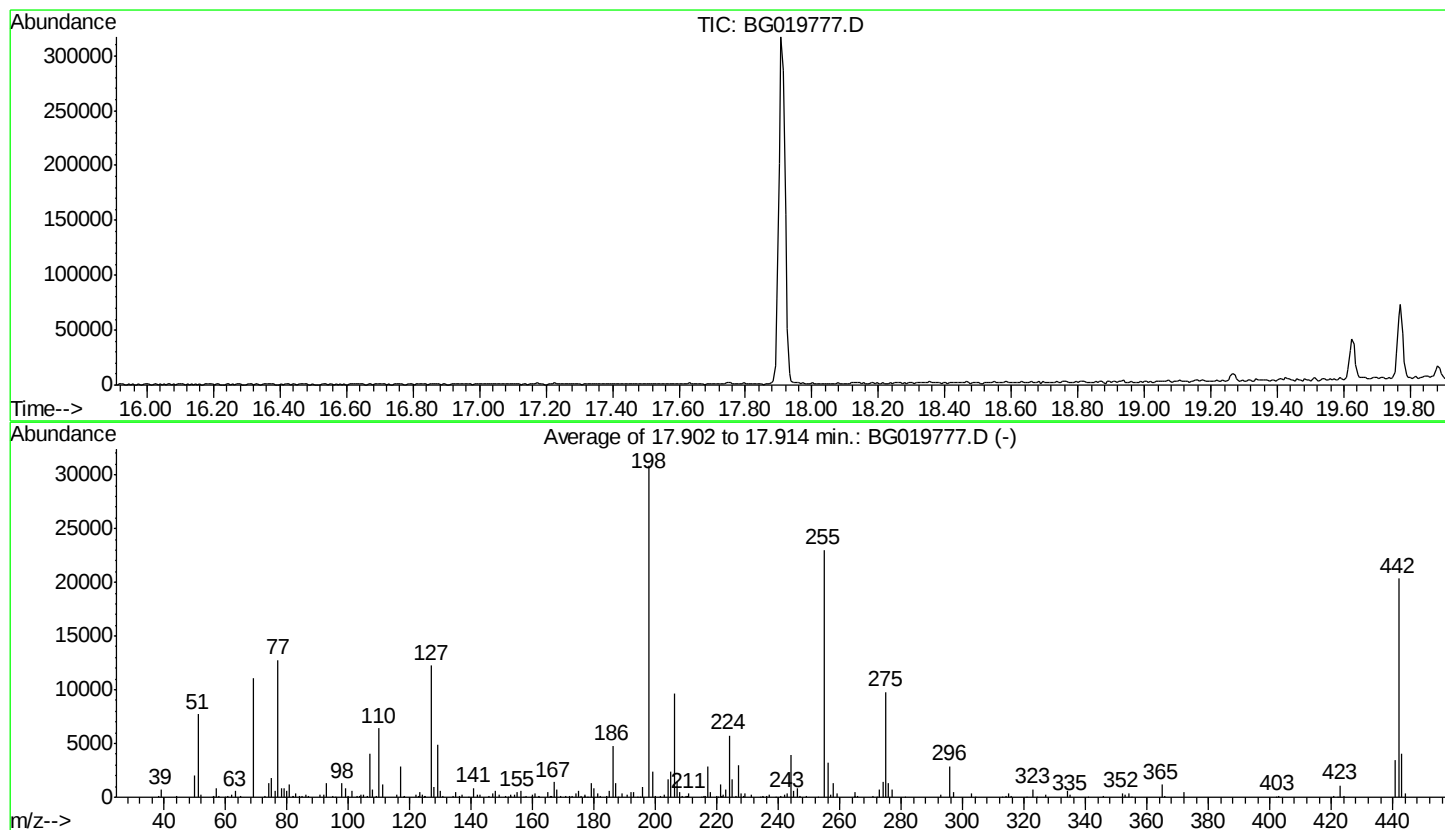

AutoFind: Scans 2564, 2565, 2566; Background Corrected with Scan 2559

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.0	7728	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.9	11065	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	39.7	12252	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	30853	PASS
199	198	5	9	7.7	2387	PASS
275	198	10	60	31.7	9790	PASS
365	198	1	100	3.7	1142	PASS
441	442	0.01	24	16.8	3416	PASS
442	198	50	100	66.0	20352	PASS
443	442	15	24	20.1	4084	PASS

m/z	Abundance
39.00	607.0
43.00	177.0
43.90	280.0
50.00	1979.0
51.00	6795.0
52.00	216.0
55.00	238.0
55.80	166.0
56.90	685.0
57.90	172.0
62.00	205.0
63.00	591.0
65.00	234.0
68.90	9982.0
73.10	264.0
73.90	1056.0
75.00	1633.0
76.00	507.0
77.00	10588.0
78.00	582.0
79.00	709.0
79.90	498.0
80.90	883.0
81.80	154.0
82.90	335.0
85.00	287.0
85.90	248.0
87.00	154.0
90.90	330.0
92.10	197.0
92.90	1019.0
98.00	1302.0
98.90	693.0
99.90	276.0
100.90	585.0
102.80	153.0
103.70	265.0
104.90	153.0
106.90	3757.0
107.90	679.0
109.90	5459.0
111.00	1035.0
115.80	150.0
117.00	2458.0
117.80	164.0
121.90	281.0
122.80	375.0
124.00	170.0
127.00	9901.0
127.90	977.0
128.90	3521.0
129.90	469.0
134.90	359.0
136.90	204.0
139.00	172.0
140.90	480.0
142.90	307.0
147.90	466.0
148.90	307.0
152.10	186.0
152.80	320.0
153.90	213.0
154.90	295.0
155.90	393.0
158.00	220.0
159.60	167.0
160.80	303.0
164.90	280.0
166.90	1100.0
168.00	636.0
172.90	258.0
173.90	337.0
175.00	445.0
176.90	302.0
178.00	155.0
178.90	1120.0
179.80	710.0
181.00	403.0
183.80	201.0
184.90	357.0
186.00	3526.0
186.90	855.0
188.90	388.0
190.80	196.0
192.00	586.0
193.00	263.0
195.90	666.0
197.90	22480.0
198.90	1595.0
200.00	279.0
202.90	231.0

Instrument :
BNA_G
ClientSampleId :
DFTPP33

203.90	1377.0
205.00	2421.0
206.00	7620.0
206.90	1206.0
207.90	479.0
210.00	263.0
210.90	260.0
215.90	164.0
216.90	2370.0
217.80	332.0
220.90	712.0
221.50	270.0
222.00	252.0
222.90	581.0
224.00	4122.0
225.00	1230.0
226.90	2121.0
227.90	364.0
228.80	338.0
231.00	249.0
234.80	175.0
235.90	198.0
236.90	250.0
239.00	184.0
243.00	380.0
243.90	2426.0
245.00	294.0
246.00	600.0
254.90	16648.0
255.90	2079.0
257.90	932.0
258.90	203.0
264.80	444.0
270.90	157.0
272.90	375.0
273.90	1139.0
275.00	8016.0
275.90	979.0
277.00	517.0
292.90	163.0
295.90	1921.0
296.90	359.0
303.00	218.0
314.90	260.0
322.90	535.0
326.90	178.0
334.00	165.0
335.00	195.0
351.90	298.0
354.00	251.0
364.90	561.0
371.90	360.0
422.90	753.0
440.90	2023.0
442.00	11394.0
442.90	2537.0
444.00	226.0

Instrument :
BNA_G
ClientSampleId :
DFTPP33

m/z	Abundance
38.00	192.0
39.00	854.0
43.00	171.0
43.90	243.0
50.00	2429.0
51.00	9625.0
52.00	423.0
56.00	372.0
57.00	817.0
58.00	158.0
60.90	266.0
62.00	204.0
63.00	652.0
64.90	299.0
68.90	12798.0
73.00	182.0
74.00	1741.0
74.90	2135.0
75.90	766.0
77.00	14988.0
78.00	912.0
78.90	937.0
79.90	825.0
80.90	1286.0
82.00	364.0
82.90	325.0
84.00	218.0
86.00	255.0
87.00	170.0
90.90	357.0
92.00	309.0
92.90	1309.0
94.90	295.0
97.90	1180.0
98.90	1050.0
100.00	159.0
100.90	619.0
104.00	508.0
104.90	323.0
106.10	212.0
106.90	4836.0
108.00	1007.0
108.90	242.0
109.90	7049.0
110.90	1331.0
115.90	350.0
117.00	3350.0
118.00	411.0
122.00	184.0
123.00	745.0
124.10	271.0
124.80	213.0
127.00	13996.0
127.90	814.0
128.90	5558.0
129.90	656.0
130.90	273.0
134.00	179.0
135.00	771.0
135.90	200.0
136.80	185.0
140.90	1142.0
141.90	377.0
142.90	200.0
145.80	163.0
147.00	667.0
147.90	886.0
148.90	344.0
151.20	186.0
153.00	333.0
153.90	172.0
154.90	691.0
156.00	756.0
157.80	306.0
159.90	240.0
160.90	557.0
161.80	174.0
165.00	648.0
165.90	204.0
167.00	1851.0
167.90	907.0
169.00	211.0
172.00	255.0
173.00	175.0
173.80	298.0
175.00	566.0
175.90	199.0
176.80	338.0
178.90	1783.0
179.90	1107.0
180.90	319.0

Instrument :
BNA_G
ClientSampleId :
DFTPP33

181.90	204.0
183.90	209.0
185.00	877.0
185.90	5733.0
187.00	1507.0
188.00	175.0
188.80	421.0
190.90	155.0
192.00	409.0
192.90	385.0
194.90	176.0
195.90	1161.0
197.90	37008.0
198.90	2815.0
201.60	224.0
202.90	308.0
203.90	1962.0
204.90	2514.0
206.00	10943.0
206.90	2429.0
207.90	474.0
209.80	165.0
210.80	327.0
216.10	276.0
216.90	3184.0
217.90	430.0
219.80	279.0
221.00	1644.0
221.70	377.0
222.90	723.0
224.00	6760.0
225.00	2205.0
226.00	245.0
226.90	3698.0
227.90	511.0
229.00	592.0
231.00	163.0
234.00	184.0
235.00	151.0
236.00	256.0
237.00	357.0
240.80	210.0
241.90	321.0
242.90	389.0
244.00	5244.0
245.00	707.0
246.00	1033.0
247.10	288.0
249.00	271.0
254.90	27432.0
256.00	3627.0
256.90	521.0
258.00	1600.0
258.80	245.0
265.00	678.0
270.80	158.0
272.90	818.0
273.90	1386.0
275.00	11202.0
275.90	1335.0
276.90	1060.0
292.90	279.0
295.90	3929.0
297.00	551.0
302.80	465.0
303.90	176.0
313.90	221.0
314.90	350.0
315.90	184.0
320.80	177.0
323.00	782.0
324.00	188.0
327.00	256.0
334.00	691.0
335.00	179.0
351.90	459.0
353.00	340.0
354.00	478.0
355.00	169.0
364.90	1367.0
365.90	256.0
372.00	500.0
402.80	297.0
420.90	286.0
422.90	1128.0
424.00	283.0
441.00	4185.0
442.00	23248.0
443.00	4490.0
443.90	459.0

Instrument :
BNA_G
ClientSampleId :
DFTPP33

m/z	Abundance
39.00	523.0
44.00	324.0
50.00	1811.0
51.00	6764.0
51.90	255.0
54.90	167.0
55.90	151.0
57.00	837.0
60.00	160.0
62.00	175.0
63.00	415.0
68.90	10415.0
73.00	258.0
74.00	1266.0
74.90	1649.0
75.90	629.0
77.00	12715.0
78.00	872.0
79.00	981.0
79.90	616.0
80.90	1297.0
81.80	264.0
83.00	396.0
85.00	211.0
85.90	276.0
92.00	283.0
93.00	1481.0
95.90	165.0
98.00	1365.0
99.00	862.0
101.00	622.0
102.80	376.0
104.00	264.0
104.90	357.0
105.90	170.0
107.00	3737.0
108.10	307.0
110.00	6668.0
111.00	1142.0
116.00	259.0
117.00	2861.0
121.80	408.0
123.00	578.0
123.90	157.0
125.00	251.0
127.00	12860.0
127.90	987.0
128.90	5553.0
129.80	629.0
130.90	225.0
134.00	206.0
134.90	323.0
136.00	182.0
136.90	203.0
140.90	1062.0
141.80	308.0
142.90	356.0
145.80	165.0
146.90	320.0
147.80	478.0
148.90	154.0
151.00	251.0
152.90	245.0
153.90	210.0
154.90	544.0
155.90	614.0
156.90	161.0
159.90	357.0
160.90	315.0
162.00	215.0
164.90	379.0
166.10	237.0
166.90	1248.0
168.00	692.0
169.00	192.0
170.90	229.0
174.00	486.0
174.90	751.0
177.10	240.0
178.80	1107.0
180.00	703.0
180.90	308.0
184.90	710.0
185.90	5158.0
187.00	1626.0
188.90	354.0
190.90	293.0
192.00	618.0
192.80	621.0
194.00	189.0
195.90	1098.0

Instrument :
BNA_G
ClientSampleId :
DFTPP33

197.90	33072.0
198.90	2751.0
199.90	224.0
202.90	181.0
203.90	1582.0
204.90	2393.0
206.00	10242.0
207.00	1443.0
207.90	482.0
208.70	207.0
210.10	270.0
210.90	405.0
214.70	179.0
215.80	236.0
216.90	2950.0
217.90	549.0
220.10	151.0
220.90	1216.0
221.90	459.0
223.00	761.0
224.00	6457.0
225.00	1612.0
226.10	274.0
226.90	3019.0
227.90	327.0
228.90	554.0
231.00	332.0
234.80	235.0
236.80	243.0
240.90	214.0
241.80	261.0
242.80	419.0
243.90	4227.0
245.00	651.0
245.90	890.0
246.90	171.0
248.90	195.0
252.70	181.0
254.90	25016.0
255.90	4127.0
256.90	307.0
257.90	1312.0
258.90	473.0
264.90	703.0
265.90	255.0
272.00	161.0
272.90	784.0
273.90	1739.0
274.90	10154.0
275.90	1746.0
276.90	746.0
281.00	174.0
292.90	221.0
295.90	2914.0
296.90	396.0
302.90	332.0
312.90	170.0
314.90	384.0
315.90	322.0
323.00	1016.0
326.90	341.0
334.00	952.0
335.00	198.0
340.90	178.0
345.90	395.0
351.80	370.0
352.90	338.0
354.00	239.0
364.90	1498.0
372.00	621.0
401.90	161.0
402.90	215.0
420.90	211.0
421.90	171.0
423.00	1521.0
423.90	233.0
441.00	4040.0
442.00	26416.0
443.00	5225.0
444.00	444.0

Instrument :
BNA_G
ClientSampleId :
DFTPP33

Scan 2559 (17.873 min): BG019777.D
DFTPP33

m/z	Abundance
41.00	180.0
43.00	289.0
44.00	199.0
54.90	205.0
67.10	167.0
72.90	153.0
206.90	237.0

Instrument :
BNA_G
ClientSampleId :
DFTPP33