
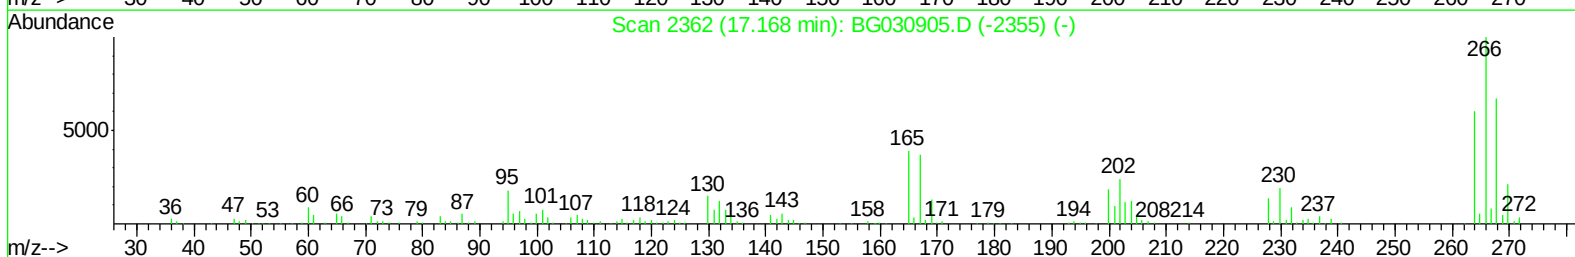
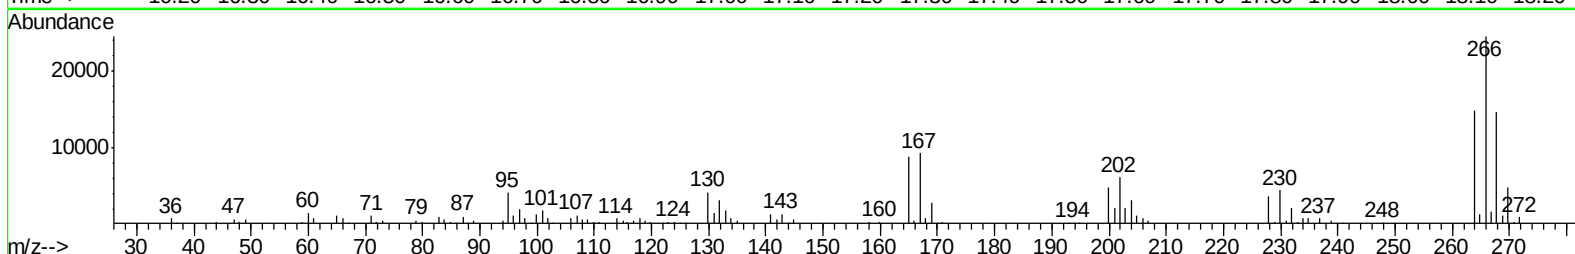


Data Path : Z:\HPCHEM1\BNA G\Data\BG112217\
 Data File : BG031204.D
 Acq On : 23 Nov 2017 00:56
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 24 01:57:05 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG111017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 10 15:38:25 2017
 Response via : Initial Calibration

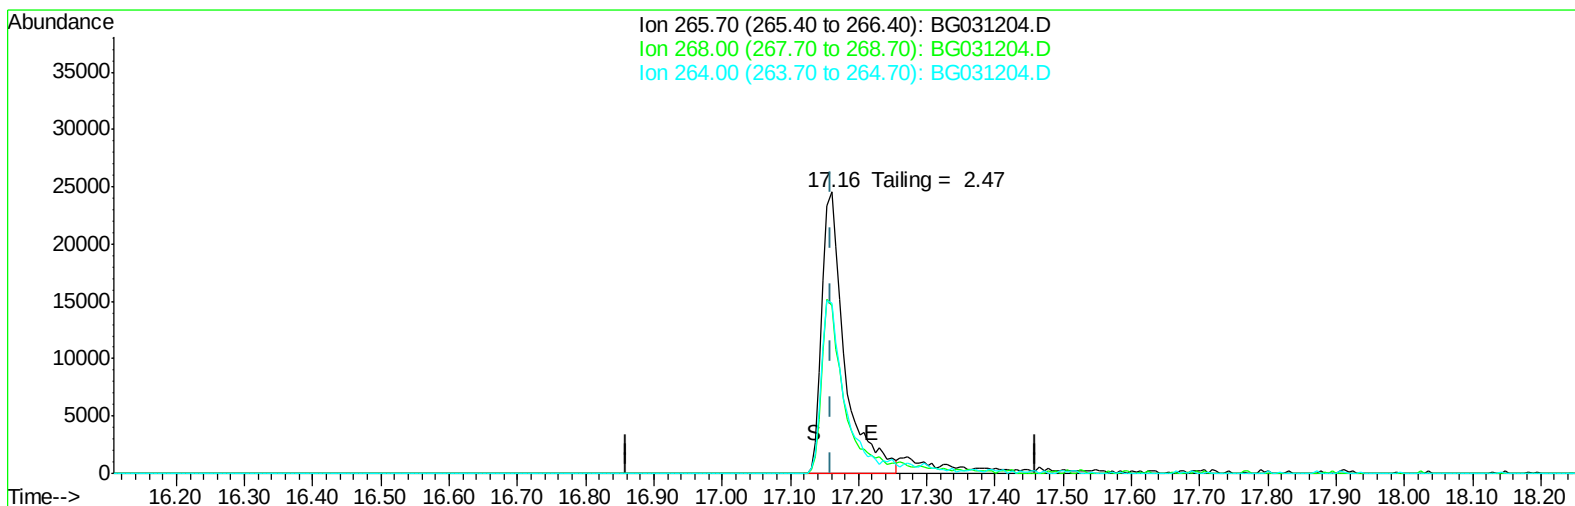

TIC: BG031204.D

(69) Pentachlorophenol (C)




17.160min (+0.000) 0.00ng

response 56626

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	59.65
264.00	62.00	60.47
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\Data\BG112217\
 Data File : BG031204.D
 Acq On : 23 Nov 2017 00:56
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 24 01:57:05 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG111017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 10 15:38:25 2017
 Response via : Initial Calibration

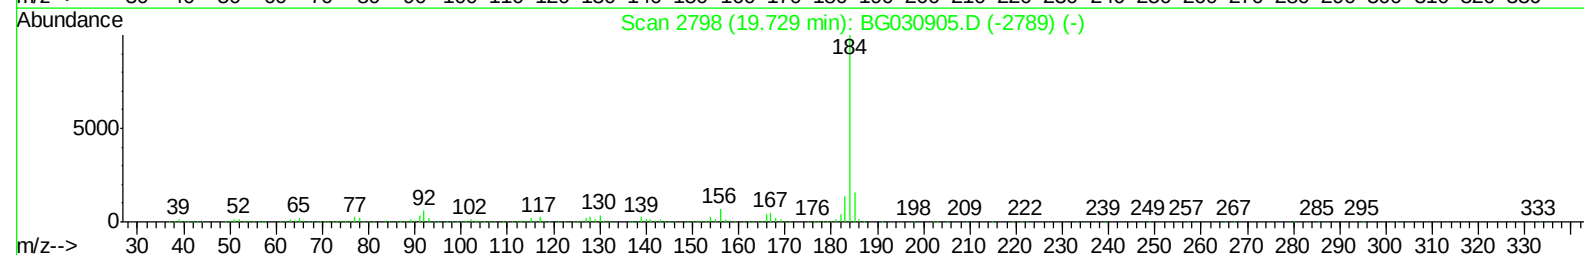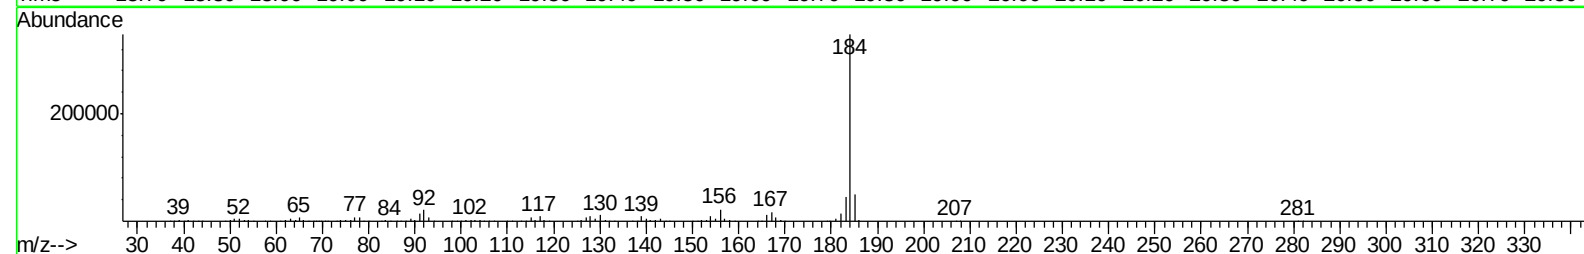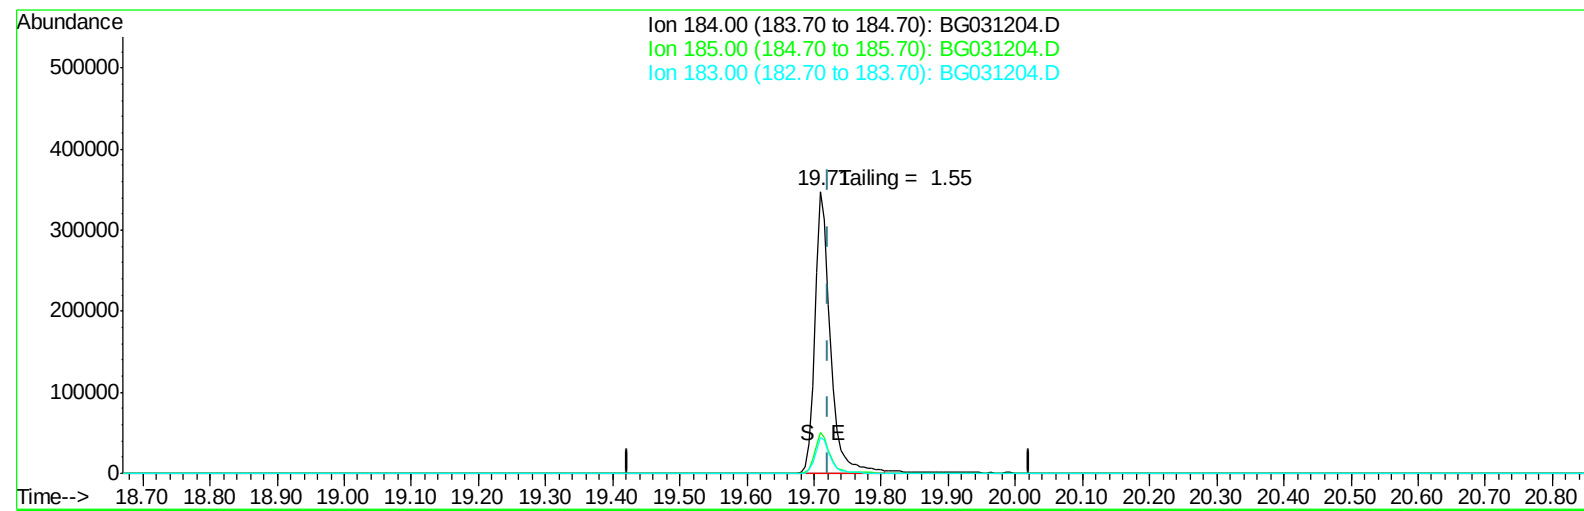

TIC: BG031204.D

(76) Benzidine

19.710min (-0.012) 0.00ng

response 553631

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.35
183.00	13.30	12.75
0.00	0.00	0.00