

Data Path : Z:\HPCHEM1\BNA G\DATA\BG112217\
 Data File : BG031196.D
 Acq On : 22 Nov 2017 19:18
 Operator : SJ/JU
 Sample : I6525-06
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MW-11

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG111017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.692	400	409	420	rBV	432304	774958	12.71%	3.292%
2	7.302	674	683	694	rBV	269289	508317	8.33%	2.160%
3	7.667	737	745	765	rBV	855748	1563106	25.63%	6.641%
4	8.137	818	825	833	rBV	193845	340128	5.58%	1.445%
5	8.460	872	880	893	rBV	846215	1509937	24.76%	6.415%
6	9.306	1013	1024	1039	rBV	608590	1193628	19.57%	5.071%
7	10.951	1297	1304	1314	rBV	250905	506588	8.31%	2.152%
8	13.378	1710	1717	1737	rBV	2089255	3470840	56.91%	14.745%
9	14.758	1944	1952	1965	rBV2	453892	807036	13.23%	3.429%
10	16.239	2197	2204	2216	rBV	1684793	2701232	44.29%	11.476%
11	17.496	2410	2418	2432	rBV2	678797	1123331	18.42%	4.772%
12	20.087	2852	2859	2870	rBV	4431700	6098732	100.00%	25.910%
13	21.768	3138	3145	3160	rBV2	845099	1512841	24.81%	6.427%
14	25.064	3695	3706	3724	rBV2	466889	1427819	23.41%	6.066%


Sum of corrected areas: 23538493

Data Path : Z:\HPCHEM1\BNA G\DATA\BG112217\
Data File : BG031196.D
Acq On : 22 Nov 2017 19:18
Operator : SJ/JU
Sample : I6525-06
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-11

Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG111017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

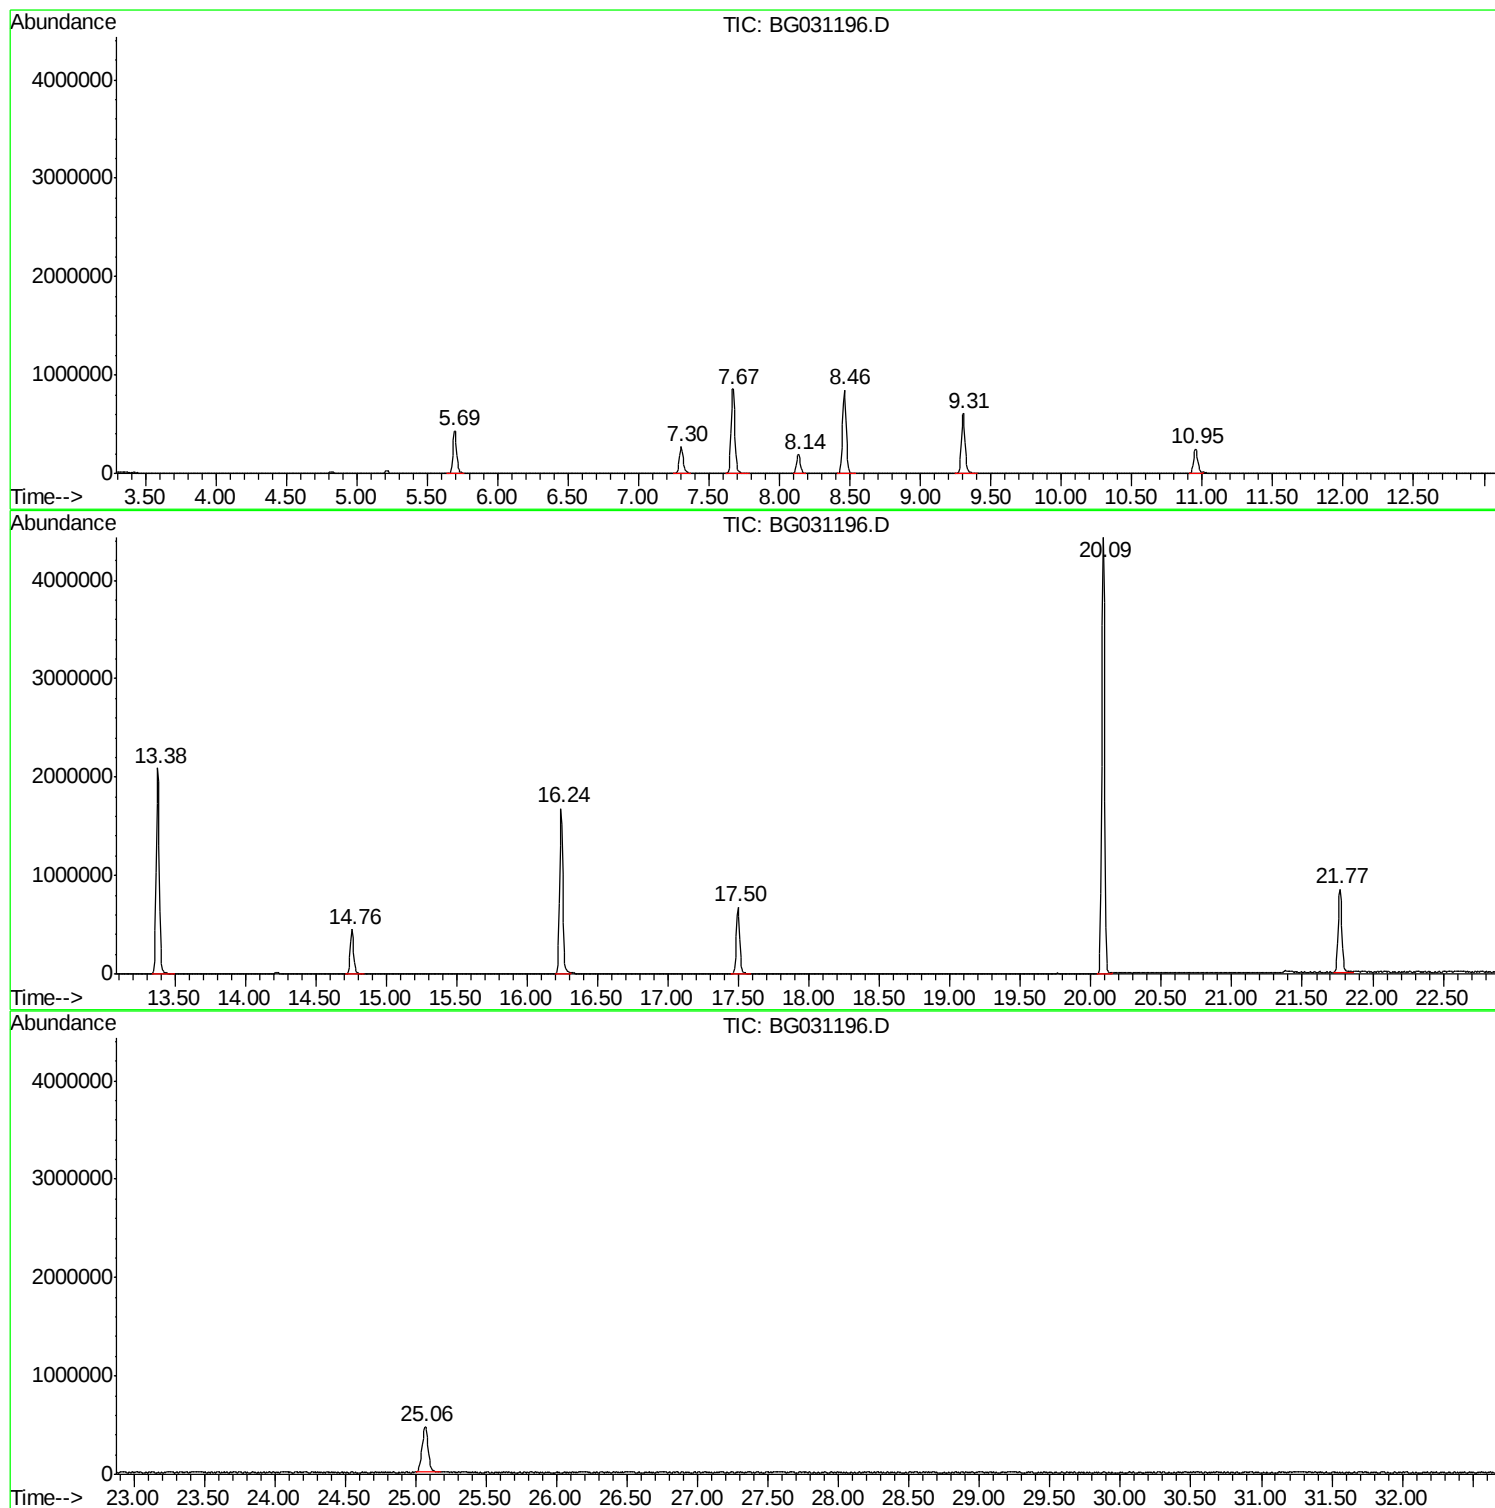

Data Path : Z:\HPCHEM1\BNA G\DATA\BG112217\
Data File : BG031196.D
Acq On : 22 Nov 2017 19:18
Operator : SJ/JU
Sample : I6525-06
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-11










Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG111017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.67 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.67	91.91 ng	1563110	1,4-Dichlorobenzene-d4	8.14

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	25
3		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	12
4		5-Aminoindole	132	C8H8N2	005192-03-0	12
5		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9

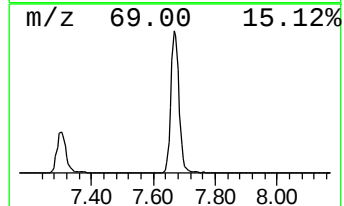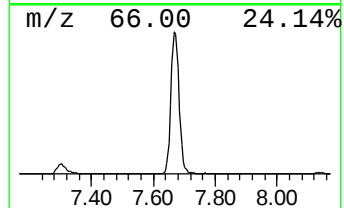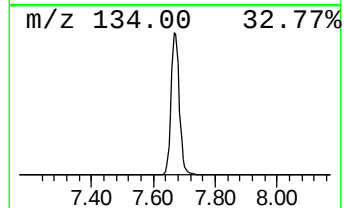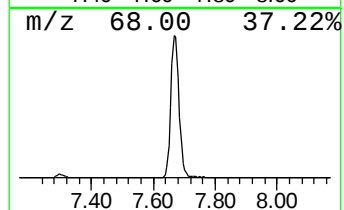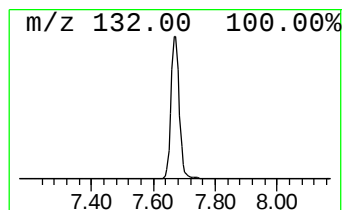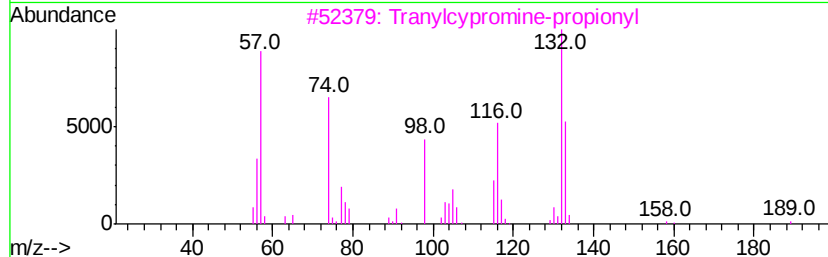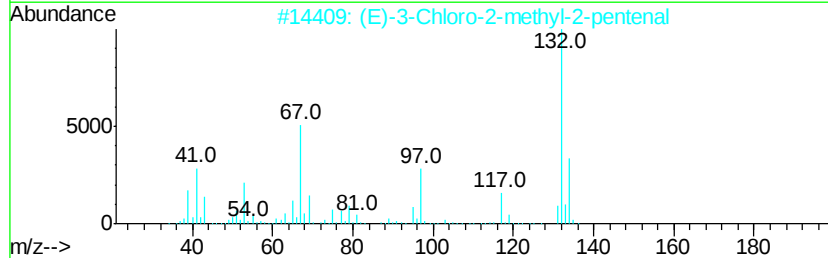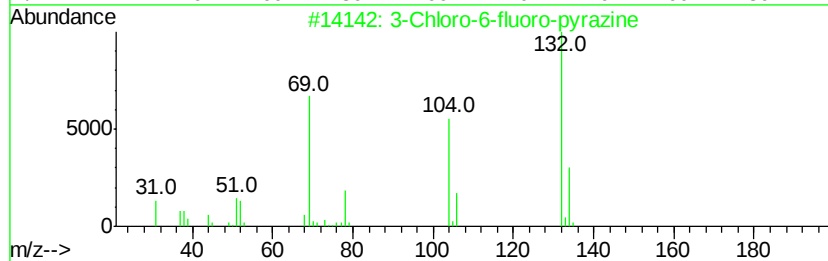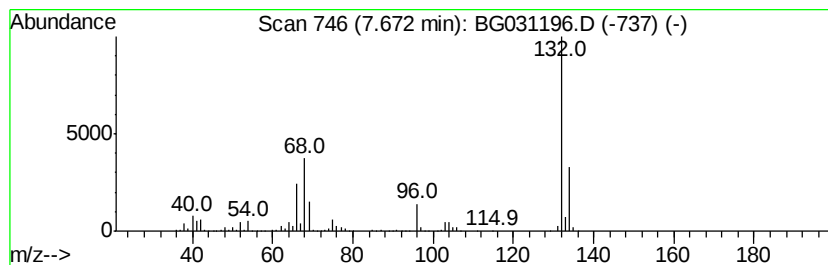

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG112217\
Data File : BG031196.D
Acq On : 22 Nov 2017 19:18
Operator : SJ/JU
Sample : I6525-06
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-11

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG111017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.67	7.67	91.9	ng	1563110	1	8.14	340128	20.0