
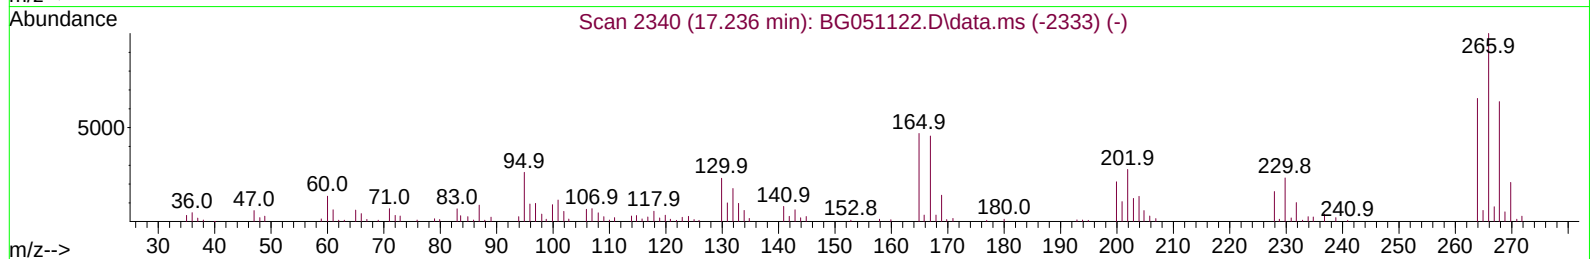
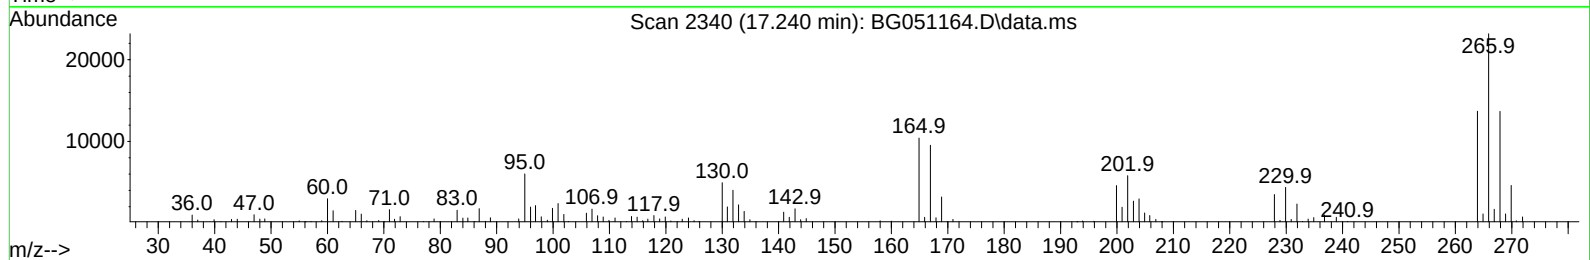


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112221\
Data File : BG051164.D
Acq On : 22 Nov 2021 9:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 22 17:13:28 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 19 16:26:22 2021
Response via : Initial Calibration

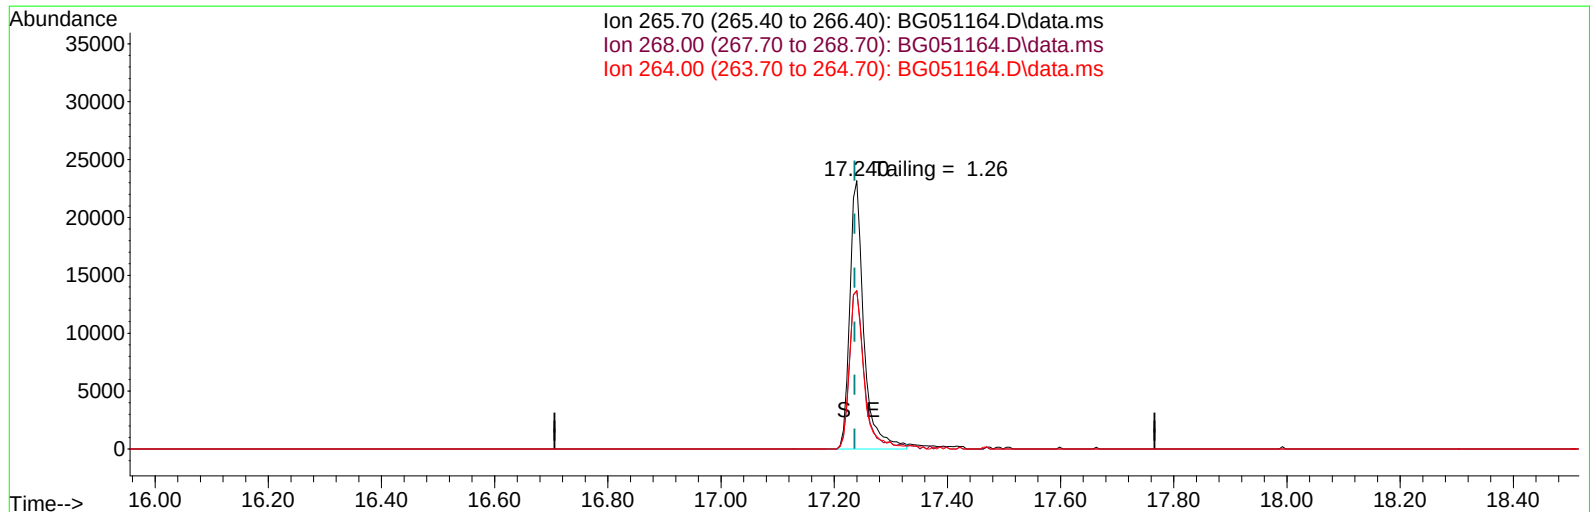

TIC: BG051164.D\data.ms

(70) Pentachlorophenol (C)




17.240min (+ 0.004) 45406.10 ng

response 41300

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	58.99
264.00	61.30	59.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112221\
Data File : BG051164.D
Acq On : 22 Nov 2021 9:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 22 17:13:28 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 19 16:26:22 2021
Response via : Initial Calibration

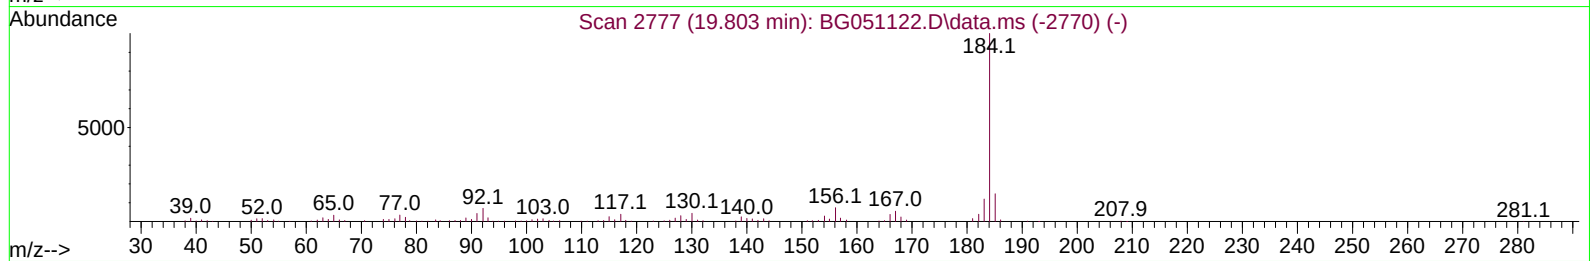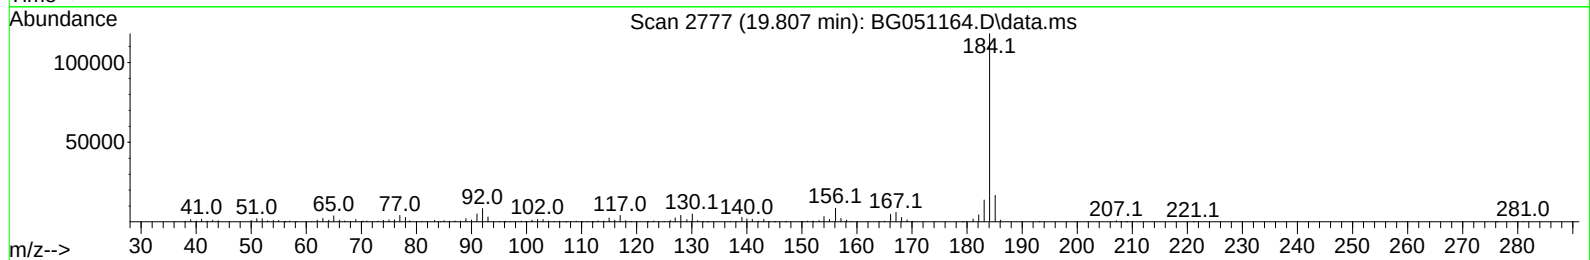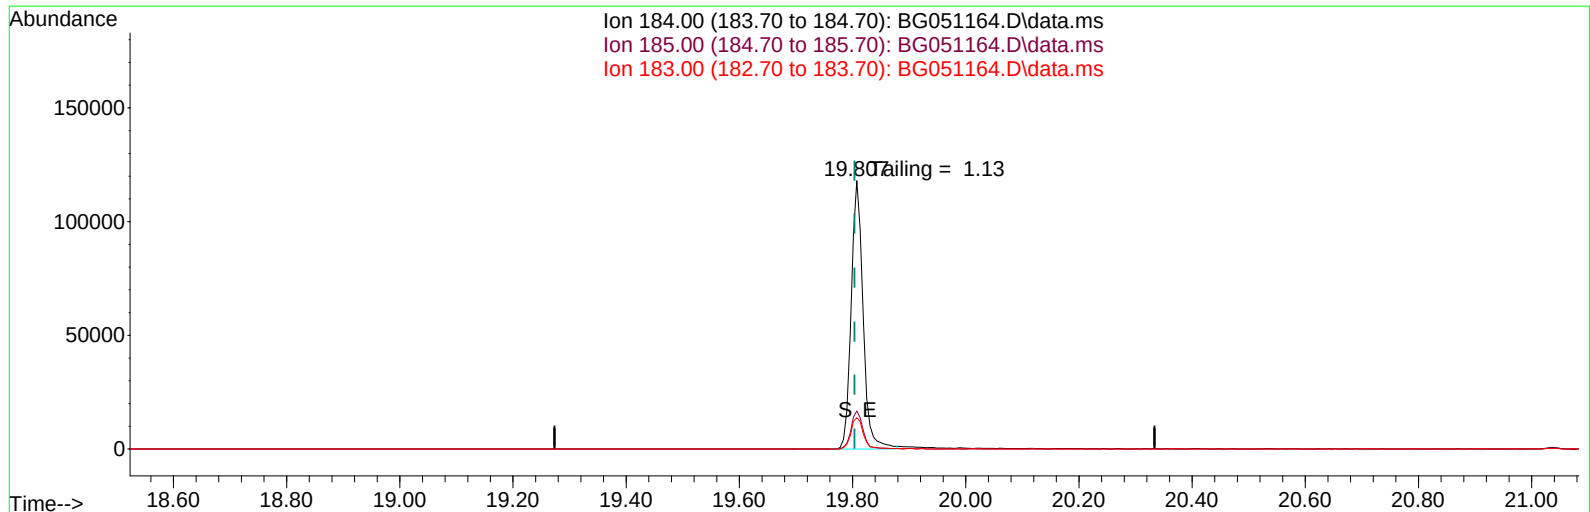

TIC: BG051164.D\data.ms

(77) Benzidine**19.807min (+ 0.004) 187225.68 ng****response 175234**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.19
183.00	11.70	11.66
0.00	0.00	0.00