
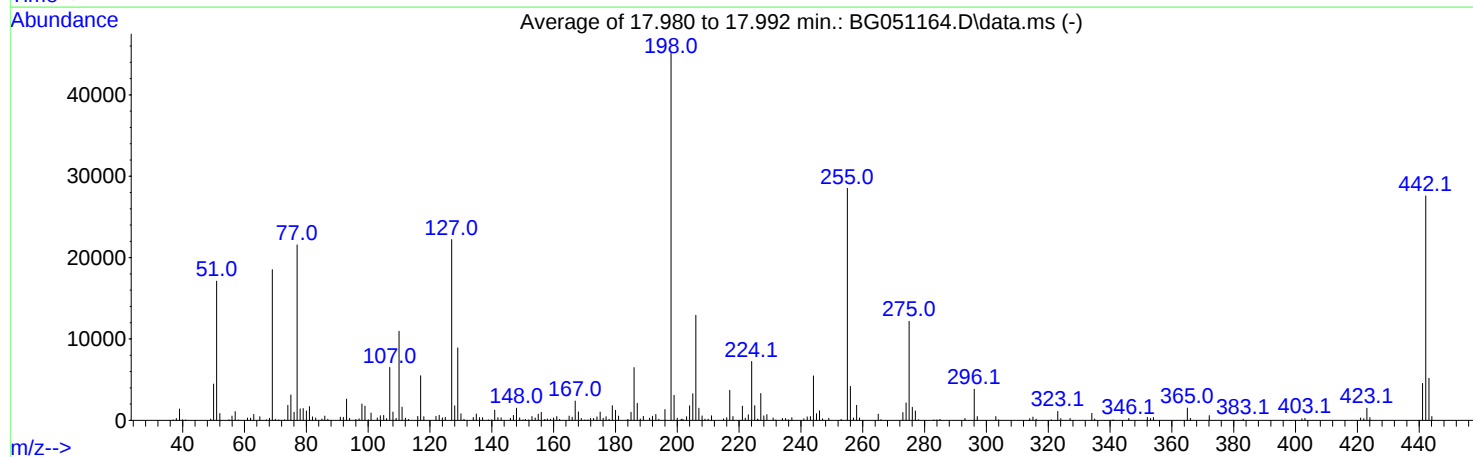


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112221\
 Data File : BG051164.D
 Acq On : 22 Nov 2021 9:25
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Nov 19 16:26:22 2021

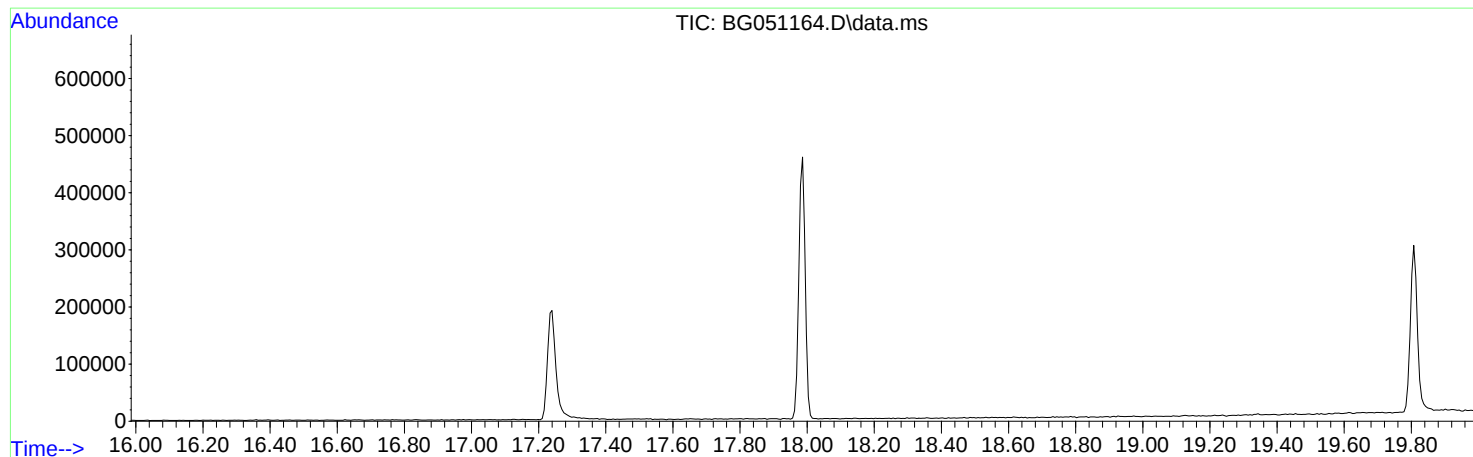




AutoFind: Scans 2466, 2467, 2468; Background Corrected with Scan 2459

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.8	17098	PASS
68	69	0.00	2	1.4	259	PASS
69	198	0.00	100	41.0	18531	PASS
70	69	0.00	2	0.7	136	PASS
127	198	10	80	49.1	22213	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	45205	PASS
199	198	5	9	6.8	3093	PASS
275	198	10	60	26.9	12173	PASS
365	198	1	100	3.4	1523	PASS
441	198	0.01	100	10.1	4544	PASS
442	442	50	100	100.0	27587	PASS
443	442	15	24	18.7	5168	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112221\
Data File : BG051164.D
Acq On : 22 Nov 2021 9:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 22 17:13:28 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 19 16:26:22 2021
Response via : Initial Calibration

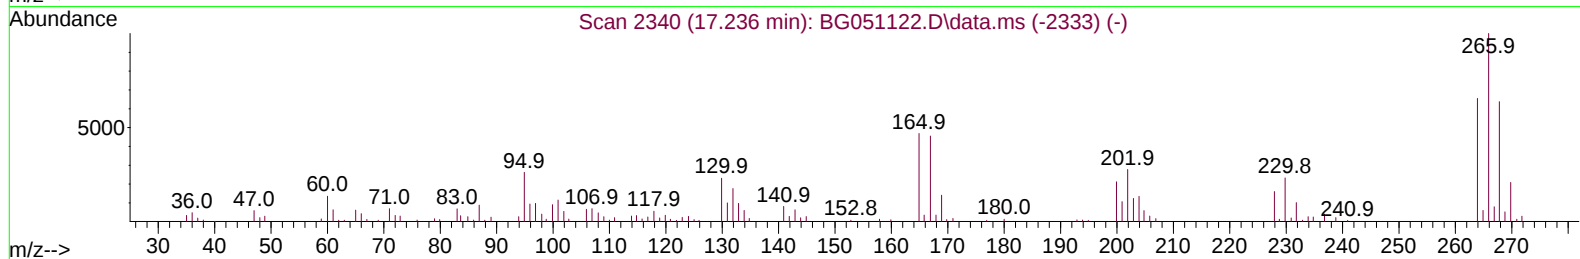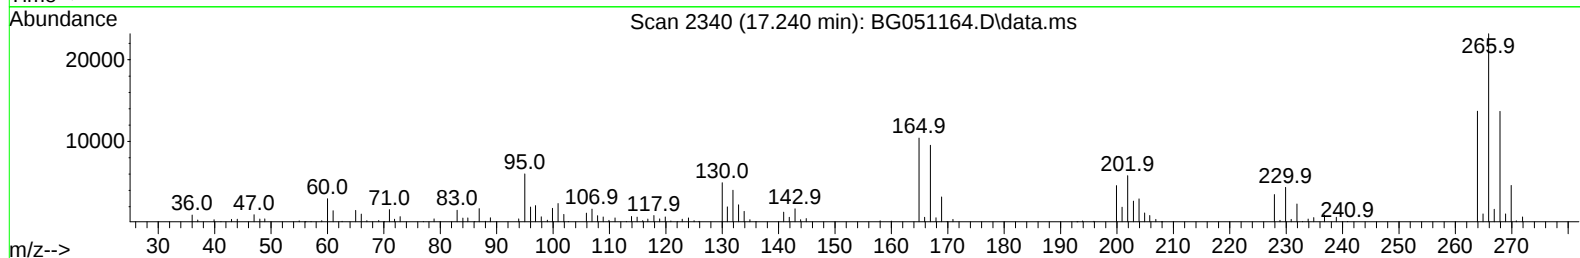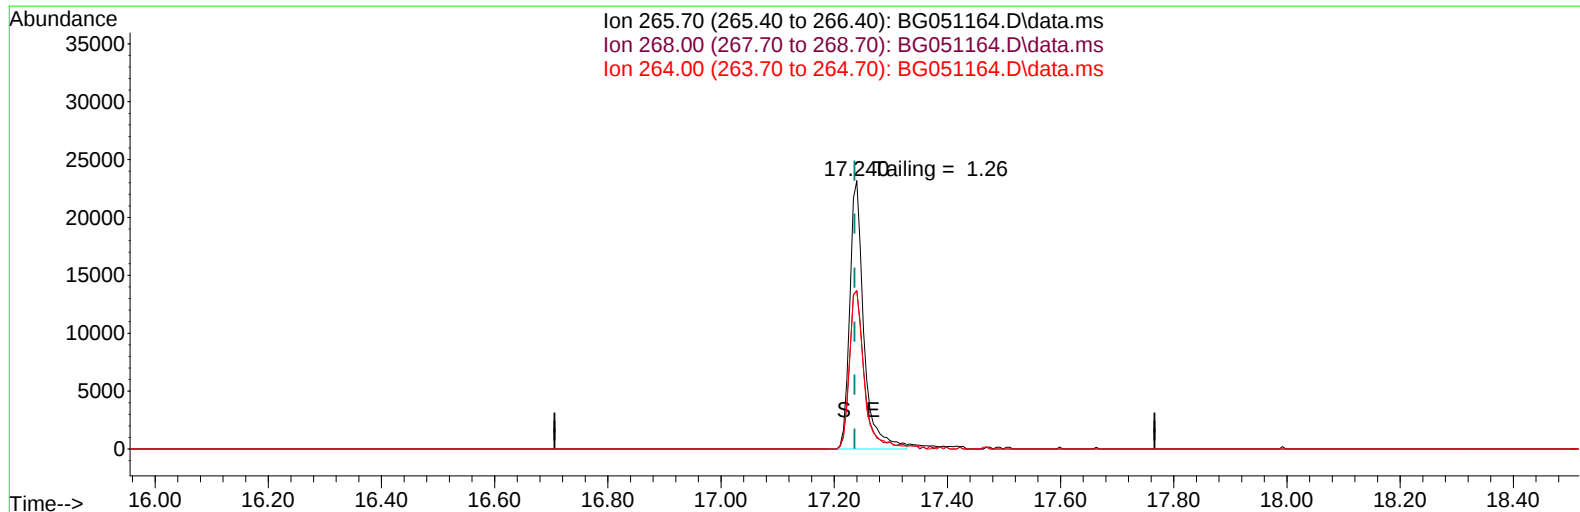

TIC: BG051164.D\data.ms

(70) Pentachlorophenol (C)

17.240min (+ 0.004) 45406.10 ng




response 41300

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	58.99
264.00	61.30	59.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112221\
Data File : BG051164.D
Acq On : 22 Nov 2021 9:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 22 17:13:28 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 19 16:26:22 2021
Response via : Initial Calibration

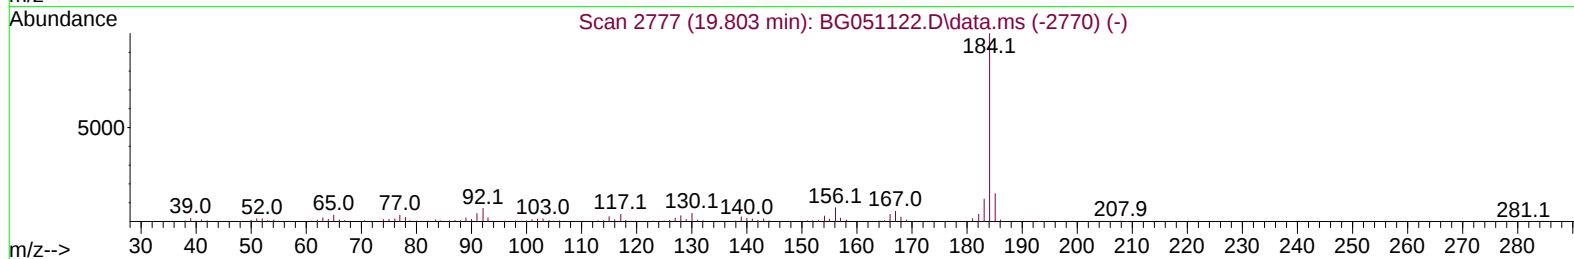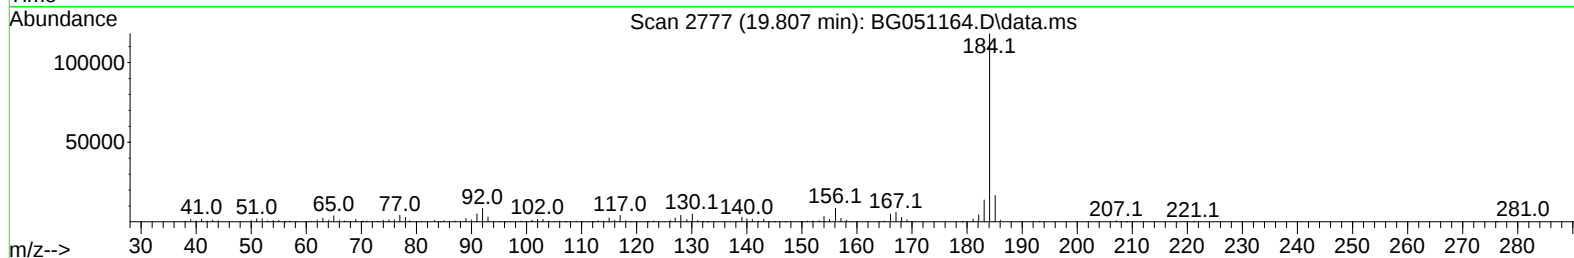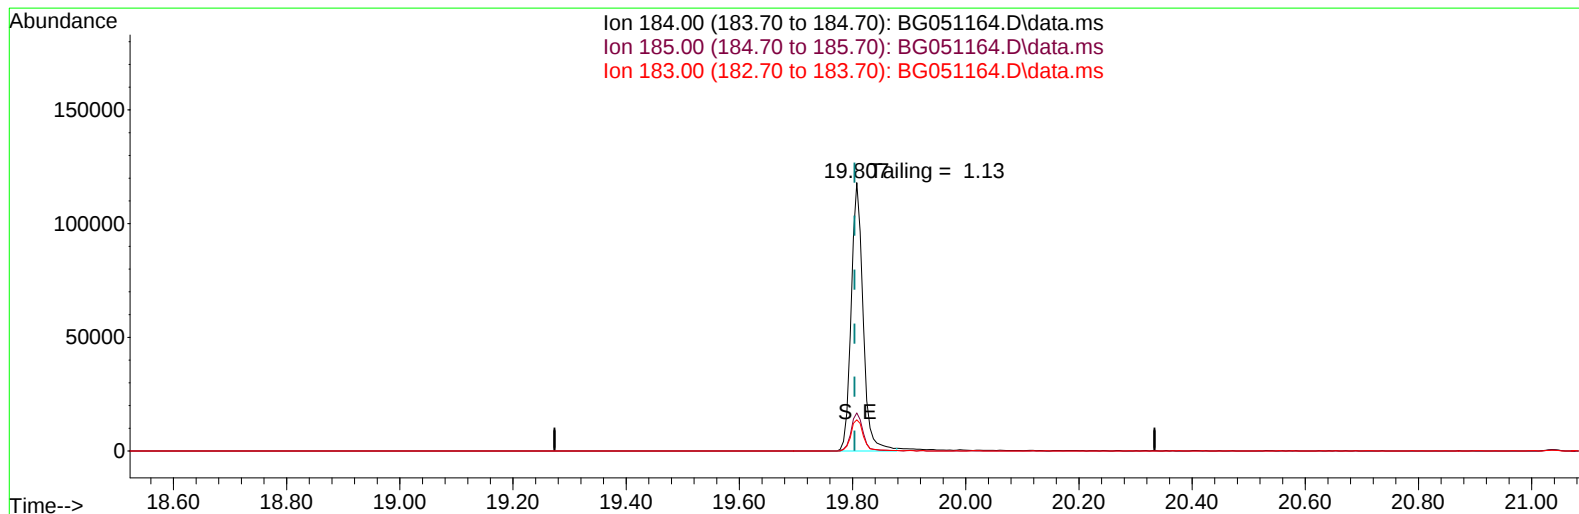

TIC: BG051164.D\data.ms

(77) Benzidine

19.807min (+ 0.004) 187225.68 ng

response 175234

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.19
183.00	11.70	11.66
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/22/2021	BNA_G	BG051164.D
Compound Name	Response	Retention Time
DDT	161491	21.03
DDD	4391	20.58
DDE	0	19.75
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4391	165882	2.65

Instrument :
BNA_G
ClientSampleId :
DFTPP