
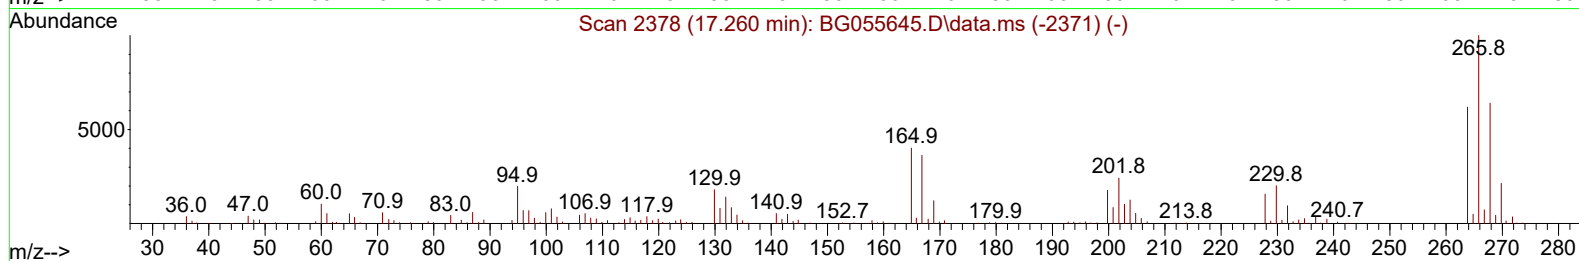
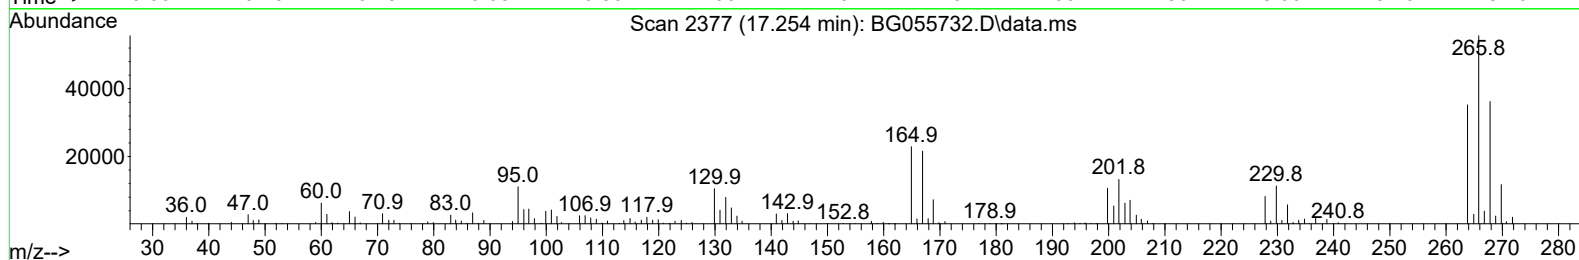


```
Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112222\  
Data File : BG055732.D  
Acq On    : 22 Nov 2022    9:25  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Nov 23 06:52:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 23 01:35:20 2022
Response via : Initial Calibration

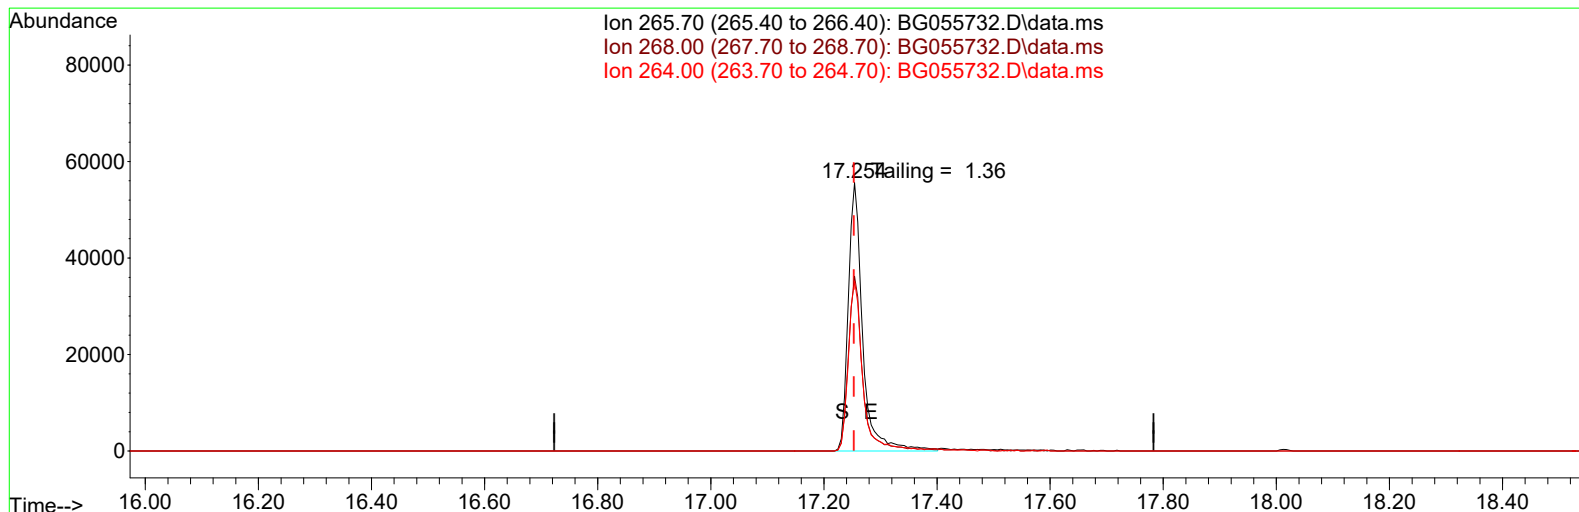

TIC: BG055732.D\data.ms

(70) Pentachlorophenol (C)




17.254min (+ 0.001) 206413.22 ng

response **98907**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	65.14
264.00	61.90	63.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112222\
Data File : BG055732.D
Acq On : 22 Nov 2022 9:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 23 06:52:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 23 01:35:20 2022
Response via : Initial Calibration

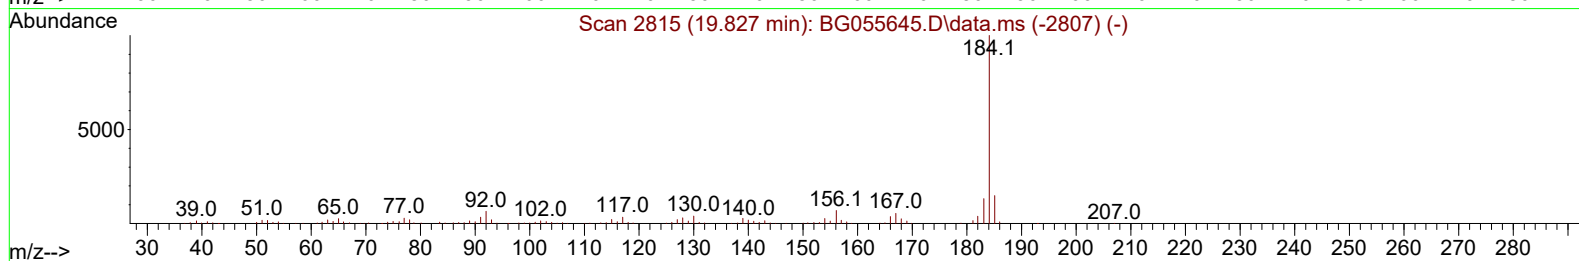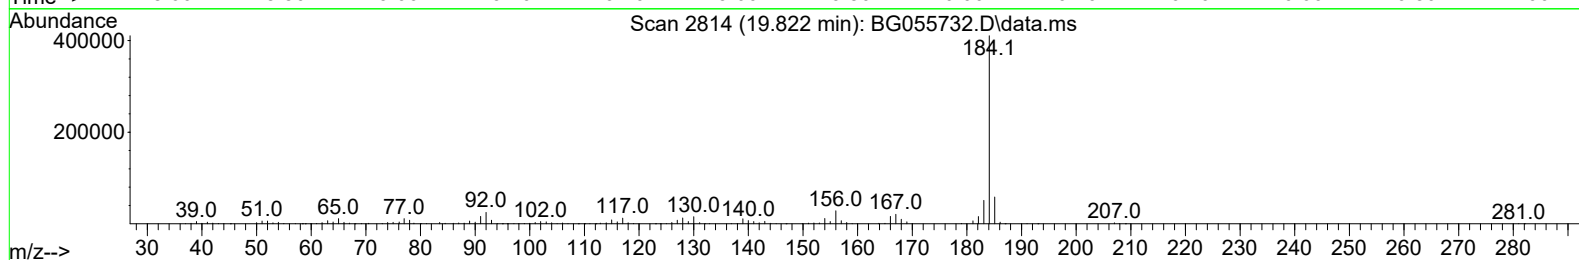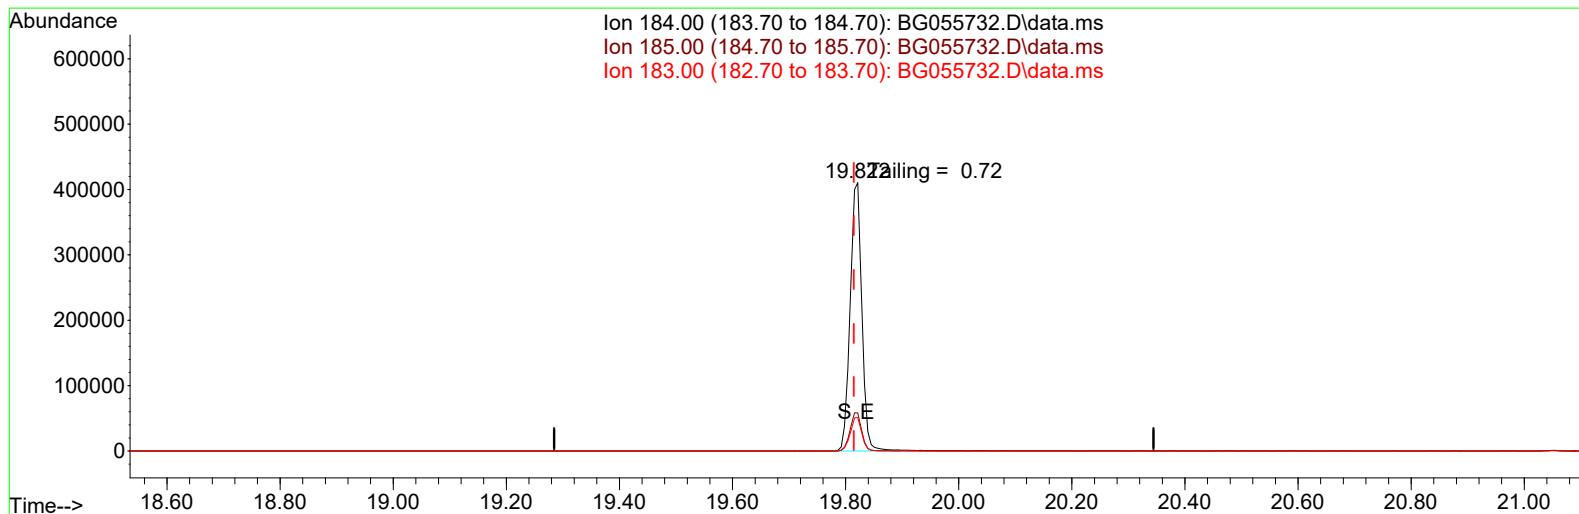

TIC: BG055732.D\data.ms

(77) Benzidine**19.822min (+ 0.007) 118403.87 ng****response 594409**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.24
183.00	13.20	12.45
0.00	0.00	0.00