
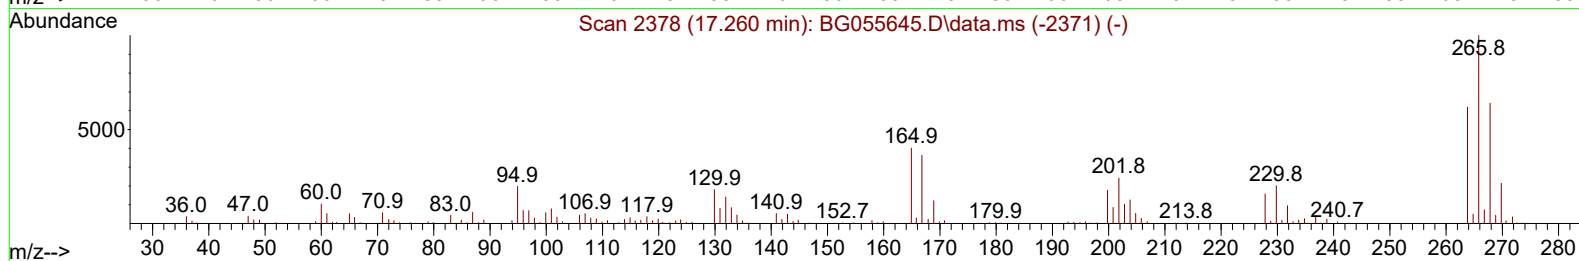
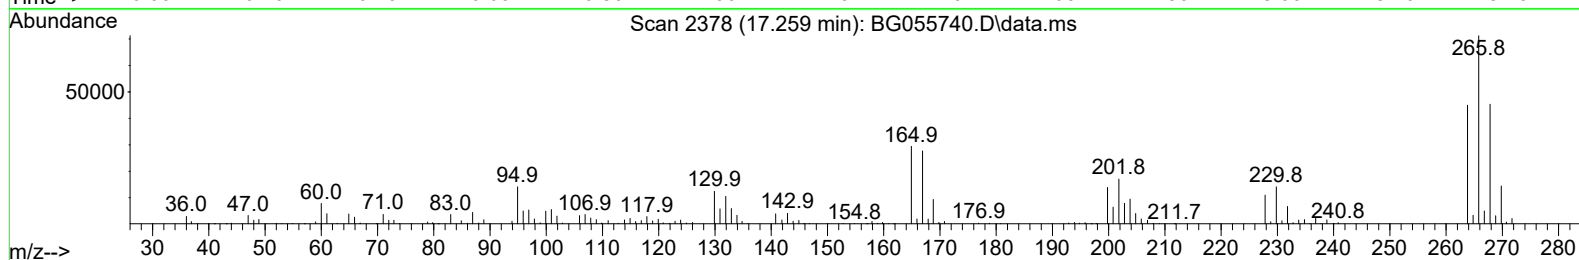


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG112222\  
Data File : BG055740.D  
Acq On : 22 Nov 2022 15:04  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 23 06:54:25 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG111622.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Nov 23 01:35:20 2022  
Response via : Initial Calibration

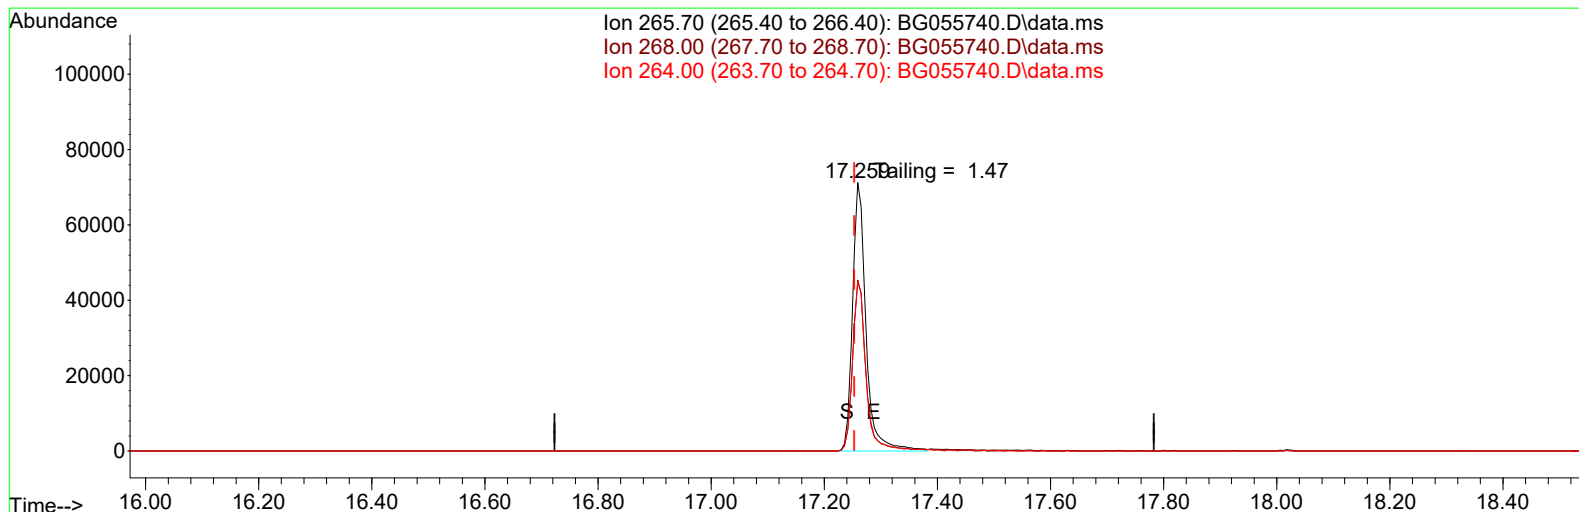

TIC: BG055740.D\data.ms

**(70) Pentachlorophenol (C)**




17.259min (+ 0.006) 22726.31 ng

response 118031

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 64.00  | 63.69  |
| 264.00 | 61.90  | 63.15  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG112222\  
Data File : BG055740.D  
Acq On : 22 Nov 2022 15:04  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 23 06:54:25 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG111622.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Nov 23 01:35:20 2022  
Response via : Initial Calibration

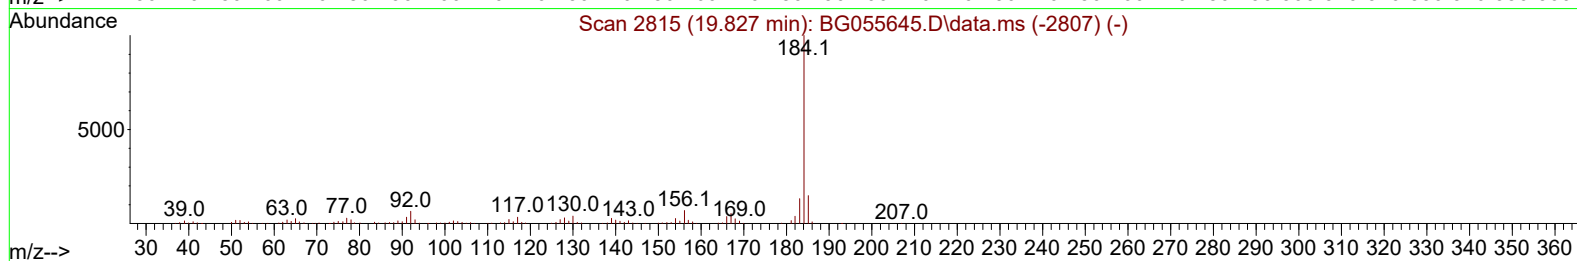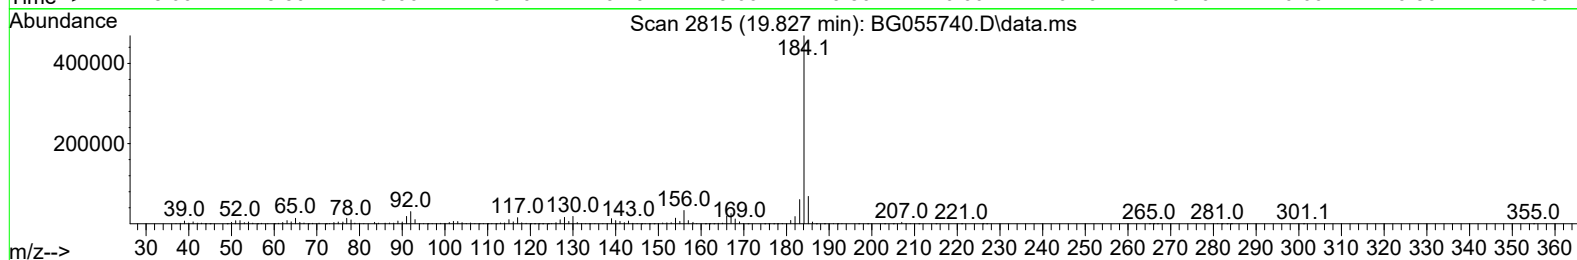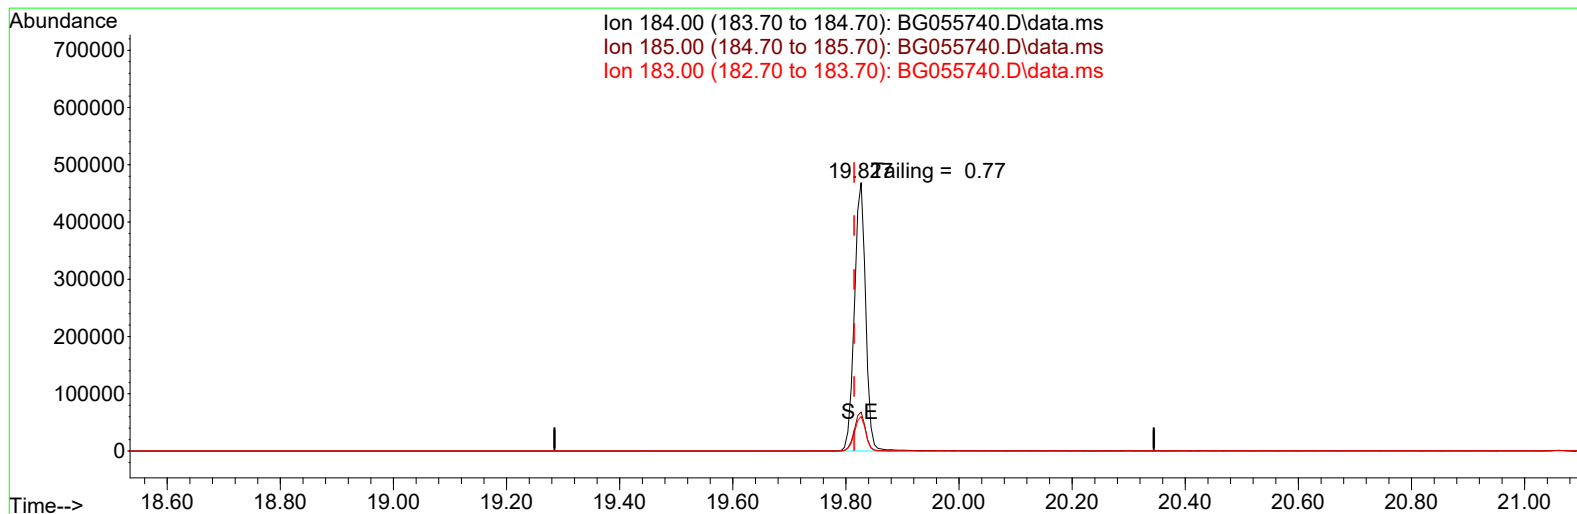

TIC: BG055740.D\data.ms

**(77) Benzidine****19.827min (+ 0.012) 78321.64 ng****response 650483**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.80  | 14.56  |
| 183.00 | 13.20  | 12.88  |
| 0.00   | 0.00   | 0.00   |