


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112222\
Data File : BG055732.D
Acq On : 22 Nov 2022 9:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 23 01:35:20 2022

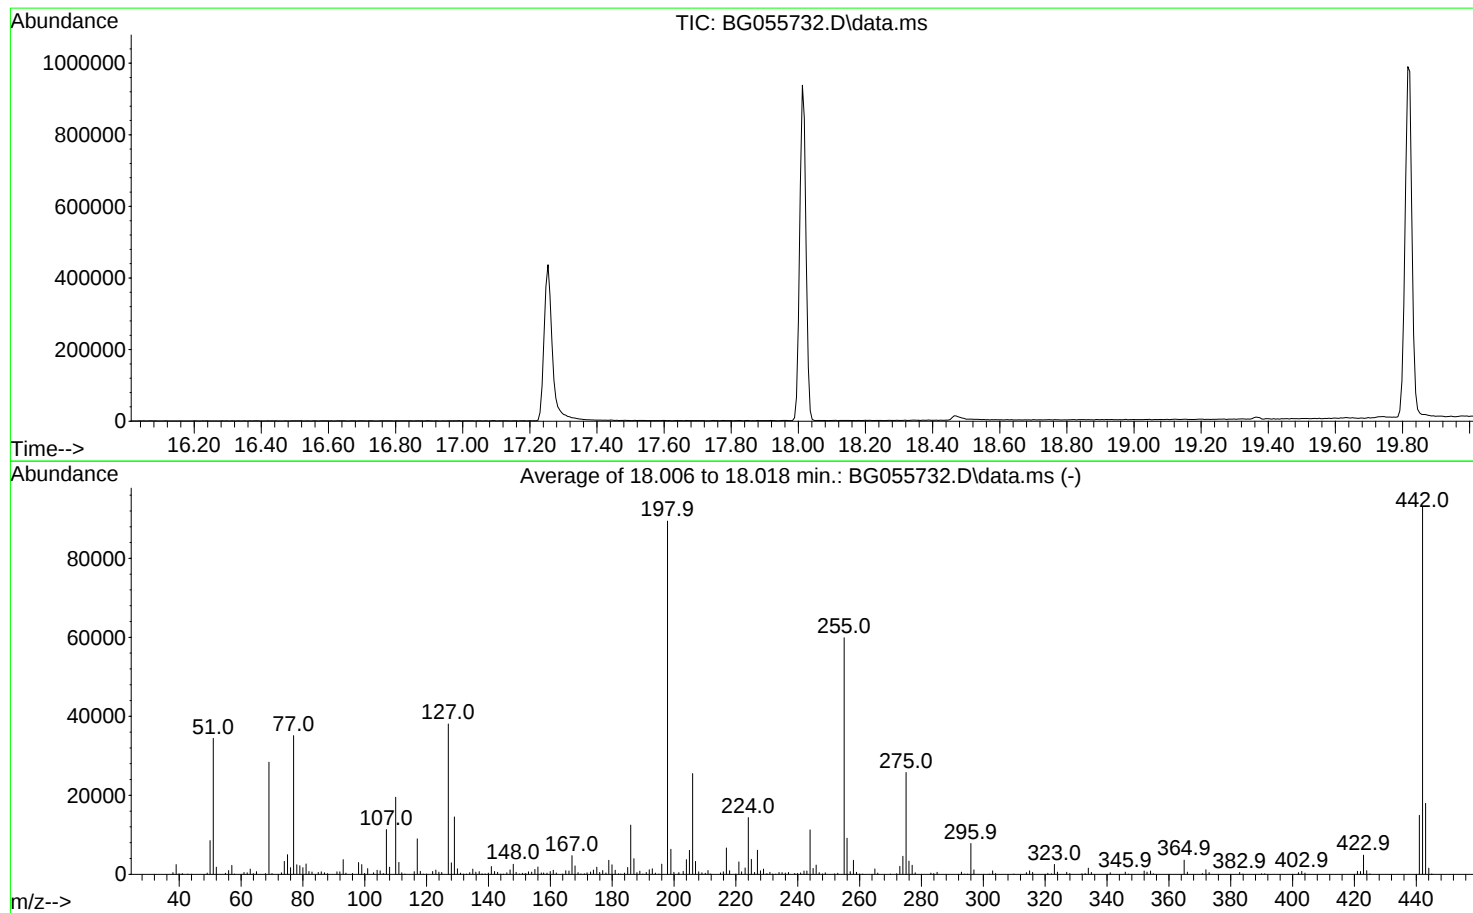




AutoFind: Scans 2505, 2506, 2507; Background Corrected with Scan 2499

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.5	34416	PASS
68	69	0.00	2	0.6	178	PASS
69	198	0.00	100	31.7	28371	PASS
70	69	0.00	2	0.7	191	PASS
127	198	10	80	42.6	38075	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	89459	PASS
199	198	5	9	7.1	6339	PASS
275	198	10	60	28.8	25781	PASS
365	198	1	100	4.0	3571	PASS
441	198	0.01	100	16.7	14927	PASS
442	442	50	100	100.0	93147	PASS
443	442	15	24	19.3	17954	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112222\
Data File : BG055732.D
Acq On : 22 Nov 2022 9:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 23 06:52:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 23 01:35:20 2022
Response via : Initial Calibration

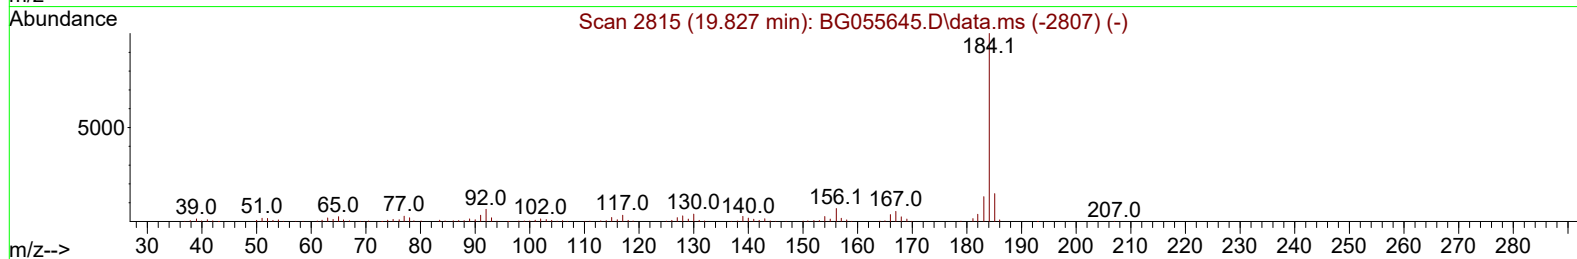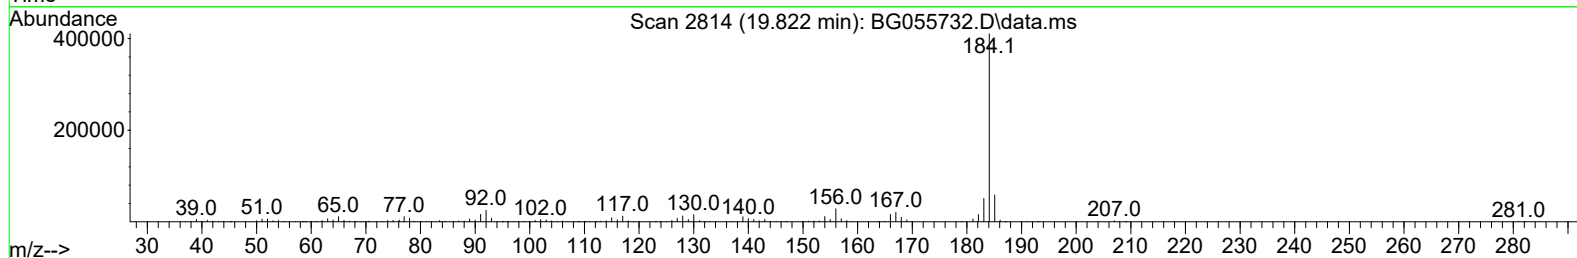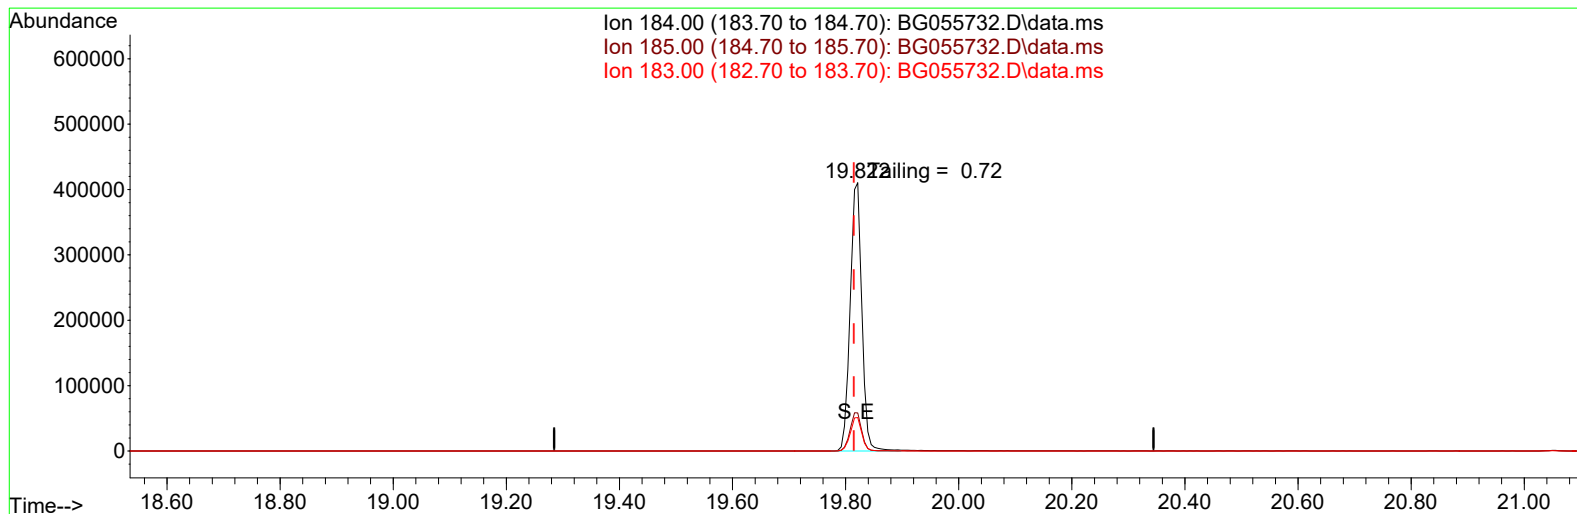

TIC: BG055732.D\data.ms

(77) Benzidine

19.822min (+ 0.007) 118403.87 ng

response 594409

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.24
183.00	13.20	12.45
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/22/2022	BNA_G	<u>BG055732.D</u>
Compound Name	Response	Retention Time
DDT	290939	21.05
DDD	6974	20.603
DDE	419	20.098
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7393	298332	2.48

Instrument :
BNA_G
ClientSampleId :
DFTPP