


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112222\
 Data File : BG055740.D
 Acq On : 22 Nov 2022 15:04
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 23 01:35:20 2022

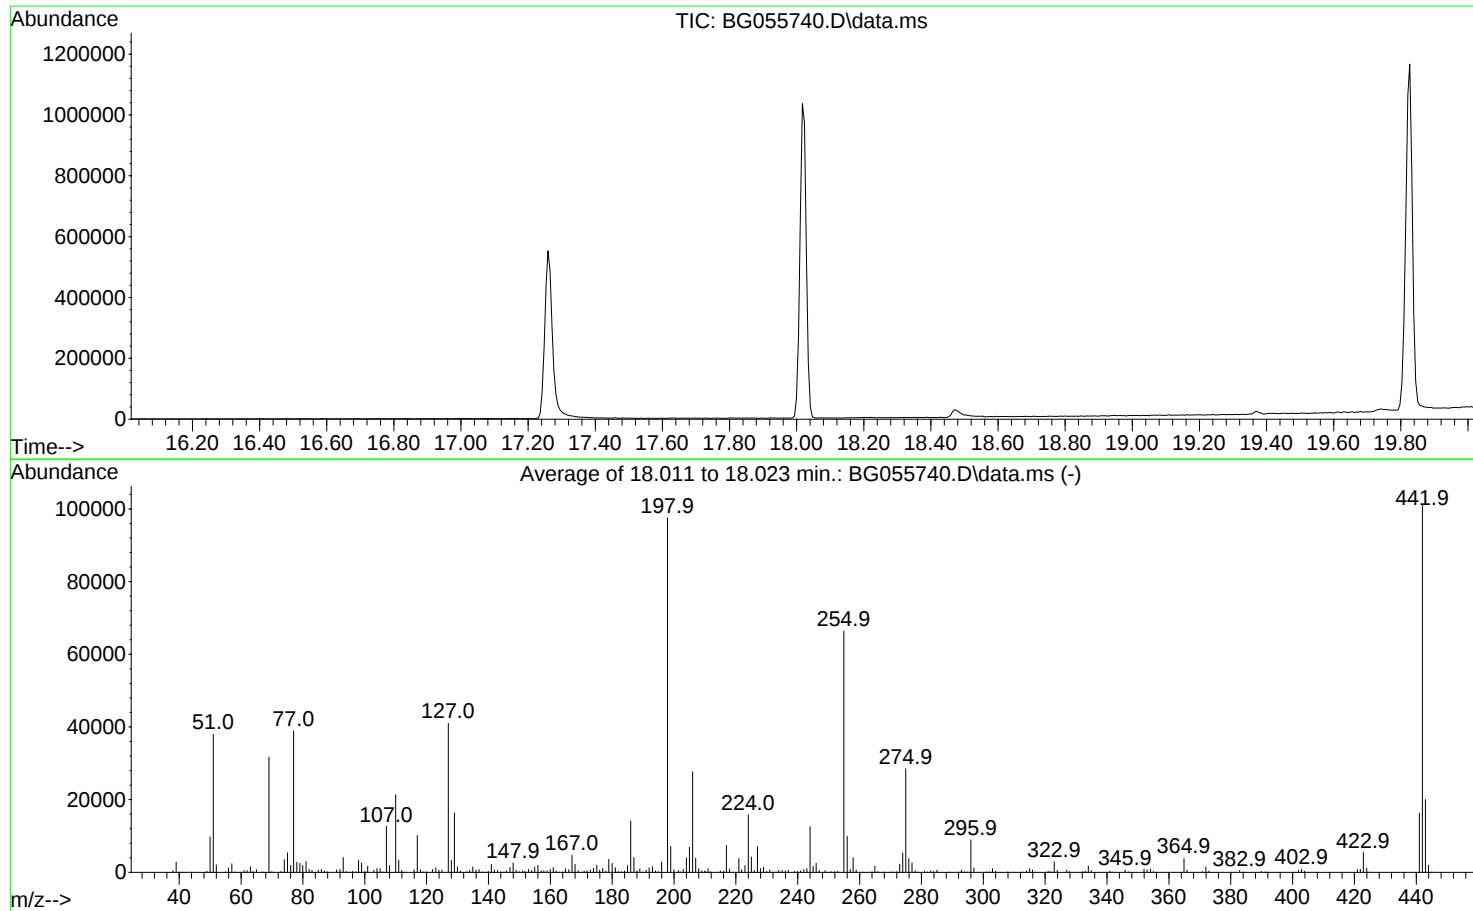




AutoFind: Scans 2506, 2507, 2508; Background Corrected with Scan 2499

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.9	37976	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	32.5	31686	PASS
70	69	0.00	2	0.7	207	PASS
127	198	10	80	42.1	41019	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	97525	PASS
199	198	5	9	7.3	7136	PASS
275	198	10	60	29.2	28483	PASS
365	198	1	100	3.9	3832	PASS
441	198	0.01	100	16.7	16296	PASS
442	442	50	100	100.0	101243	PASS
443	442	15	24	19.8	20021	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112222\
Data File : BG055740.D
Acq On : 22 Nov 2022 15:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 23 06:54:25 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 23 01:35:20 2022
Response via : Initial Calibration

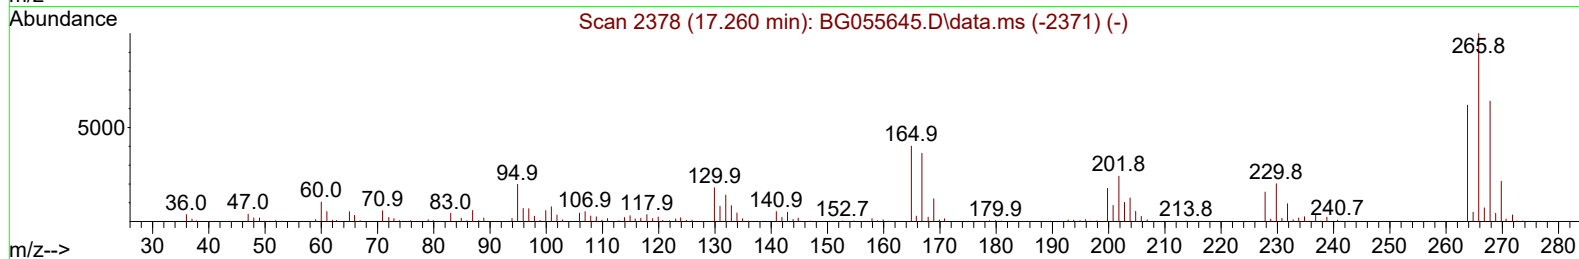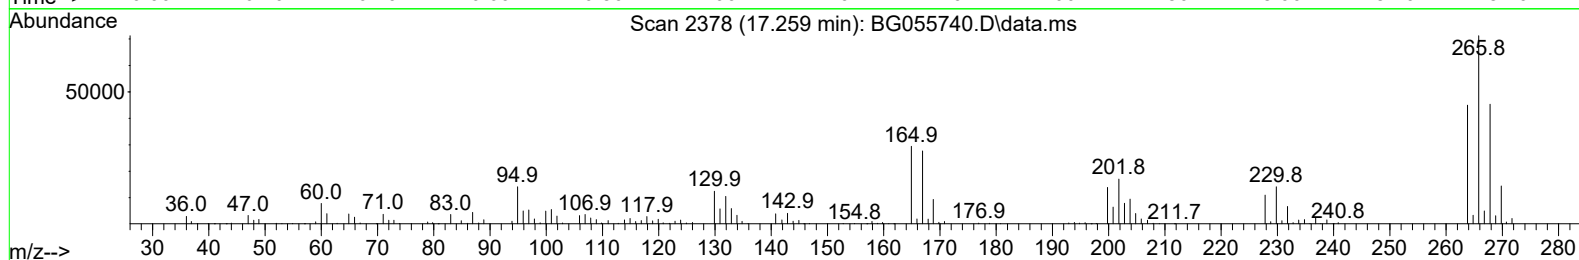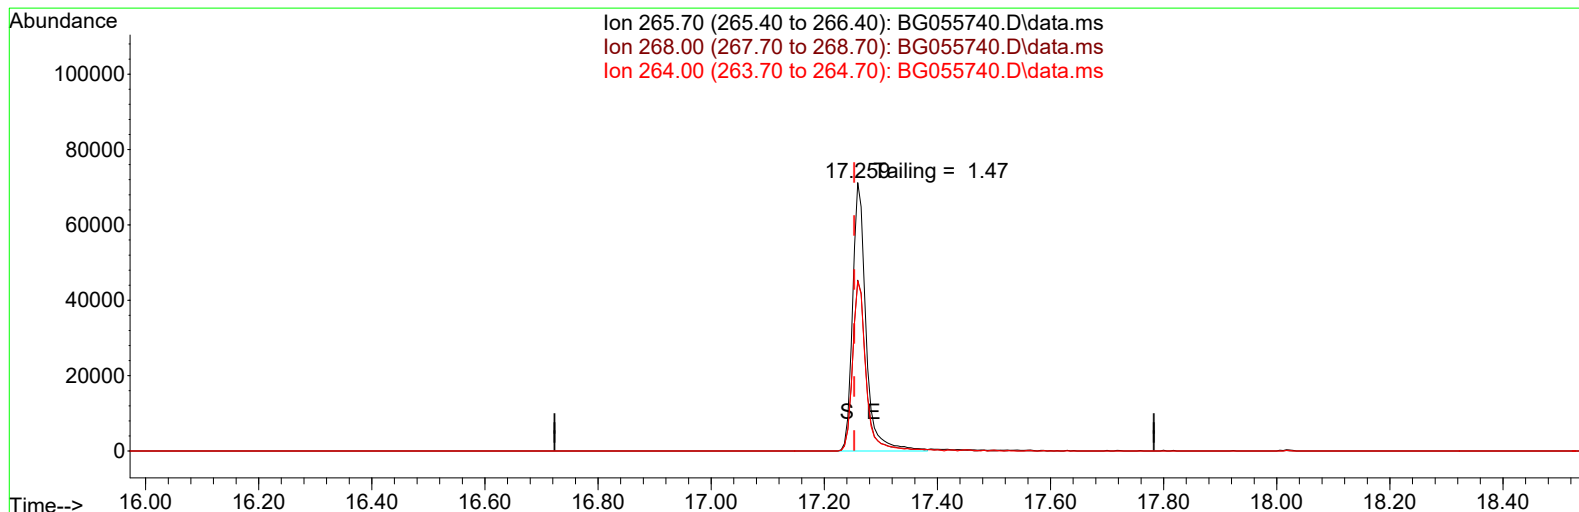

TIC: BG055740.D\data.ms

(70) Pentachlorophenol (C)

17.259min (+ 0.006) 22726.31 ng




response 118031

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	63.69
264.00	61.90	63.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112222\
Data File : BG055740.D
Acq On : 22 Nov 2022 15:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 23 06:54:25 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 23 01:35:20 2022
Response via : Initial Calibration

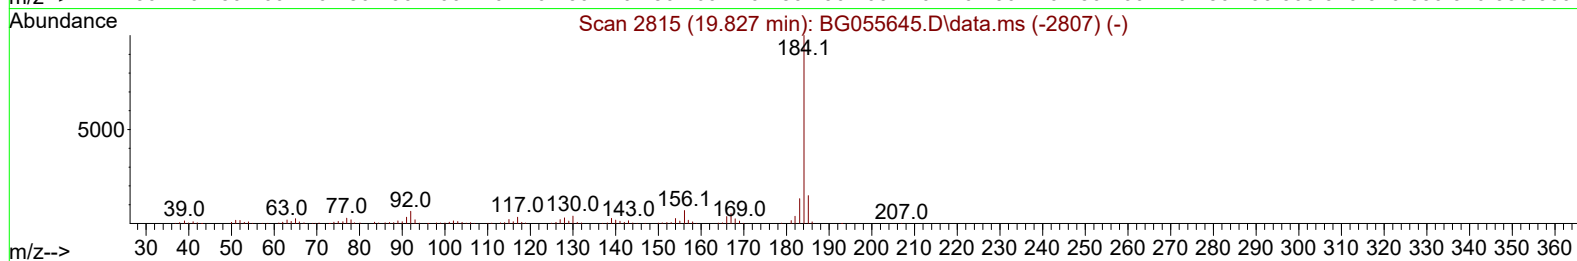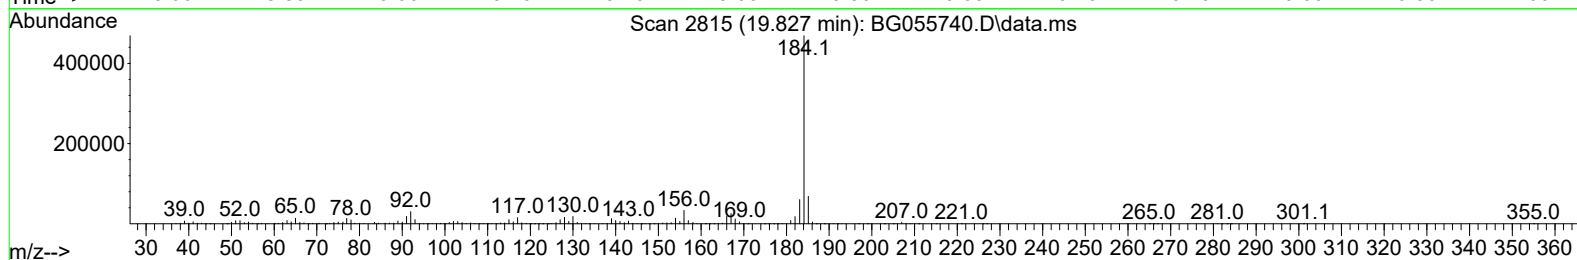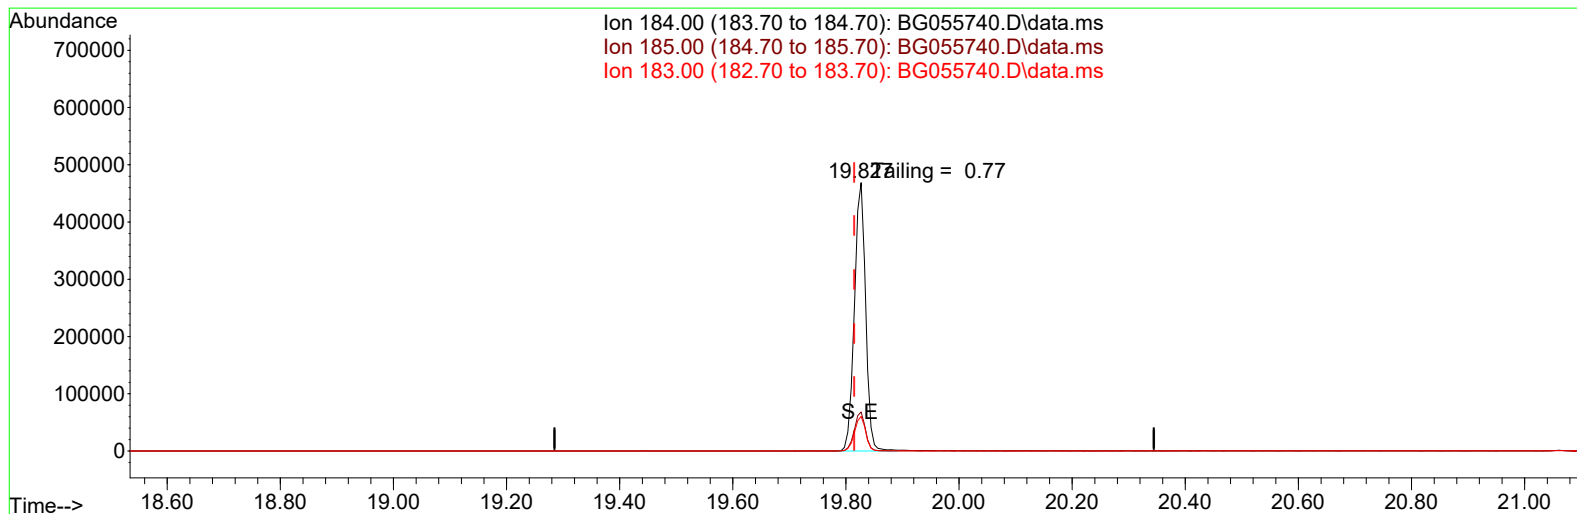

TIC: BG055740.D\data.ms

(77) Benzidine

19.827min (+ 0.012) 78321.64 ng

response 650483

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.56
183.00	13.20	12.88
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/22/2022	BNA_G	BG055740.D
Compound Name	Response	Retention Time
DDT	316123	21.061
DDD	6372	20.661
DDE	509	20.109
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6881	323004	2.13

Instrument :
BNA_G
ClientSampleId :
DFTPP