




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112224\
Data File : BG063526.D
Acq On : 22 Nov 2024 19:00
Operator : RC/JU
Sample : P4943-07
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0TG0

Manual IntegrationsAPPROVED

Quant Time: Nov 22 22:22:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 20 14:52:38 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/25/2024
Supervised By :mohammad ahmed 11/27/2024

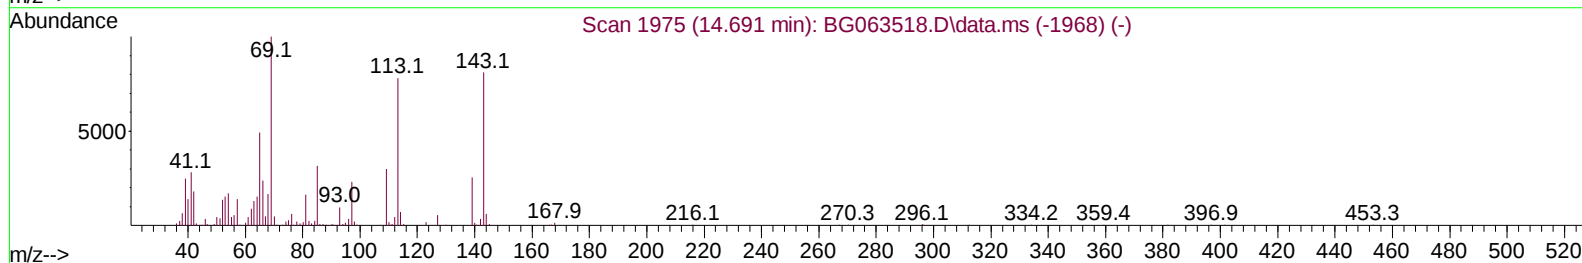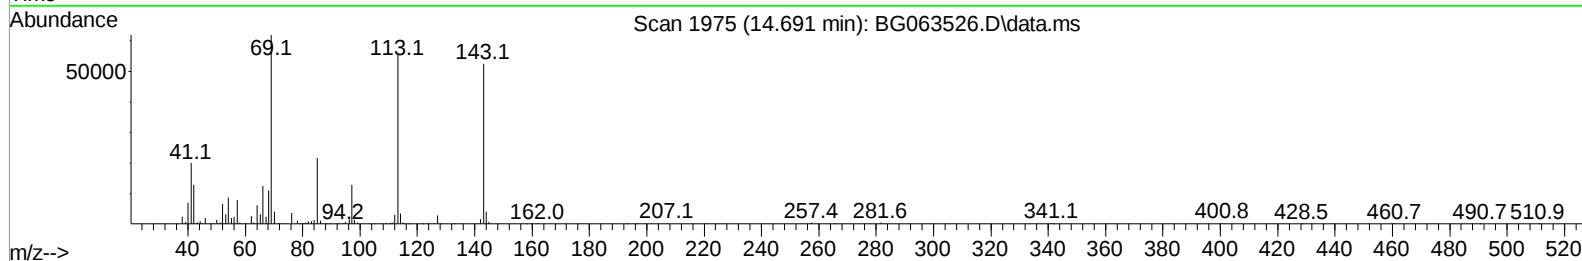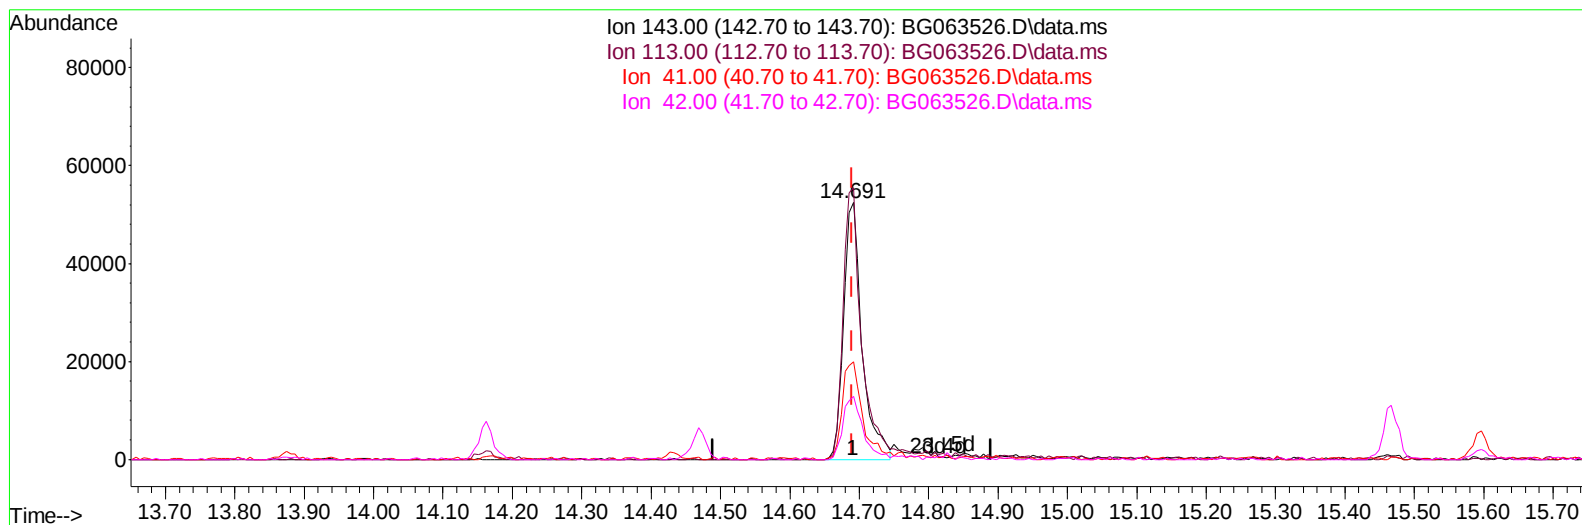

TIC: BG063526.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.691min (+ 0.002) 30.29 ng/u1

response 97563

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	103.10	105.67
41.00	38.80	38.08
42.00	26.30	24.61




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112224\
Data File : BG063526.D
Acq On : 22 Nov 2024 19:00
Operator : RC/JU
Sample : P4943-07
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0TG0

Manual IntegrationsAPPROVED

Quant Time: Nov 22 22:22:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 20 14:52:38 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/25/2024
Supervised By :mohammad ahmed 11/27/2024

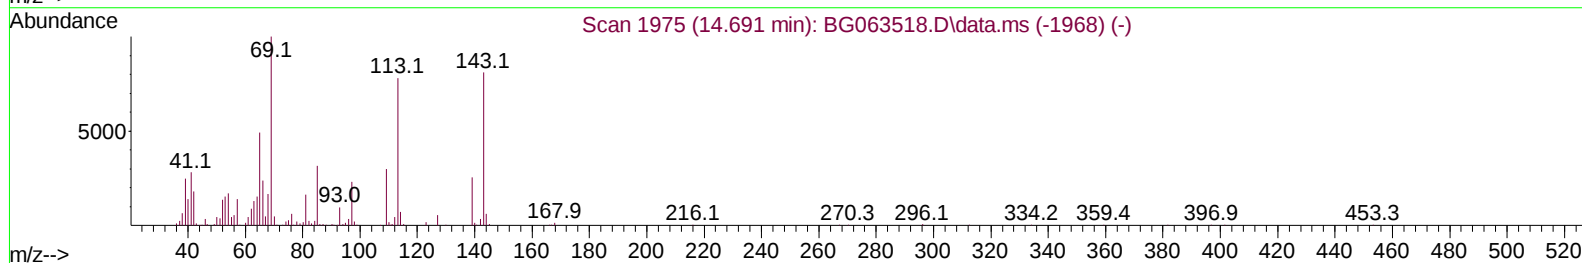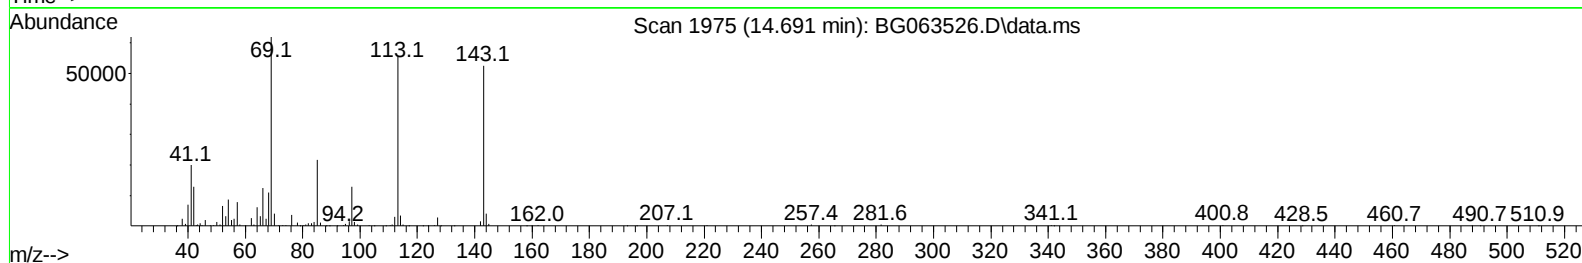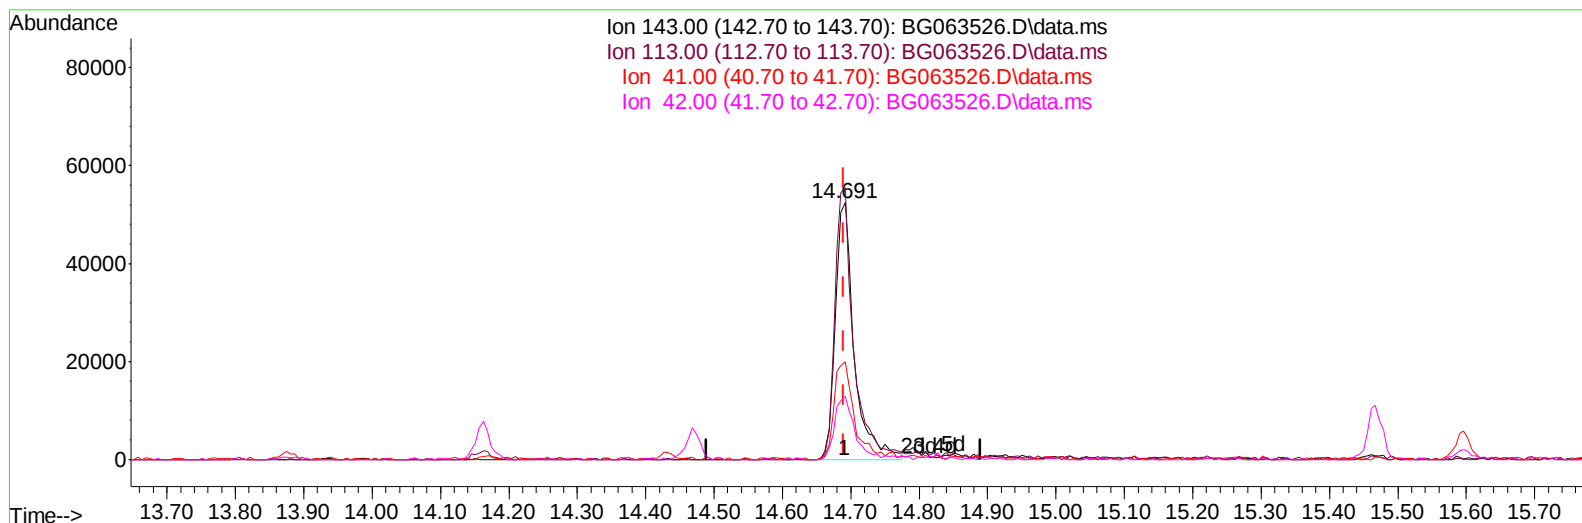

TIC: BG063526.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.691min (+ 0.002) 31.30 ng/ul m

response 100818

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	103.10	105.67
41.00	38.80	38.08
42.00	26.30	24.61

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112224\
 Data File : BG063526.D
 Acq On : 22 Nov 2024 19:00
 Operator : RC/JU
 Sample : P4943-07
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0TG0

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/25/2024
 Supervised By :mohammad ahmed 11/27/2024

Quant Time: Nov 22 22:23:29 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 20 14:52:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.829	152	101583	20.000	ng/ul	0.00
20) Naphthalene-d8	10.620	136	405417	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.468	164	319282	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.224	188	787918	20.000	ng/ul	0.00
79) Chrysene-d12	21.483	240	852723	20.000	ng/ul	0.00
88) Perylene-d12	24.527	264	929552	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	14300	5.556	ng/uL	0.00
4) Pyridine-d5	3.704	84	32517	4.031	ng/ul	0.00
7) Phenol-d5	7.006	99	254491	30.461	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.159	67	171662	32.036	ng/ul	0.00
11) 2-Chlorophenol-d4	7.365	132	183803	31.044	ng/ul	0.00
15) 4-Methylphenol-d8	8.540	113	216406	30.997	ng/ul	0.00
21) Nitrobenzene-d5	8.986	128	99230	34.083	ng/ul	0.00
24) 2-Nitrophenol-d4	9.709	143	121849	33.879	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.250	165	220798	32.163	ng/ul	0.00
31) 4-Chloroaniline-d4	10.761	131	277684	31.980	ng/ul	0.00
46) Dimethylphthalate-d6	13.875	166	795624	36.708	ng/ul	0.00
49) Acenaphthylene-d8	14.163	160	874525	35.382	ng/ul	0.00
54) 4-Nitrophenol-d4	14.691	143	100818m	31.305	ng/ul	0.00
60) Fluorene-d10	15.467	176	722919	36.707	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.596	200	135739	30.643	ng/ul	0.00
73) Anthracene-d10	17.324	188	1247961	36.457	ng/ul	0.00
81) Pyrene-d10	19.627	212	1619144	37.880	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.321	264	1633290	36.226	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112224\
Data File : BG063526.D
Acq On : 22 Nov 2024 19:00
Operator : RC/JU
Sample : P4943-07
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0TG0

Manual IntegrationsAPPROVED

Quant Time: Nov 22 22:23:29 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 20 14:52:38 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/25/2024
Supervised By :mohammad ahmed 11/27/2024

