

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112224\
 Data File : BG063512.D
 Acq On : 22 Nov 2024 9:44
 Operator : RC/JU
 Sample : PB165168BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK168

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063512.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.299	32	36	44	rVB2	29864	51995	1.36%	0.158%
2	3.699	100	104	119	rBV	348347	612500	15.97%	1.862%
3	4.040	159	162	167	rBV2	8642	10638	0.28%	0.032%
4	6.707	613	616	619	rVB4	6628	6287	0.16%	0.019%
5	7.007	656	667	678	rBV	407302	715845	18.66%	2.177%
6	7.159	685	693	704	rBV	317461	531907	13.87%	1.617%
7	7.289	712	715	718	rBV4	3682	6075	0.16%	0.018%
8	7.365	721	728	738	rBV2	419425	712143	18.57%	2.165%
9	7.829	799	807	816	rBV	337477	566370	14.77%	1.722%
10	7.917	820	822	825	rVB3	4382	5127	0.13%	0.016%
11	8.000	834	836	839	rVB2	6263	5677	0.15%	0.017%
12	8.540	921	928	938	rBV	506422	888551	23.17%	2.702%
13	8.916	989	992	994	rBV2	4732	5114	0.13%	0.016%
14	8.987	997	1004	1015	rVV	394913	708763	18.48%	2.155%
15	9.416	1076	1077	1082	rVB3	5107	5859	0.15%	0.018%
16	9.609	1106	1110	1114	rBV	3320	5534	0.14%	0.017%
17	9.703	1119	1126	1135	rBV	342816	630705	16.44%	1.918%
18	10.250	1212	1219	1231	rBV	491369	918528	23.95%	2.793%
19	10.356	1234	1237	1240	rVB2	5068	6625	0.17%	0.020%
20	10.620	1273	1282	1291	rBV	448990	780770	20.36%	2.374%
21	10.755	1298	1305	1315	rBV	455041	872239	22.74%	2.652%
22	11.913	1498	1502	1506	rVB2	5082	5878	0.15%	0.018%
23	12.230	1551	1556	1557	rBV3	7145	9746	0.25%	0.030%
24	12.412	1584	1587	1590	rBV	3377	5656	0.15%	0.017%
25	13.575	1782	1785	1789	rVB3	4634	6246	0.16%	0.019%
26	13.611	1789	1791	1794	rBV2	5678	5412	0.14%	0.016%
27	13.875	1830	1836	1846	rVB	989862	1487283	38.78%	4.522%
28	14.163	1878	1885	1900	rBV2	1110316	1710058	44.59%	5.200%
29	14.474	1931	1938	1945	rBV	749884	1183443	30.86%	3.598%
30	14.686	1965	1974	1991	rBV	290972	631568	16.47%	1.920%
31	15.279	2072	2075	2080	rBV3	4567	5697	0.15%	0.017%
32	15.467	2099	2107	2119	rBV	1488650	2282463	59.51%	6.940%
33	15.597	2123	2129	2138	rBV	408716	649473	16.93%	1.975%
34	15.702	2145	2147	2152	rVB5	7968	11090	0.29%	0.034%
35	15.855	2170	2173	2175	rBV2	4690	5819	0.15%	0.018%
36	16.137	2218	2221	2223	rBV3	5002	6025	0.16%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112224\
Data File : BG063512.D
Acq On : 22 Nov 2024 9:44
Operator : RC/JU
Sample : PB165168BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK168

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
Title : SVOA CALIBRATION

37	16.255	2238	2241	2242	rBV	5510	5169	0.13%	0.016%
38	16.537	2285	2289	2291	rVB2	4933	5908	0.15%	0.018%
39	16.607	2299	2301	2304	rBV2	6423	7473	0.19%	0.023%
40	16.672	2309	2312	2315	rBV2	4553	6206	0.16%	0.019%
41	17.224	2399	2406	2415	rBV	1127103	1665979	43.44%	5.066%
42	17.324	2416	2423	2431	rBV2	1849755	2781227	72.51%	8.457%
43	17.900	2518	2521	2524	rVB2	8757	10099	0.26%	0.031%
44	18.182	2566	2569	2572	rBV	3920	6169	0.16%	0.019%
45	18.728	2661	2662	2665	rBV2	5705	5742	0.15%	0.017%
46	18.987	2705	2706	2711	rBV3	4485	5431	0.14%	0.017%
47	19.186	2736	2740	2745	rBV3	28087	43376	1.13%	0.132%
48	19.263	2749	2753	2758	rVB3	23276	33376	0.87%	0.101%
49	19.557	2802	2803	2808	rBV4	9591	10126	0.26%	0.031%
50	19.627	2809	2815	2826	rVV	2664924	3739076	97.49%	11.369%
51	19.774	2836	2840	2841	rBV4	6668	6801	0.18%	0.021%
52	19.974	2873	2874	2880	rBV5	5614	8871	0.23%	0.027%
53	20.738	3002	3004	3006	rBV2	9026	5419	0.14%	0.016%
54	21.484	3125	3131	3142	rBV2	1310992	2217527	57.82%	6.743%
55	22.606	3318	3322	3327	rVB4	75224	111321	2.90%	0.338%
56	22.900	3370	3372	3381	rVB9	25258	40696	1.06%	0.124%
57	24.322	3604	3614	3626	rBV	1494123	3835466	100.00%	11.662%
58	24.533	3641	3650	3662	rVB2	833824	2277319	59.38%	6.924%
59	26.642	4007	4009	4010	rBV2	11976	6437	0.17%	0.020%




Sum of corrected areas: 32888323

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112224\
Data File : BG063512.D
Acq On : 22 Nov 2024 9:44
Operator : RC/JU
Sample : PB165168BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK168

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

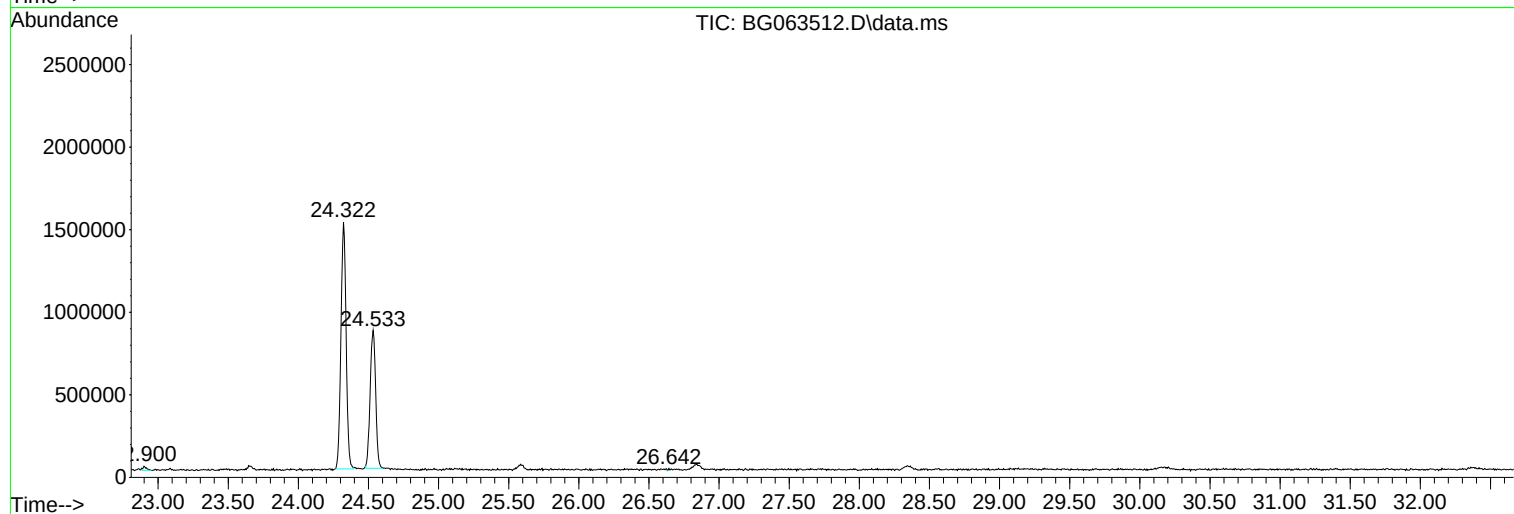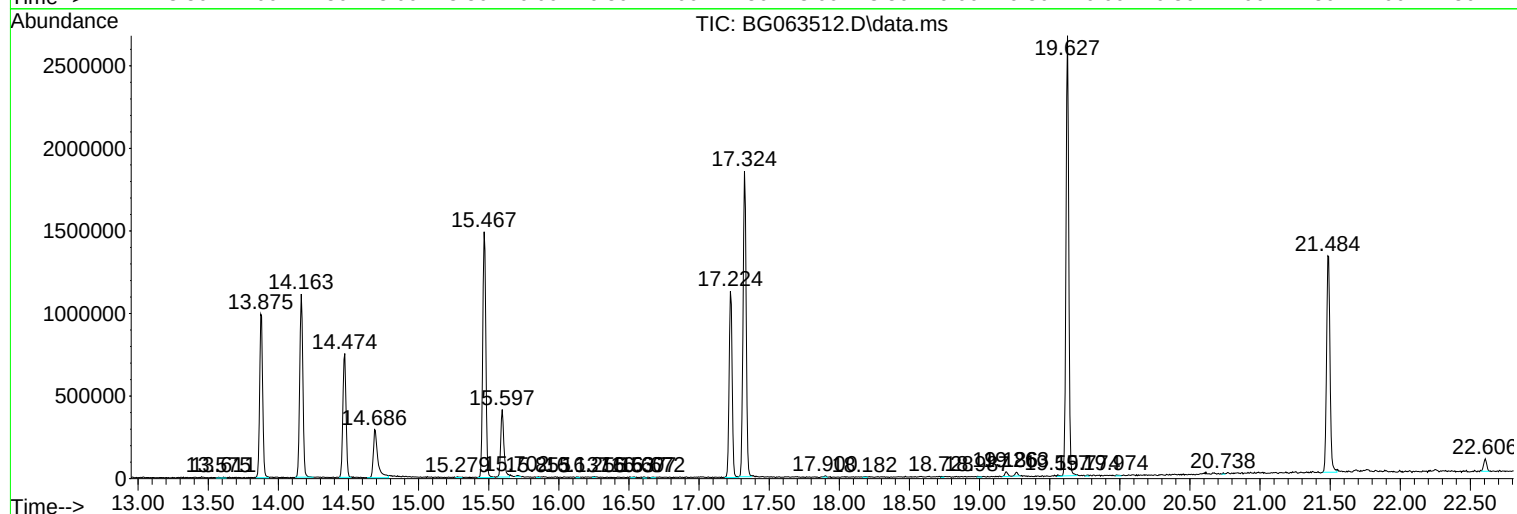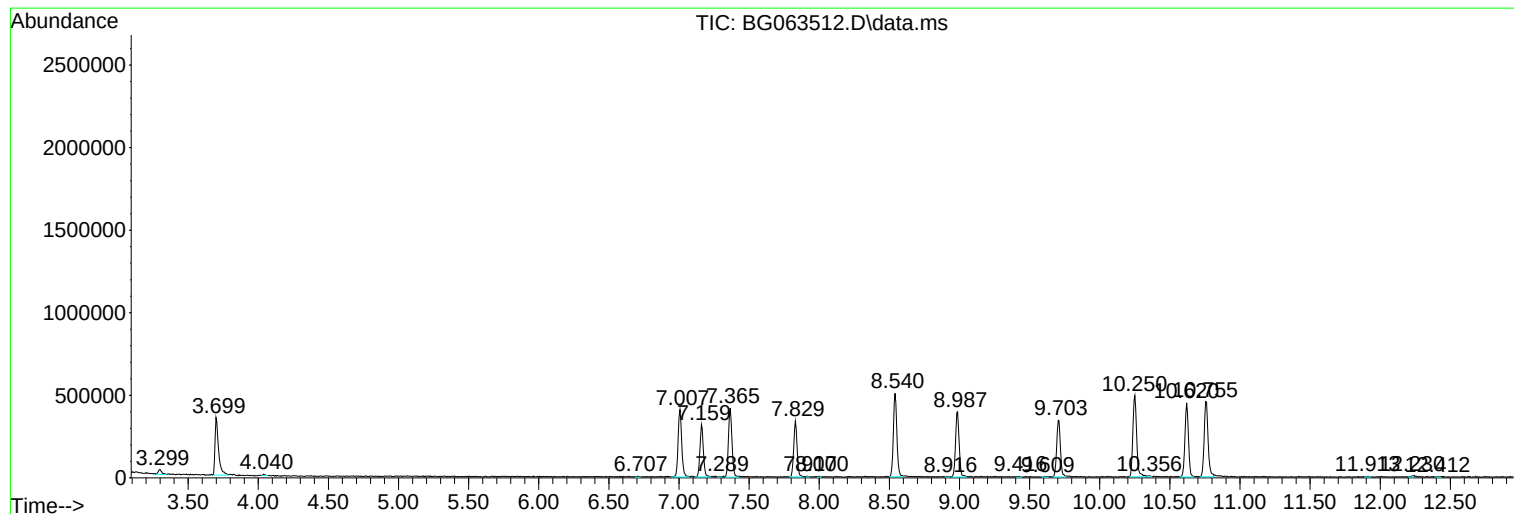

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112224\
Data File : BG063512.D
Acq On : 22 Nov 2024 9:44
Operator : RC/JU
Sample : PB165168BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK168

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112224\
Data File : BG063512.D
Acq On : 22 Nov 2024 9:44
Operator : RC/JU
Sample : PB165168BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK168

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------