

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112224\
 Data File : BG063513.D
 Acq On : 22 Nov 2024 10:22
 Operator : RC/JU
 Sample : PB165149BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK149

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063513.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.293	32	35	44	rVB3	27326	41274	1.08%	0.129%
2	3.605	86	88	91	rVB2	7170	6403	0.17%	0.020%
3	3.704	100	105	119	rVB	319548	544297	14.30%	1.705%
4	4.033	158	161	164	rBV3	7450	9698	0.25%	0.030%
5	4.480	233	237	239	rBV3	4910	6976	0.18%	0.022%
6	4.903	305	309	312	rBV4	3250	5491	0.14%	0.017%
7	5.408	391	395	398	rBV4	5148	5508	0.14%	0.017%
8	5.720	442	448	449	rBV3	4218	5985	0.16%	0.019%
9	7.006	659	667	678	rBV	409639	717352	18.84%	2.247%
10	7.159	687	693	702	rVB	315352	514916	13.53%	1.613%
11	7.312	714	719	722	rBV3	5409	6524	0.17%	0.020%
12	7.365	722	728	739	rVB	412900	694183	18.23%	2.174%
13	7.547	755	759	762	rVB3	4245	5204	0.14%	0.016%
14	7.829	801	807	814	rVB2	308004	523117	13.74%	1.639%
15	8.540	920	928	936	rBV2	523749	887012	23.30%	2.778%
16	8.851	976	981	983	rBV	6954	9822	0.26%	0.031%
17	8.986	994	1004	1012	rBV	400377	714665	18.77%	2.239%
18	9.415	1073	1077	1083	rVB5	5039	7853	0.21%	0.025%
19	9.703	1118	1126	1137	rBV	340275	633451	16.64%	1.984%
20	9.891	1157	1158	1161	rBV2	6824	5656	0.15%	0.018%
21	10.068	1185	1188	1193	rVB2	3932	5423	0.14%	0.017%
22	10.250	1210	1219	1228	rBV	505052	909094	23.88%	2.848%
23	10.620	1275	1282	1292	rVB	427258	737352	19.37%	2.310%
24	10.761	1296	1306	1318	rBV	447911	893560	23.47%	2.799%
25	12.224	1549	1555	1558	rBV4	9679	17312	0.45%	0.054%
26	12.547	1605	1610	1613	rBV	3236	5067	0.13%	0.016%
27	13.610	1789	1791	1796	rBV2	5195	6748	0.18%	0.021%
28	13.875	1829	1836	1846	rBV	990336	1467032	38.54%	4.595%
29	14.163	1878	1885	1896	rBV	1099261	1727355	45.37%	5.411%
30	14.474	1931	1938	1946	rVB	680981	1085914	28.52%	3.401%
31	14.692	1968	1975	1987	rBV	283031	594209	15.61%	1.861%
32	15.467	2101	2107	2118	rBV	1537010	2215378	58.19%	6.939%
33	15.596	2123	2129	2136	rBV	398173	634296	16.66%	1.987%
34	15.702	2146	2147	2155	rVB5	12731	21911	0.58%	0.069%
35	16.254	2237	2241	2243	rVV4	5510	6858	0.18%	0.021%
36	16.284	2243	2246	2252	rVB2	4267	6166	0.16%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112224\
 Data File : BG063513.D
 Acq On : 22 Nov 2024 10:22
 Operator : RC/JU
 Sample : PB165149BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK149

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
 Title : SVOA CALIBRATION

37	16.619	2300	2303	2306	rVB2	5159	5160	0.14%	0.016%
38	16.842	2336	2341	2342	rBV2	6483	8250	0.22%	0.026%
39	16.901	2348	2351	2354	rVB3	5630	5808	0.15%	0.018%
40	17.224	2399	2406	2414	rBV	1043216	1513833	39.76%	4.742%
41	17.324	2416	2423	2438	rVV2	1828551	2732438	71.77%	8.559%
42	17.430	2440	2441	2446	rVB2	7623	6978	0.18%	0.022%
43	17.894	2519	2520	2523	rBV	8946	5728	0.15%	0.018%
44	17.982	2531	2535	2536	rBV4	4724	5156	0.14%	0.016%
45	18.405	2604	2607	2609	rBV3	5484	5032	0.13%	0.016%
46	18.487	2617	2621	2623	rBV3	4159	5024	0.13%	0.016%
47	18.992	2704	2707	2712	rVB4	5253	8187	0.22%	0.026%
48	19.192	2735	2741	2745	rBV4	30011	45135	1.19%	0.141%
49	19.263	2749	2753	2757	rBV2	26318	37794	0.99%	0.118%
50	19.627	2807	2815	2829	rBV	2611323	3669056	96.38%	11.492%
51	19.733	2831	2833	2837	rVB4	6681	7450	0.20%	0.023%
52	19.844	2848	2852	2854	rBV3	5092	6065	0.16%	0.019%
53	20.044	2883	2886	2888	rBV4	5190	5765	0.15%	0.018%
54	21.489	3125	3132	3142	rBV	1202848	2000391	52.55%	6.266%
55	22.606	3318	3322	3330	rVB4	69034	123278	3.24%	0.386%
56	23.658	3496	3501	3508	rVB10	35182	70780	1.86%	0.222%
57	24.321	3604	3614	3627	rBV	1467908	3806953	100.00%	11.924%
58	24.527	3640	3649	3663	rVB2	809951	2172460	57.07%	6.805%




Sum of corrected areas: 31925783

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112224\
Data File : BG063513.D
Acq On : 22 Nov 2024 10:22
Operator : RC/JU
Sample : PB165149BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK149

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

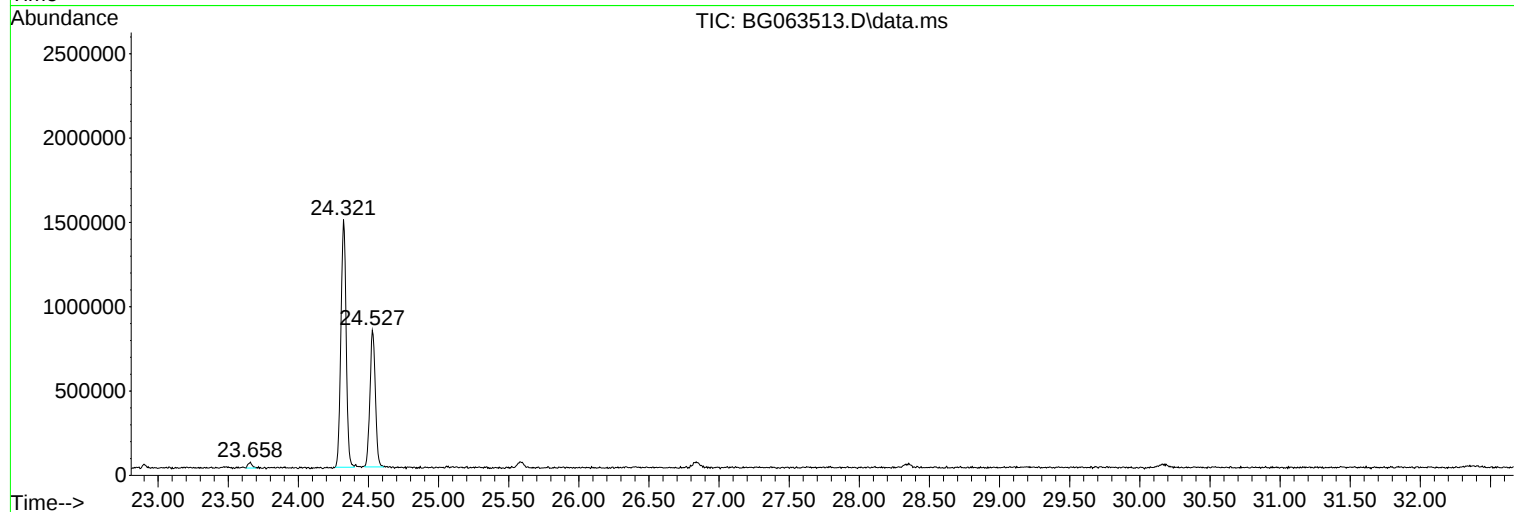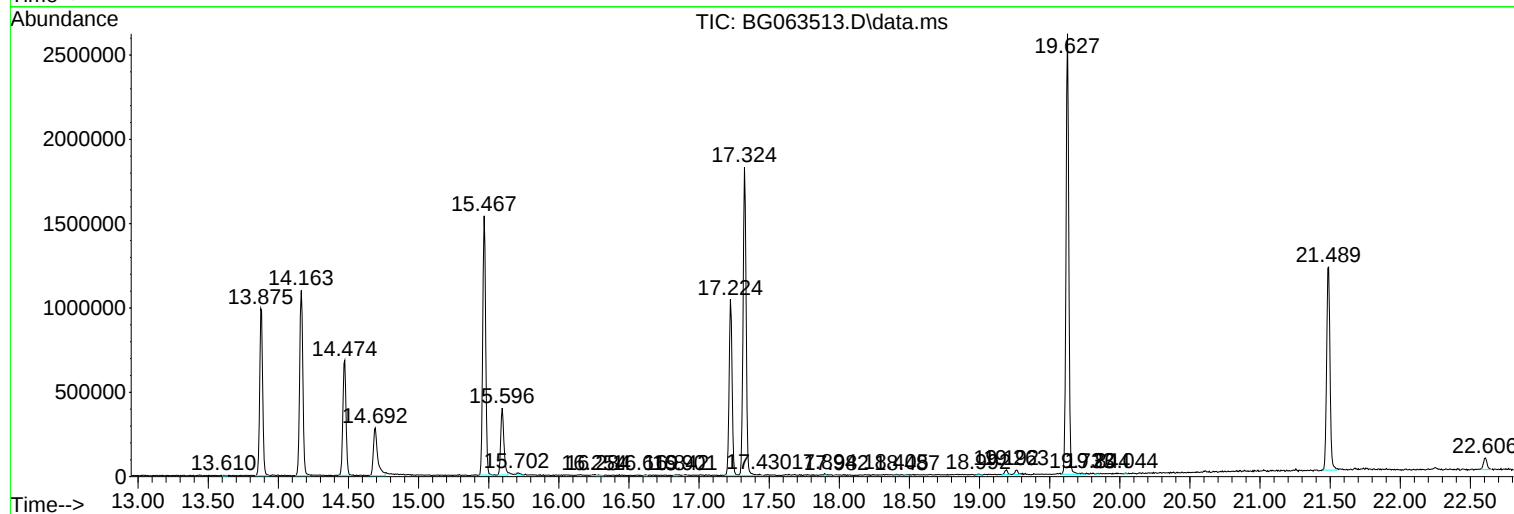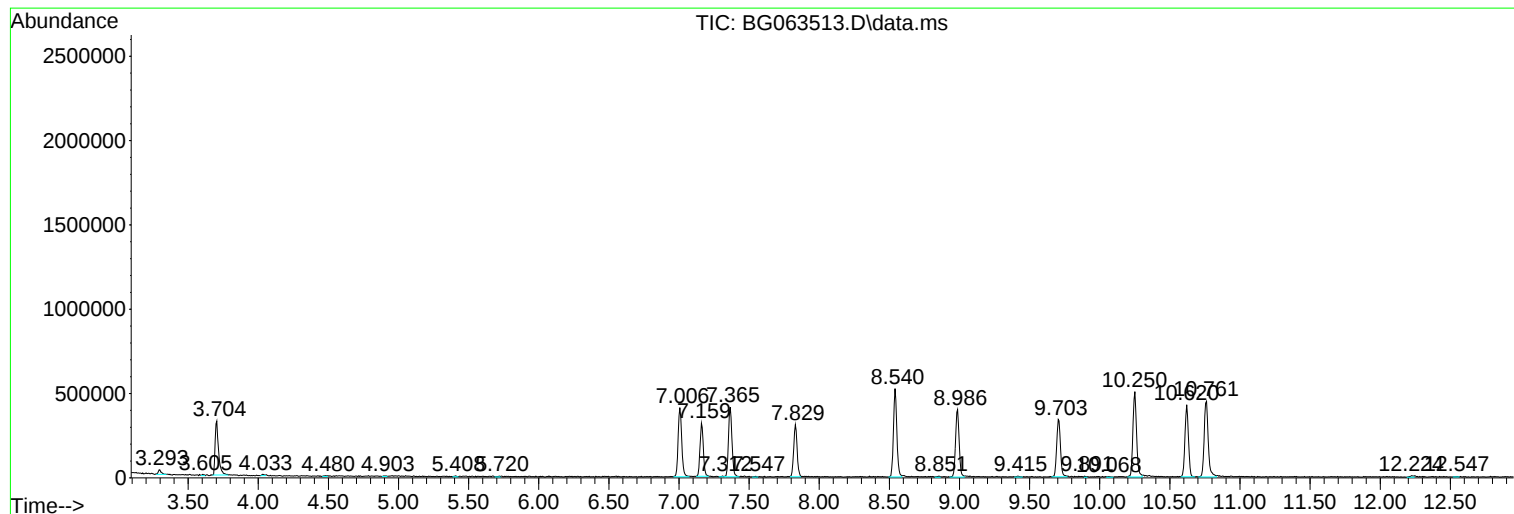

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112224\
Data File : BG063513.D
Acq On : 22 Nov 2024 10:22
Operator : RC/JU
Sample : PB165149BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK149

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112224\
Data File : BG063513.D
Acq On : 22 Nov 2024 10:22
Operator : RC/JU
Sample : PB165149BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK149

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------