

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112224\
 Data File : BG063514.D
 Acq On : 22 Nov 2024 11:00
 Operator : RC/JU
 Sample : PB165173BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK173

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063514.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.302	33	36	45	rVB2	30647	51542	1.35%	0.152%
2	3.502	68	70	72	rBV	6486	5232	0.14%	0.015%
3	3.702	100	104	117	rBV	331249	585627	15.33%	1.732%
4	4.037	159	161	166	rVB4	10714	16826	0.44%	0.050%
5	5.206	357	360	364	rVB5	4674	5092	0.13%	0.015%
6	5.382	389	390	395	rVB4	5655	5141	0.13%	0.015%
7	5.705	439	445	448	rBV4	3120	5879	0.15%	0.017%
8	6.269	539	541	546	rVB3	4365	5352	0.14%	0.016%
9	6.510	580	582	584	rBV3	5482	5579	0.15%	0.016%
10	6.916	648	651	656	rVB5	2869	5498	0.14%	0.016%
11	7.004	660	666	679	rVB	423159	756611	19.80%	2.237%
12	7.162	686	693	705	rBV	338974	560919	14.68%	1.658%
13	7.362	720	727	738	rBV	423252	743034	19.44%	2.197%
14	7.832	799	807	815	rBV	328074	559291	14.64%	1.654%
15	8.543	921	928	940	rBV	554888	951456	24.90%	2.813%
16	8.984	997	1003	1011	rBV2	422968	742210	19.42%	2.195%
17	9.419	1072	1077	1080	rBV6	5757	8457	0.22%	0.025%
18	9.706	1118	1126	1135	rBV	379027	689691	18.05%	2.039%
19	10.130	1197	1198	1203	rVB2	5386	6346	0.17%	0.019%
20	10.165	1203	1204	1207	rBV	5881	5721	0.15%	0.017%
21	10.247	1211	1218	1229	rBV	518082	993701	26.00%	2.938%
22	10.394	1241	1243	1245	rVB3	7210	6123	0.16%	0.018%
23	10.423	1245	1248	1250	rBV3	4148	5009	0.13%	0.015%
24	10.623	1273	1282	1291	rBV	449227	804538	21.05%	2.379%
25	10.758	1296	1305	1316	rBV	501286	973786	25.48%	2.879%
26	12.227	1551	1555	1558	rBV2	6505	9237	0.24%	0.027%
27	13.008	1686	1688	1693	rBV2	3187	5140	0.13%	0.015%
28	13.655	1797	1798	1801	rBV	4857	5050	0.13%	0.015%
29	13.878	1829	1836	1845	rBV	1122215	1603415	41.96%	4.741%
30	14.160	1877	1884	1893	rBV	1171412	1860545	48.69%	5.501%
31	14.471	1929	1937	1947	rBV	783501	1215531	31.81%	3.594%
32	14.689	1967	1974	1987	rBV	318480	647993	16.96%	1.916%
33	15.470	2099	2107	2116	rBV	1607715	2442588	63.92%	7.222%
34	15.594	2123	2128	2139	rBV	405922	681272	17.83%	2.014%
35	15.870	2172	2175	2178	rBV3	4573	6600	0.17%	0.020%
36	16.028	2200	2202	2208	rBV4	3534	6218	0.16%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112224\
 Data File : BG063514.D
 Acq On : 22 Nov 2024 11:00
 Operator : RC/JU
 Sample : PB165173BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK173

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
 Title : SVOA CALIBRATION

37	16.258	2237	2241	2243	rBV4	5885	8247	0.22%	0.024%
38	16.916	2350	2353	2356	rBV2	5540	9109	0.24%	0.027%
39	17.004	2363	2368	2369	rBV2	4866	7737	0.20%	0.023%
40	17.227	2399	2406	2414	rBV	1129461	1617527	42.33%	4.783%
41	17.327	2416	2423	2434	rVB	1892191	2906561	76.06%	8.594%
42	17.691	2482	2485	2488	rBV3	3714	5473	0.14%	0.016%
43	17.891	2517	2519	2520	rBV	5566	5296	0.14%	0.016%
44	17.997	2533	2537	2540	rVB4	6293	6738	0.18%	0.020%
45	18.032	2540	2543	2546	rBV3	4690	6288	0.16%	0.019%
46	18.696	2655	2656	2659	rBV	7626	6307	0.17%	0.019%
47	19.189	2734	2740	2744	rBV4	29699	44642	1.17%	0.132%
48	19.266	2747	2753	2756	rBV	27910	44630	1.17%	0.132%
49	19.624	2808	2814	2825	rBV	2568658	3717956	97.29%	10.993%
50	19.912	2861	2863	2866	rBV2	7025	5297	0.14%	0.016%
51	20.071	2886	2890	2891	rBV4	7196	9040	0.24%	0.027%
52	20.600	2977	2980	2986	rBV8	13818	19503	0.51%	0.058%
53	21.487	3125	3131	3141	rBV	1295625	1984245	51.92%	5.867%
54	22.603	3317	3321	3327	rVB5	77046	131016	3.43%	0.387%
55	22.903	3368	3372	3379	rVB8	36334	56682	1.48%	0.168%
56	23.649	3497	3499	3507	rVB4	44805	74074	1.94%	0.219%
57	24.325	3603	3614	3629	rBV	1465828	3821377	100.00%	11.299%
58	24.530	3639	3649	3662	rVB	811123	2211952	57.88%	6.540%
59	25.582	3823	3828	3836	rVB4	54430	139318	3.65%	0.412%




Sum of corrected areas: 33821265

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112224\
Data File : BG063514.D
Acq On : 22 Nov 2024 11:00
Operator : RC/JU
Sample : PB165173BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK173

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

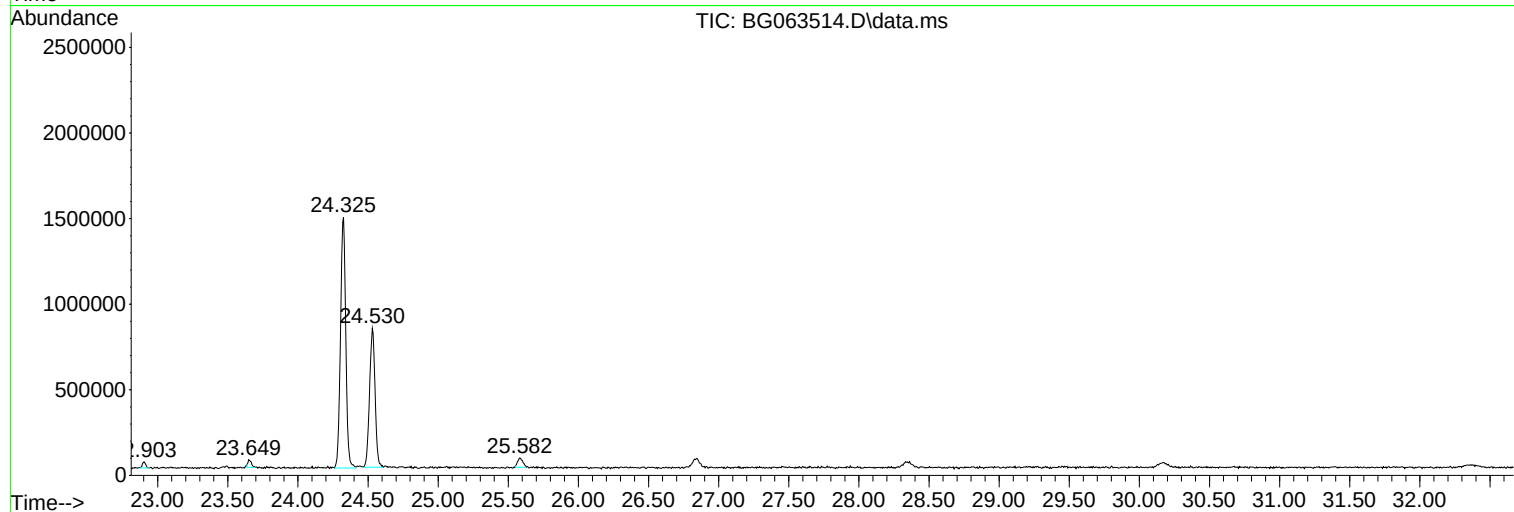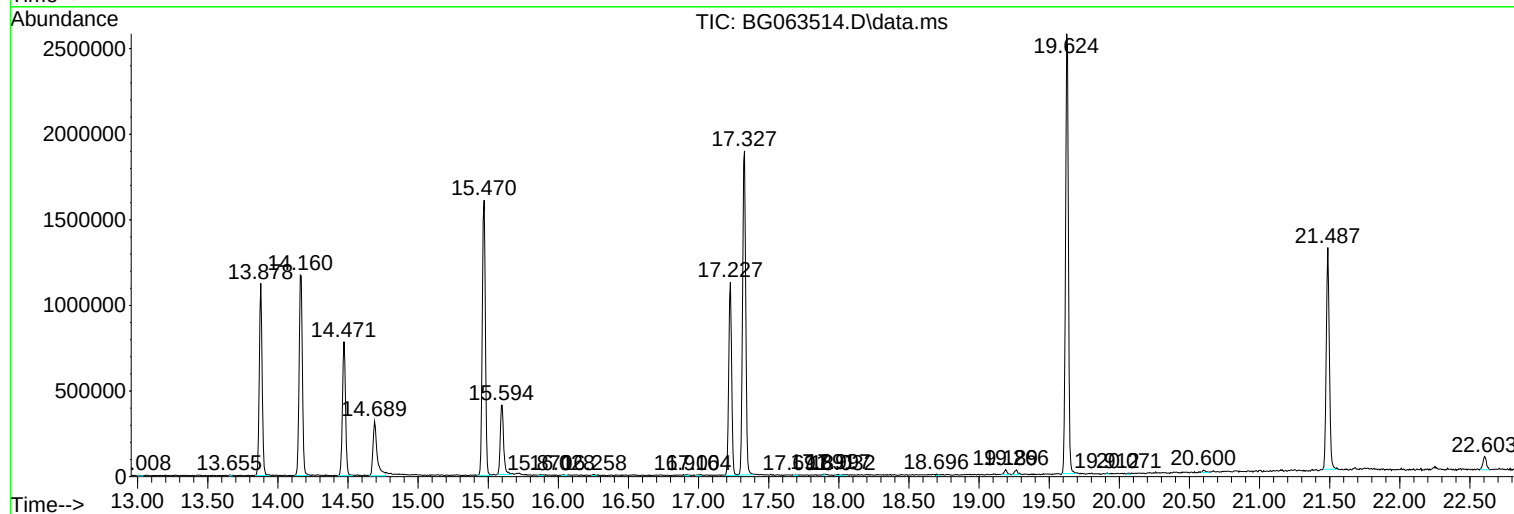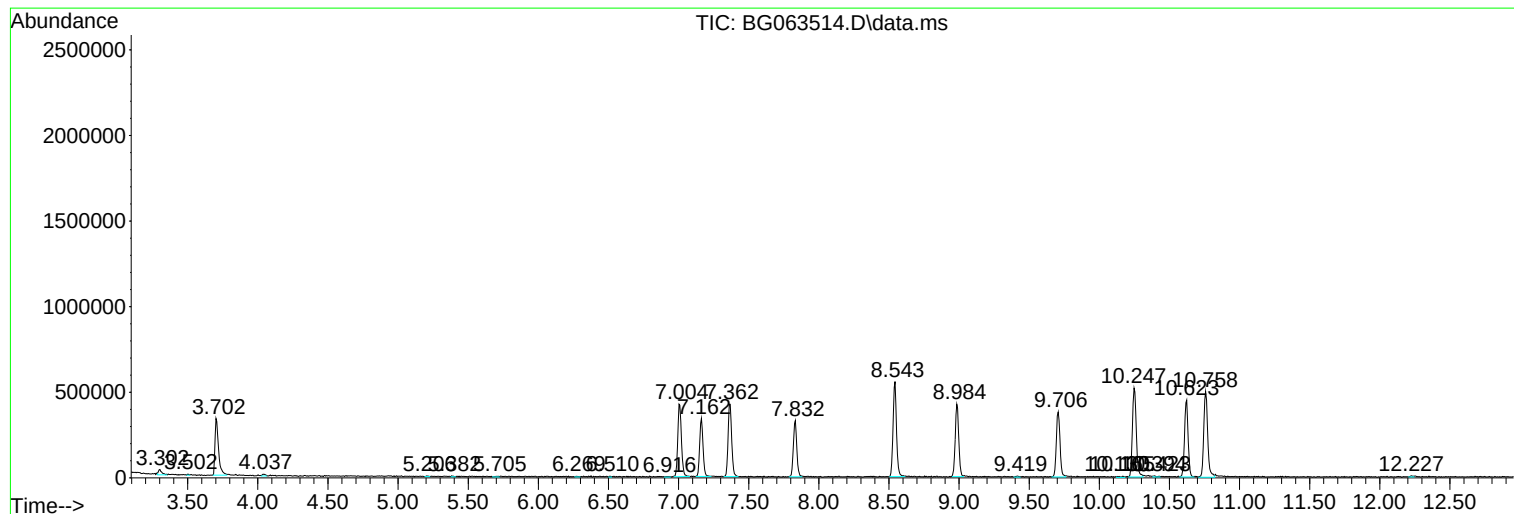

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112224\
Data File : BG063514.D
Acq On : 22 Nov 2024 11:00
Operator : RC/JU
Sample : PB165173BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK173

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112224\
Data File : BG063514.D
Acq On : 22 Nov 2024 11:00
Operator : RC/JU
Sample : PB165173BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK173

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------