

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112224\
 Data File : BG063519.D
 Acq On : 22 Nov 2024 14:26
 Operator : RC/JU
 Sample : PB165173BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK173

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063519.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.299	32	36	42	rVB4	24870	39225	1.43%	0.147%
2	3.699	100	104	118	rBV	252127	448142	16.36%	1.683%
3	4.392	221	222	227	rVB2	4043	4647	0.17%	0.017%
4	4.563	249	251	253	rBV2	4759	3824	0.14%	0.014%
5	5.109	341	344	347	rVB2	6223	6882	0.25%	0.026%
6	5.791	455	460	461	rBV4	4014	5472	0.20%	0.021%
7	5.867	470	473	475	rBV2	3527	4013	0.15%	0.015%
8	5.914	479	481	483	rVB2	5294	3759	0.14%	0.014%
9	6.167	519	524	525	rVB2	3347	4828	0.18%	0.018%
10	6.360	555	557	562	rBV4	4691	6773	0.25%	0.025%
11	6.507	579	582	585	rVB2	5882	6679	0.24%	0.025%
12	6.543	585	588	589	rBV3	5051	4470	0.16%	0.017%
13	6.813	631	634	636	rVB3	5654	5787	0.21%	0.022%
14	6.901	647	649	651	rBV2	4972	5504	0.20%	0.021%
15	7.007	661	667	677	rBV	296105	521260	19.03%	1.957%
16	7.160	687	693	704	rBV	227302	400603	14.63%	1.504%
17	7.365	721	728	739	rBV	306993	527178	19.25%	1.979%
18	7.536	754	757	759	rBV3	4105	4620	0.17%	0.017%
19	7.594	764	767	769	rBV3	4019	4392	0.16%	0.016%
20	7.788	796	800	801	rBV2	3948	4175	0.15%	0.016%
21	7.829	801	807	816	rVV	308912	523913	19.13%	1.967%
22	8.135	857	859	862	rVB3	3427	4154	0.15%	0.016%
23	8.182	862	867	868	rBV4	3472	5491	0.20%	0.021%
24	8.311	886	889	890	rBV2	3764	3753	0.14%	0.014%
25	8.540	920	928	940	rBV2	388601	677910	24.75%	2.545%
26	8.681	947	952	954	rVB4	3685	5415	0.20%	0.020%
27	8.981	994	1003	1011	rBV	280908	512296	18.70%	1.924%
28	9.545	1097	1099	1101	rVB	4565	3998	0.15%	0.015%
29	9.563	1101	1102	1105	rBV	4086	4571	0.17%	0.017%
30	9.704	1120	1126	1134	rBV2	259968	472861	17.26%	1.776%
31	9.804	1141	1143	1146	rVB2	4768	4494	0.16%	0.017%
32	9.874	1152	1155	1156	rBV	4265	3744	0.14%	0.014%
33	9.980	1170	1173	1174	rBV	4766	4627	0.17%	0.017%
34	10.121	1194	1197	1198	rBV	4066	3999	0.15%	0.015%
35	10.185	1205	1208	1209	rVB	6203	4384	0.16%	0.016%
36	10.250	1209	1219	1230	rBV	367549	704440	25.72%	2.645%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112224\
 Data File : BG063519.D
 Acq On : 22 Nov 2024 14:26
 Operator : RC/JU
 Sample : PB165173BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK173

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
 Title : SVOA CALIBRATION

37	10.620	1274	1282	1292	rBV	451239	785408	28.67%	2.949%
38	10.755	1298	1305	1316	rBV	344228	672014	24.53%	2.523%
39	10.879	1325	1326	1329	rVB3	5621	4173	0.15%	0.016%
40	11.290	1391	1396	1397	rBV2	3773	4186	0.15%	0.016%
41	11.325	1400	1402	1404	rBV2	5104	4848	0.18%	0.018%
42	11.449	1420	1423	1427	rBV	3978	4642	0.17%	0.017%
43	11.731	1470	1471	1475	rVB	4447	3964	0.14%	0.015%
44	11.772	1475	1478	1481	rBV2	4437	4658	0.17%	0.017%
45	12.130	1536	1539	1542	rBV2	2886	4259	0.16%	0.016%
46	12.236	1552	1557	1561	rBV4	6793	13554	0.49%	0.051%
47	12.530	1602	1607	1608	rBV2	4067	4287	0.16%	0.016%
48	12.718	1635	1639	1642	rBV2	2785	4614	0.17%	0.017%
49	12.747	1642	1644	1648	rBV2	3812	5626	0.21%	0.021%
50	12.865	1658	1664	1666	rBV2	4797	7958	0.29%	0.030%
51	13.012	1687	1689	1692	rBV	3267	4103	0.15%	0.015%
52	13.487	1764	1770	1773	rBV	3159	6401	0.23%	0.024%
53	13.875	1830	1836	1844	rBV	755412	1125489	41.09%	4.226%
54	14.163	1877	1885	1894	rBV	812141	1300785	47.49%	4.884%
55	14.286	1903	1906	1909	rBV3	4483	6589	0.24%	0.025%
56	14.469	1931	1937	1945	rBV	741272	1171535	42.77%	4.399%
57	14.557	1950	1952	1955	rVB2	3479	4225	0.15%	0.016%
58	14.692	1969	1975	1990	rBV2	184557	412230	15.05%	1.548%
59	14.898	2009	2010	2013	rVB3	4707	4701	0.17%	0.018%
60	15.156	2051	2054	2057	rBV4	3268	4242	0.15%	0.016%
61	15.256	2068	2071	2072	rBV	3419	3870	0.14%	0.015%
62	15.373	2089	2091	2094	rBV2	3446	3906	0.14%	0.015%
63	15.467	2098	2107	2116	rBV	1169189	1725635	63.00%	6.480%
64	15.597	2123	2129	2136	rBV	271770	442729	16.16%	1.662%
65	15.708	2145	2148	2149	rBV3	5883	5863	0.21%	0.022%
66	15.738	2151	2153	2156	rVB3	4158	4440	0.16%	0.017%
67	15.767	2156	2158	2162	rVB4	5071	5032	0.18%	0.019%
68	16.049	2204	2206	2209	rVB2	4681	4934	0.18%	0.019%
69	16.090	2209	2213	2215	rBV	5687	7120	0.26%	0.027%
70	16.413	2266	2268	2271	rVB3	5017	3924	0.14%	0.015%
71	17.019	2368	2371	2374	rVV3	4648	5456	0.20%	0.020%
72	17.048	2374	2376	2379	rVB2	5983	4747	0.17%	0.018%
73	17.224	2399	2406	2415	rBV	1113661	1684612	61.50%	6.326%
74	17.324	2417	2423	2433	rBV2	1389335	2090075	76.31%	7.848%
75	17.483	2448	2450	2454	rVB4	3740	4880	0.18%	0.018%
76	17.765	2496	2498	2501	rBV3	4523	5989	0.22%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112224\
 Data File : BG063519.D
 Acq On : 22 Nov 2024 14:26
 Operator : RC/JU
 Sample : PB165173BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK173

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
 Title : SVOA CALIBRATION

77	17.929	2523	2526	2529	rVB2	4265	5485	0.20%	0.021%
78	18.041	2540	2545	2549	rBV5	6664	10913	0.40%	0.041%
79	18.088	2549	2553	2554	rBV2	3536	4073	0.15%	0.015%
80	18.270	2582	2584	2586	rBV3	4046	3697	0.13%	0.014%

81	18.611	2640	2642	2647	rVB2	5061	5588	0.20%	0.021%
82	18.799	2672	2674	2675	rBV2	7024	4050	0.15%	0.015%
83	19.005	2705	2709	2713	rBV4	3552	6923	0.25%	0.026%
84	19.069	2718	2720	2724	rVB3	4619	6040	0.22%	0.023%
85	19.193	2736	2741	2745	rVB3	26053	38220	1.40%	0.144%

86	19.269	2750	2754	2759	rVB3	22795	34168	1.25%	0.128%
87	19.569	2801	2805	2807	rBV3	5649	7749	0.28%	0.029%
88	19.627	2809	2815	2822	rBV	1920100	2739029	100.00%	10.285%
89	19.739	2833	2834	2837	rBV3	7856	6164	0.23%	0.023%
90	19.804	2844	2845	2847	rBV2	5834	4744	0.17%	0.018%

91	21.484	3125	3131	3143	rBV2	1307464	2154376	78.65%	8.089%
92	21.737	3172	3174	3177	rBV4	15249	24289	0.89%	0.091%
93	22.248	3259	3261	3262	rBV2	15839	12957	0.47%	0.049%
94	24.322	3605	3614	3624	rBV	1069665	2730064	99.67%	10.251%
95	24.533	3640	3650	3660	rBV	906942	2313473	84.46%	8.687%




Sum of corrected areas: 26631988

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112224\
Data File : BG063519.D
Acq On : 22 Nov 2024 14:26
Operator : RC/JU
Sample : PB165173BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK173

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

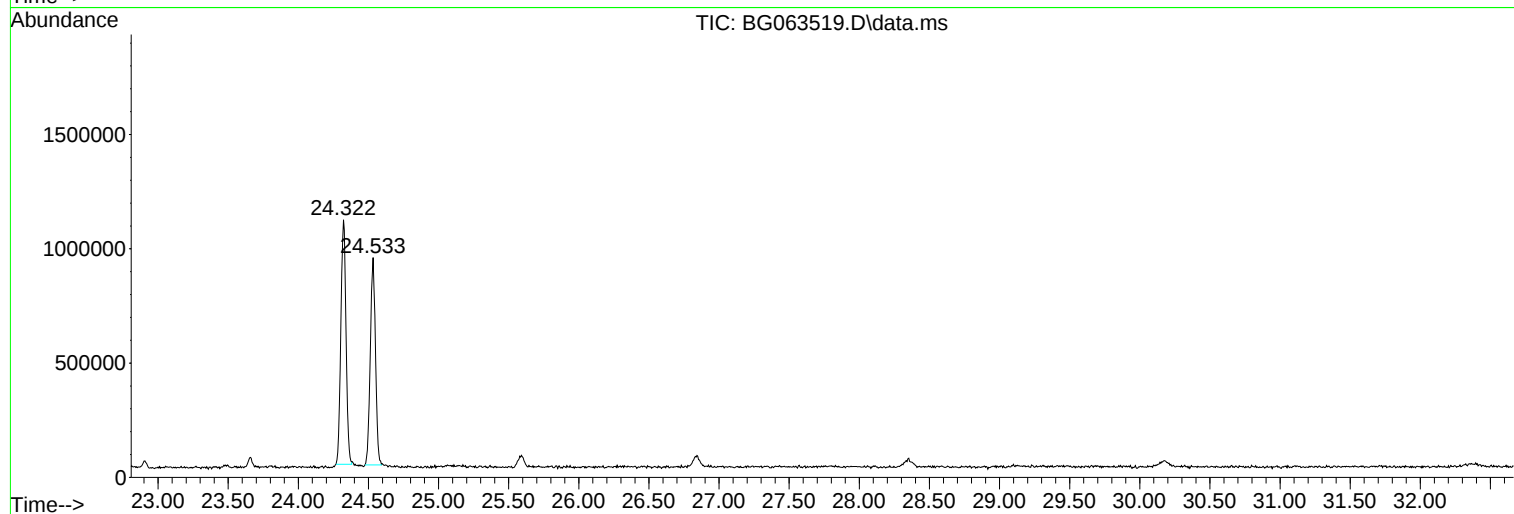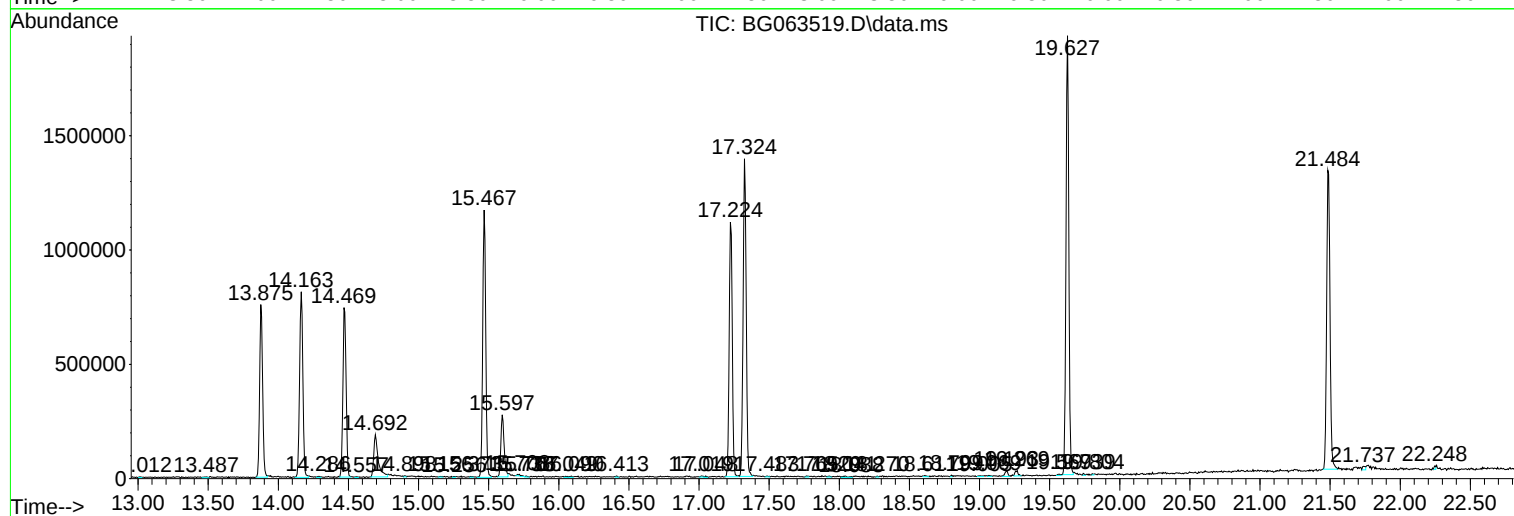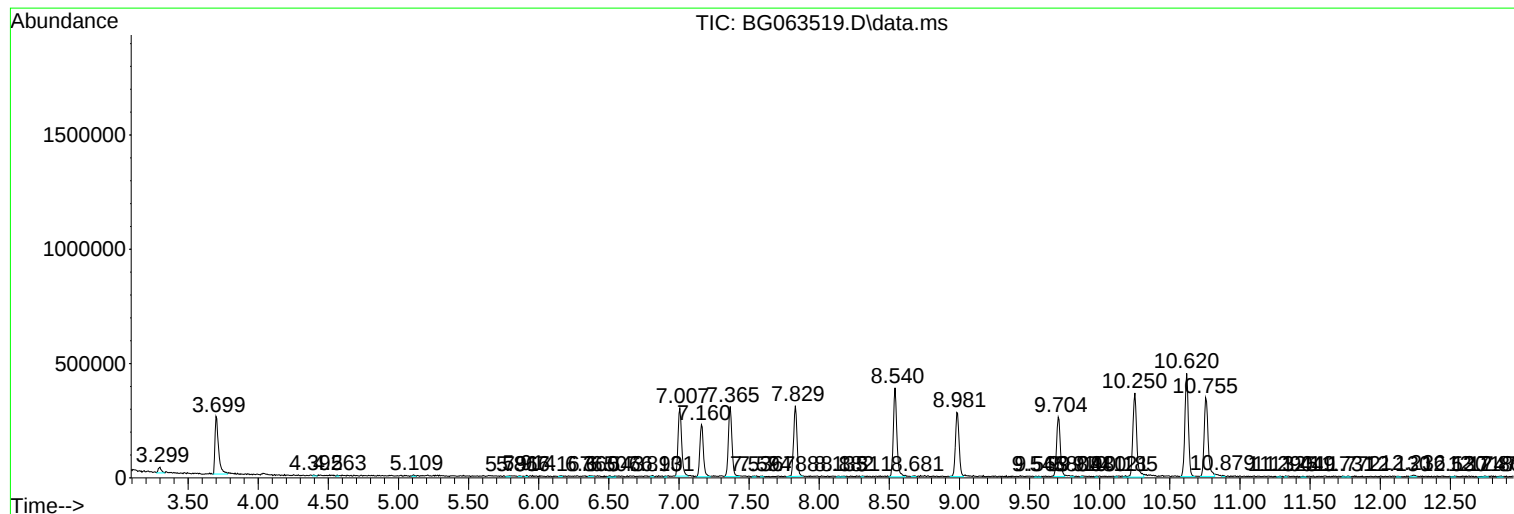

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112224\
Data File : BG063519.D
Acq On : 22 Nov 2024 14:26
Operator : RC/JU
Sample : PB165173BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK173

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112224\
Data File : BG063519.D
Acq On : 22 Nov 2024 14:26
Operator : RC/JU
Sample : PB165173BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK173

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc