

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112522\
 Data File : BG055791.D
 Acq On : 25 Nov 2022 22:06
 Operator : CG/JU
 Sample : N5641-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Nov 26 00:29:57 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 24 06:05:02 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.234	152	48393	20.000	ng	0.00
21) Naphthalene-d8	11.060	136	198944	20.000	ng	0.00
39) Acenaphthene-d10	14.856	164	134762	20.000	ng	0.00
64) Phenanthrene-d10	17.600	188	305100	20.000	ng	0.00
76) Chrysene-d12	21.895	240	293295	20.000	ng	0.00
86) Perylene-d12	25.291	264	306130	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.767	112	270544	101.050	ng	0.00
7) Phenol-d6	7.382	99	350792	98.428	ng	0.00
23) Nitrobenzene-d5	9.403	82	217143	57.690	ng	0.00
42) 2,4,6-Tribromophenol	16.342	330	158726	83.645	ng	0.00
45) 2-Fluorobiphenyl	13.481	172	513232	57.055	ng	0.00
79) Terphenyl-d14	20.185	244	774426	52.812	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propyla...	9.403	70	28968	10.579	ng	Qvalue # 78
51) 2,6-Dinitrotoluene	14.856	165	17553	7.991	ng	# 24
57) 2,4-Dinitrotoluene	14.856	165	17553	5.668	ng	# 22
67) 4-Bromophenyl-phenylether	16.342	248	10212	2.938	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112522\
Data File : BG055791.D
Acq On : 25 Nov 2022 22:06
Operator : CG/JU
Sample : N5641-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Nov 26 00:29:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 24 06:05:02 2022
Response via : Initial Calibration




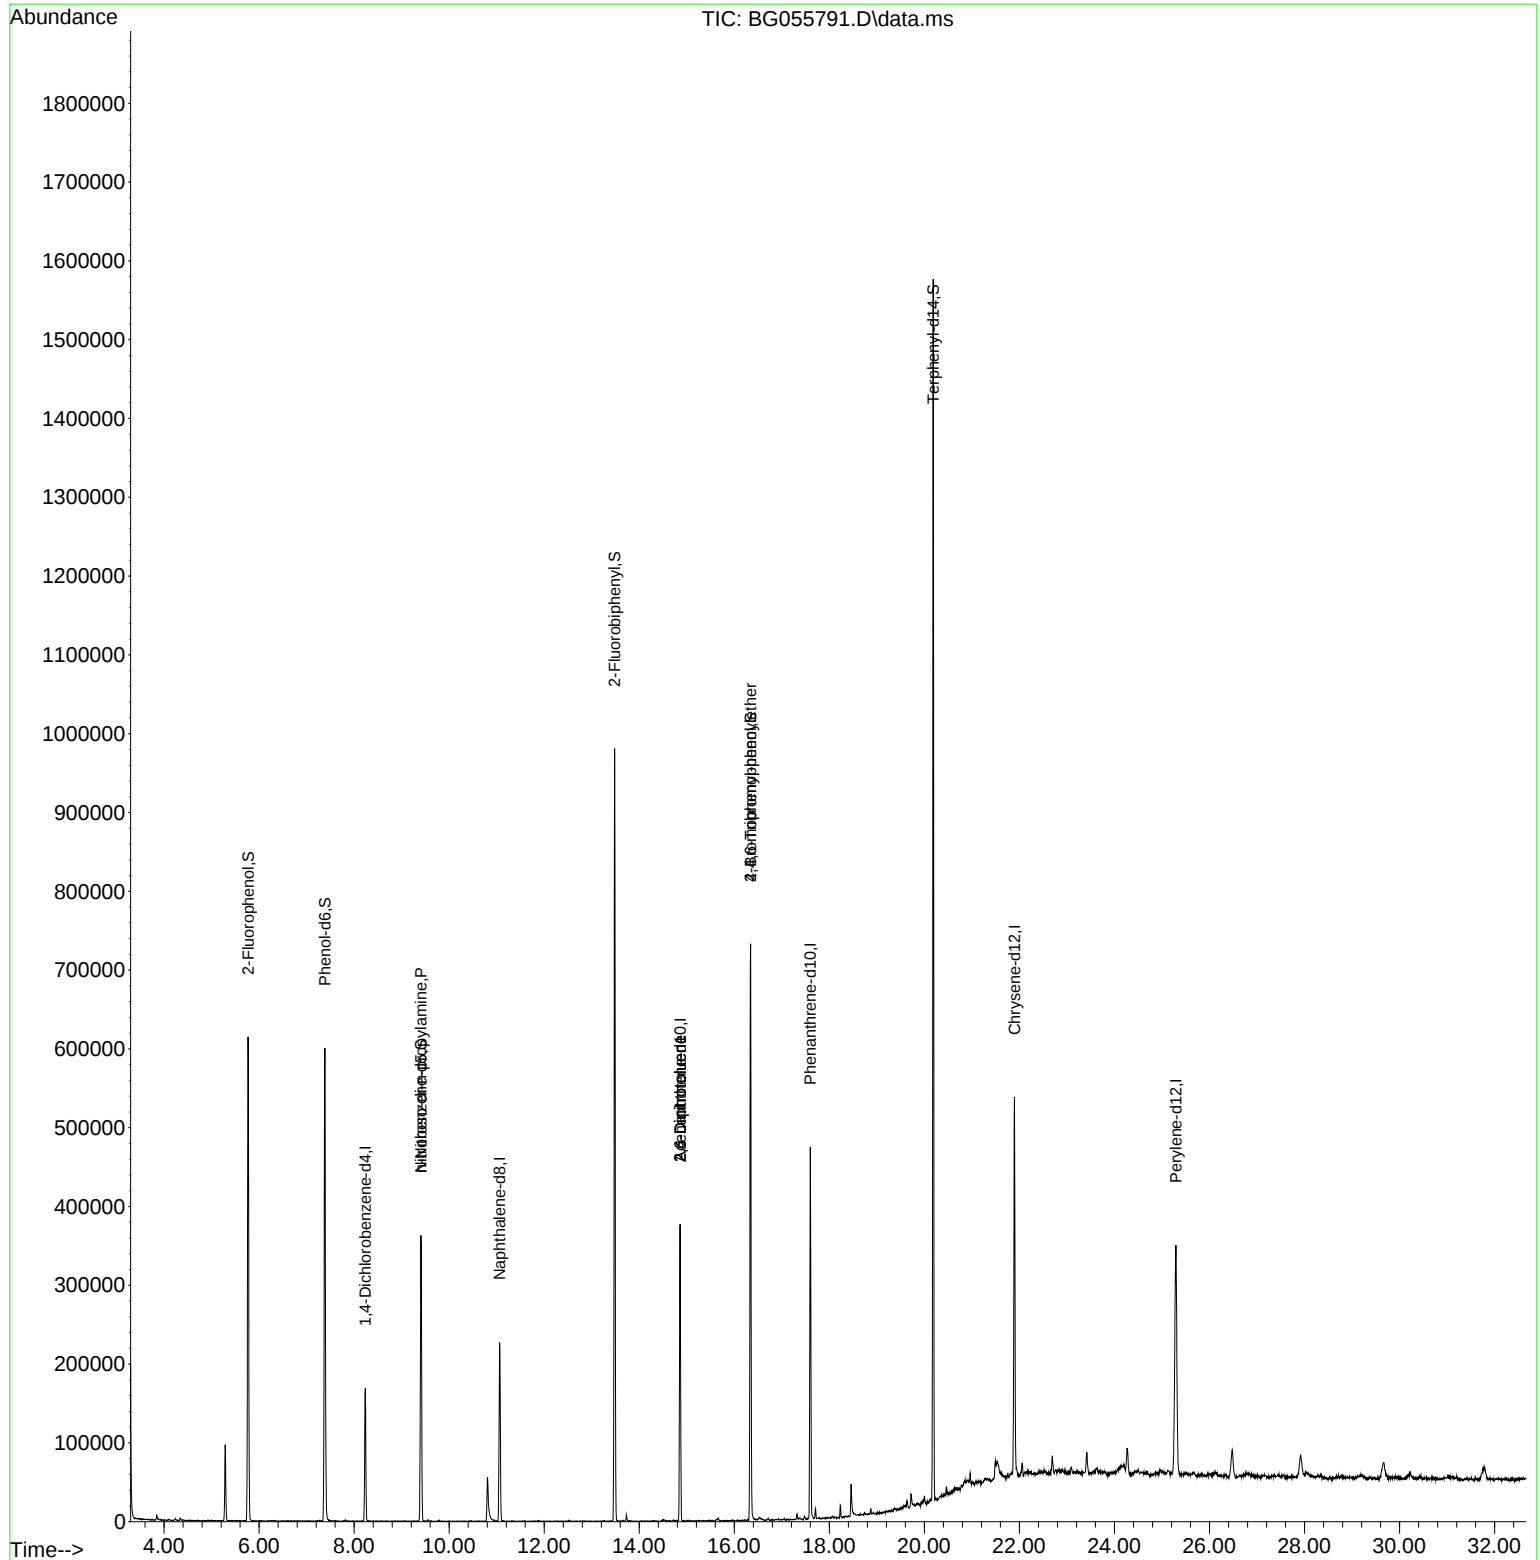


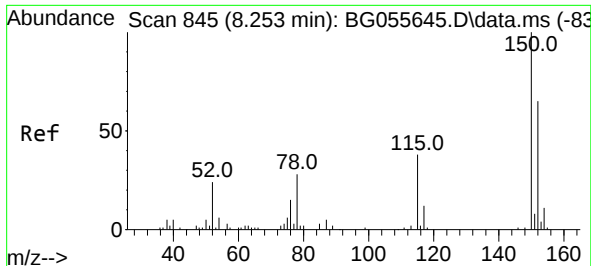

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.234 min Scan# 84
Delta R.T. -0.002 min
Lab File: BG055791.D
Acq: 25 Nov 2022 22:06




Instrument :
BNA_G
ClientSampleId :

Tgt Ion:152 Resp: 48393
Ion Ratio Lower Upper
152 100
150 155.4 123.0 184.6
115 59.5 47.0 70.4

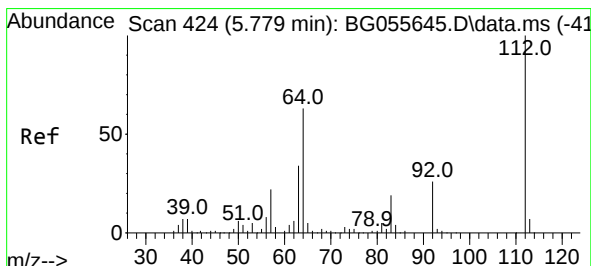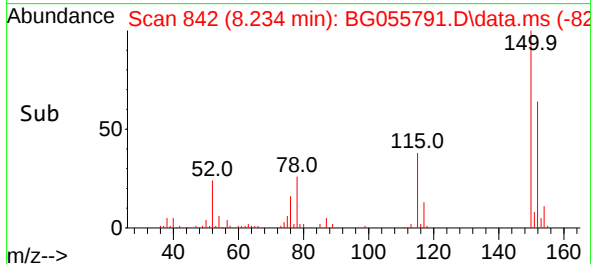

#5
2-Fluorophenol
Concen: 101.050 ng
RT: 5.767 min Scan# 422
Delta R.T. -0.001 min
Lab File: BG055791.D
Acq: 25 Nov 2022 22:06

Tgt Ion:112 Resp: 270544
Ion Ratio Lower Upper
112 100
64 66.6 50.6 76.0
63 34.8 27.5 41.3


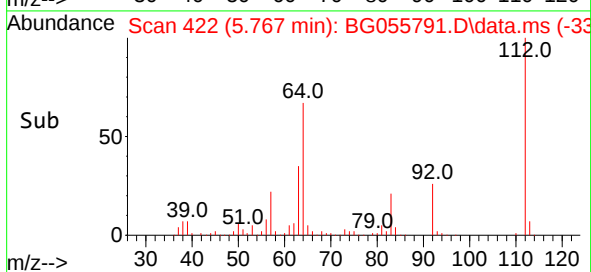

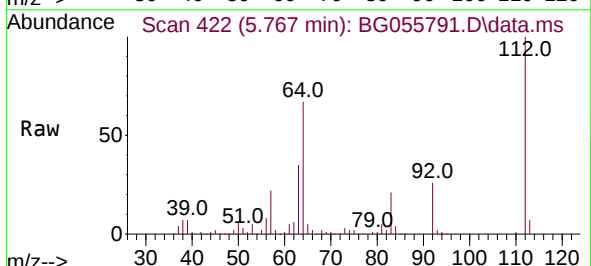




#7
Phenol-d6
Concen: 98.428 ng
RT: 7.382 min Scan# 69
Delta R.T. -0.001 min
Lab File: BG055791.D
Acq: 25 Nov 2022 22:06




Instrument :
BNA_G
ClientSampleId :


Tgt Ion: 99 Resp: 350792
Ion Ratio Lower Upper
99 100
42 21.5 18.0 27.0
71 35.5 29.0 43.6

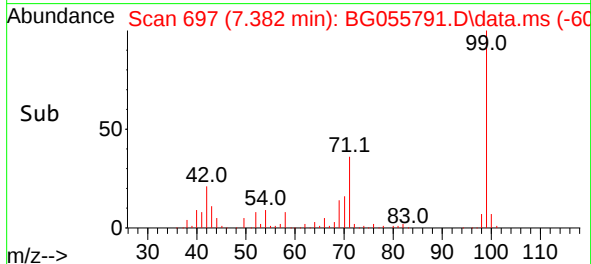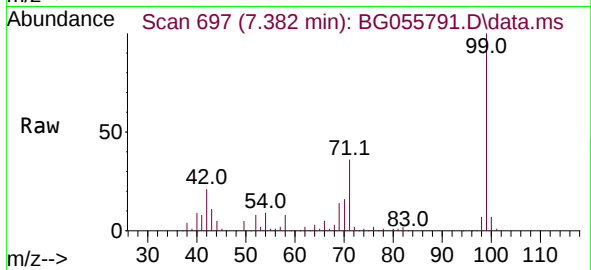

#19
n-Nitroso-di-n-propylamine
Concen: 10.579 ng
RT: 9.403 min Scan# 1041
Delta R.T. 0.357 min
Lab File: BG055791.D
Acq: 25 Nov 2022 22:06


Tgt Ion: 70 Resp: 28968
Ion Ratio Lower Upper
70 100
42 56.1 55.2 82.8
101 0.0 7.1 10.7#
130 1.8 16.1 24.1#

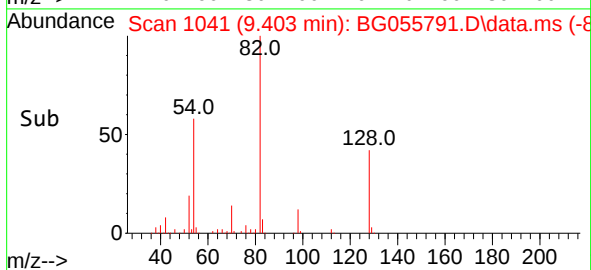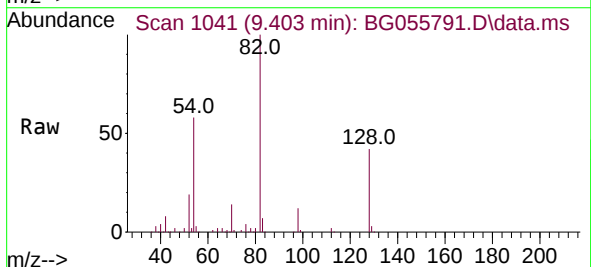



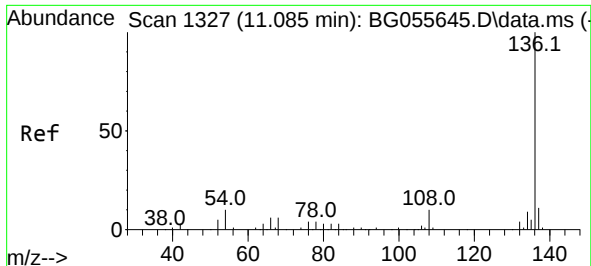


#21
Naphthalene-d8
Concen: 20.000 ng
RT: 11.060 min Scan# 1323
Delta R.T. -0.007 min
Lab File: BG055791.D
Acq: 25 Nov 2022 22:06

Instrument :
BNA_G
ClientSampleId :







Tgt Ion:136 Resp: 198944
Ion Ratio Lower Upper
136 100
137 11.4 9.0 13.6
54 9.4 7.8 11.6
68 5.8 5.0 7.4

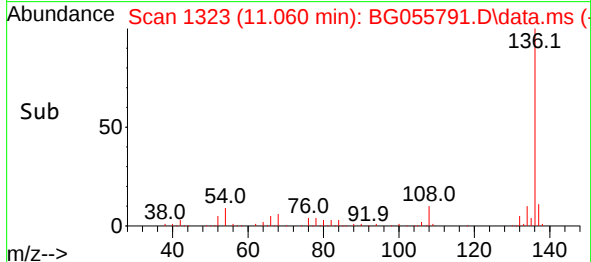

#23
Nitrobenzene-d5
Concen: 57.690 ng
RT: 9.403 min Scan# 1041
Delta R.T. -0.007 min
Lab File: BG055791.D
Acq: 25 Nov 2022 22:06


Tgt Ion: 82 Resp: 217143
Ion Ratio Lower Upper
82 100
128 42.1 34.1 51.1
54 57.7 47.3 70.9

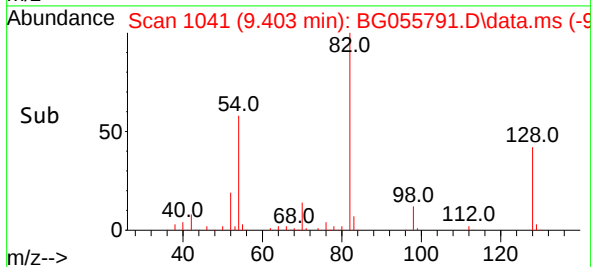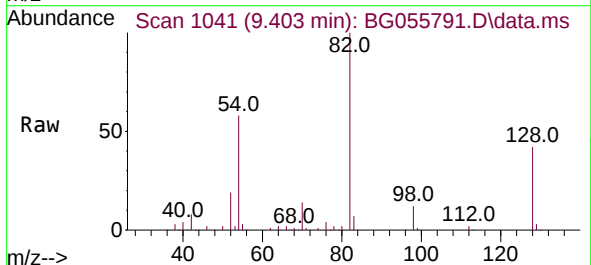






#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.856 min Scan# 1972
Delta R.T. -0.007 min
Lab File: BG055791.D
Acq: 25 Nov 2022 22:06

Instrument :
BNA_G
ClientSampleId :







Tgt Ion:164 Resp: 134762
Ion Ratio Lower Upper
164 100
162 102.4 81.1 121.7
160 43.4 34.8 52.2

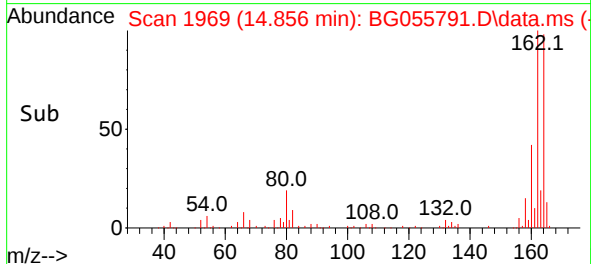

#42
2,4,6-Tribromophenol
Concen: 83.645 ng
RT: 16.342 min Scan# 2222
Delta R.T. -0.007 min
Lab File: BG055791.D
Acq: 25 Nov 2022 22:06

Tgt Ion:330 Resp: 158726
Ion Ratio Lower Upper
330 100
332 95.5 77.8 116.8
141 29.9 23.9 35.9

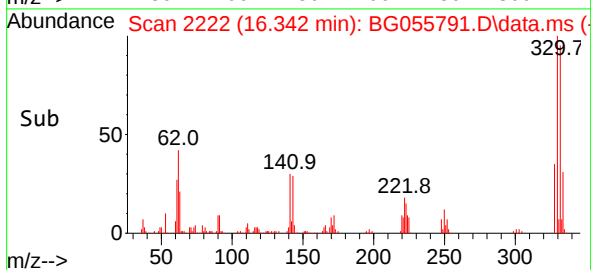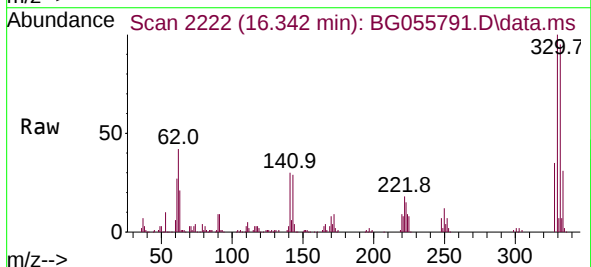



#45

2-Fluorobiphenyl

Concen: 57.055 ng

RT: 13.481 min Scan# 11

Delta R.T. -0.007 min


Lab File: BG055791.D

Acq: 25 Nov 2022 22:06

Instrument :

BNA_G

ClientSampleId :

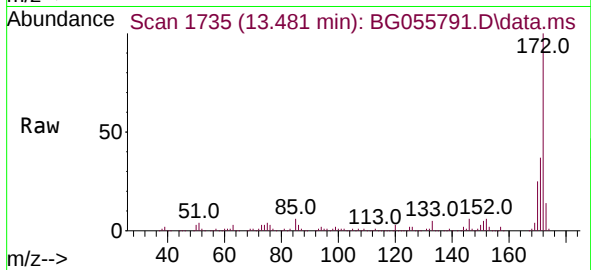




Tgt Ion:172 Resp: 513232

Ion Ratio Lower Upper

172 100

171 36.6 29.8 44.6

170 24.7 20.2 30.4

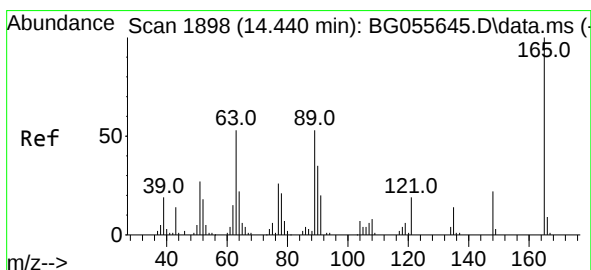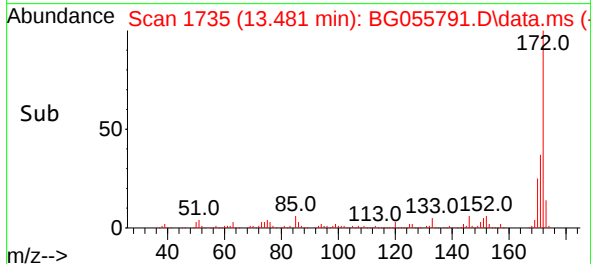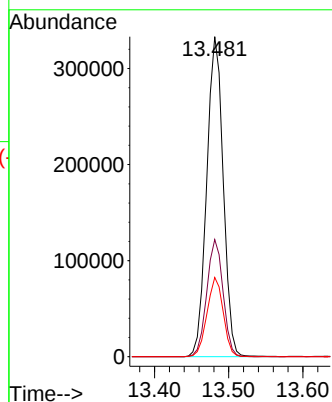

#51

2,6-Dinitrotoluene

Concen: 7.991 ng

RT: 14.856 min Scan# 1969

Delta R.T. 0.422 min

Lab File: BG055791.D

Acq: 25 Nov 2022 22:06




Tgt Ion:165 Resp: 17553


Ion Ratio Lower Upper

165 100

63 0.0 44.6 66.8#


89 0.0 42.2 63.4#

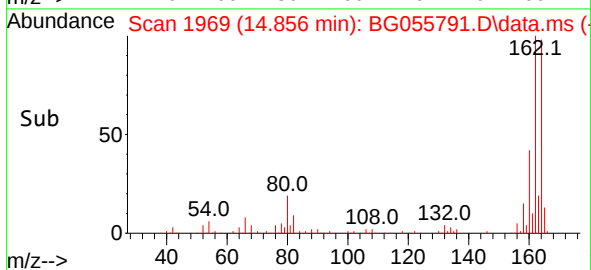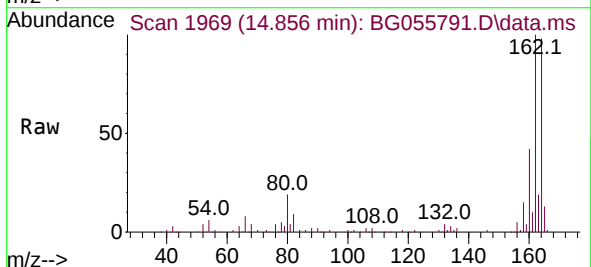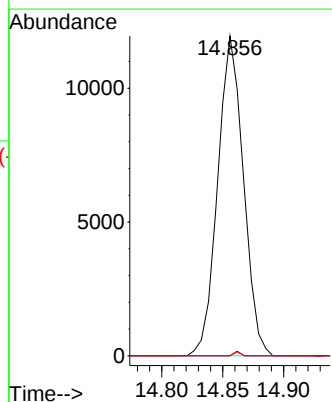



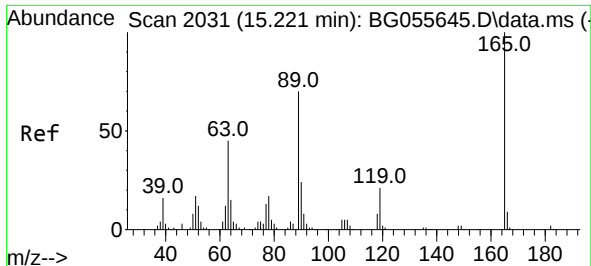


#57
2,4-Dinitrotoluene
Concen: 5.668 ng
RT: 14.856 min Scan# 1969
Delta R.T. -0.360 min
Lab File: BG055791.D
Acq: 25 Nov 2022 22:06


Instrument :
BNA_G
ClientSampleId :





Tgt Ion:165 Resp: 17553
Ion Ratio Lower Upper
165 100
63 0.0 35.8 53.8#
89 0.0 56.2 84.4#
182 0.0 1.8 2.8#

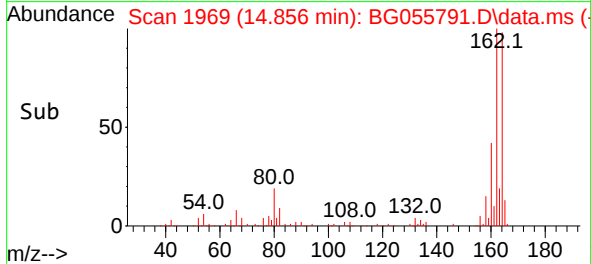


#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.600 min Scan# 2436
Delta R.T. -0.007 min
Lab File: BG055791.D
Acq: 25 Nov 2022 22:06

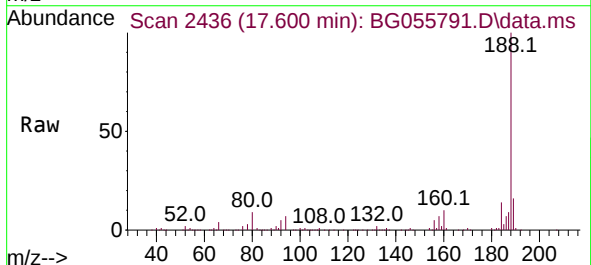


Tgt Ion:188 Resp: 305100
Ion Ratio Lower Upper
188 100
94 7.2 5.4 8.2
80 8.5 6.6 10.0

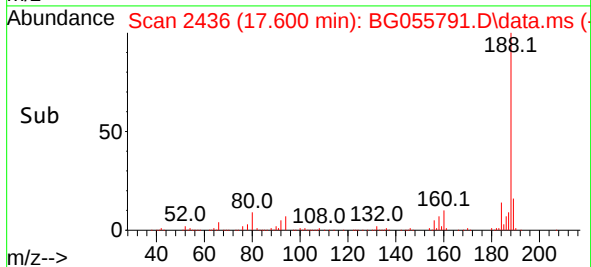



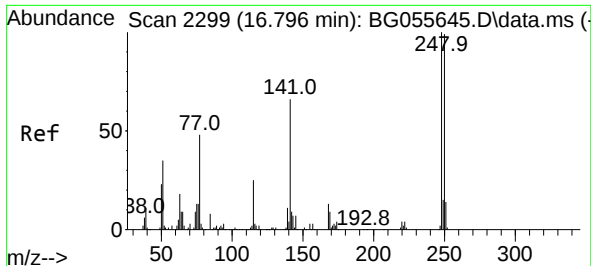


#67
4-Bromophenyl-phenylether
Concen: 2.938 ng
RT: 16.342 min Scan# 21
Delta R.T. -0.442 min
Lab File: BG055791.D
Acq: 25 Nov 2022 22:06


Instrument :
BNA_G
ClientSampleId :





Tgt Ion:248 Resp: 10212
Ion Ratio Lower Upper
248 100
250 190.3 79.0 118.4#
141 453.6 52.9 79.3#

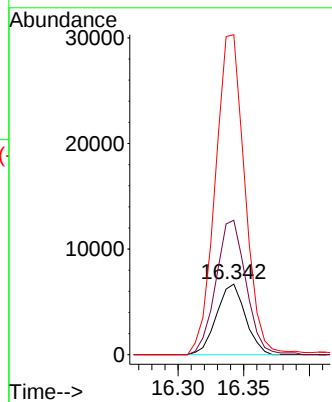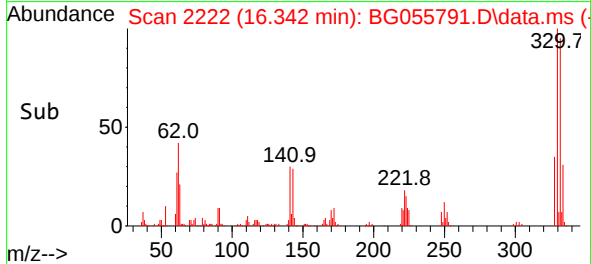


#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.895 min Scan# 3167
Delta R.T. -0.007 min
Lab File: BG055791.D
Acq: 25 Nov 2022 22:06

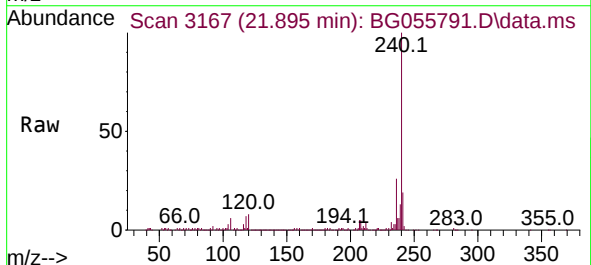


Tgt Ion:240 Resp: 293295
Ion Ratio Lower Upper
240 100
120 7.8 6.3 9.5
236 25.8 21.9 32.9

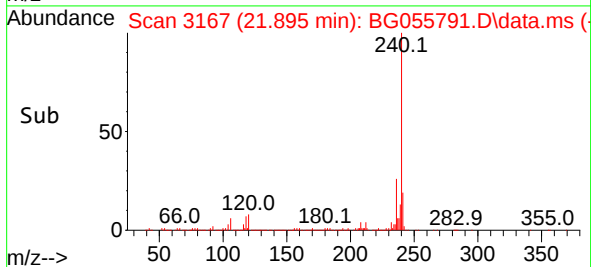



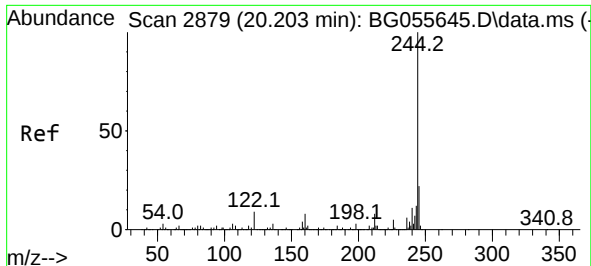


#79
 Terphenyl-d14
 Concen: 52.812 ng
 RT: 20.185 min Scan# 2879
 Delta R.T. -0.007 min
 Lab File: BG055791.D
 Acq: 25 Nov 2022 22:06

Instrument :
 BNA_G
 ClientSampleId :



Tgt Ion:244 Resp: 774426
 Ion Ratio Lower Upper
 244 100
 212 7.4 6.3 9.5
 122 8.7 6.9 10.3

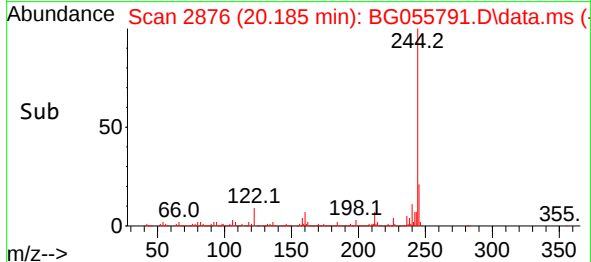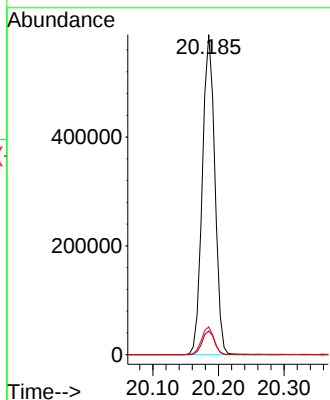

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 25.291 min Scan# 3745
 Delta R.T. -0.013 min
 Lab File: BG055791.D
 Acq: 25 Nov 2022 22:06

Tgt Ion:264 Resp: 306130
 Ion Ratio Lower Upper
 264 100
 260 24.0 19.5 29.3
 265 22.0 17.1 25.7

