
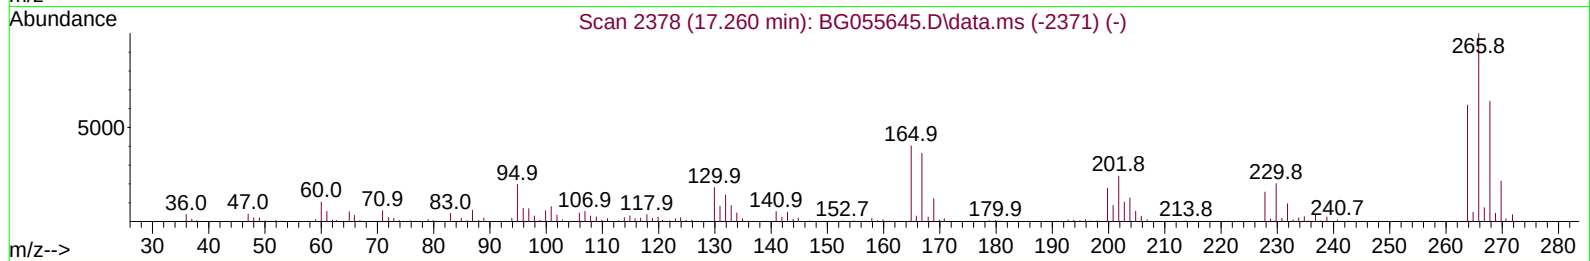
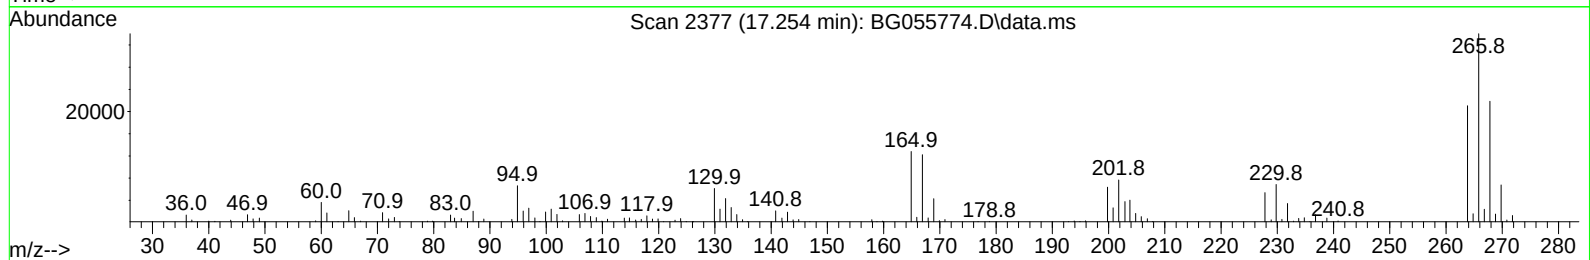


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112522\
Data File : BG055774.D
Acq On : 25 Nov 2022 10:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 26 01:44:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 24 06:05:02 2022
Response via : Initial Calibration

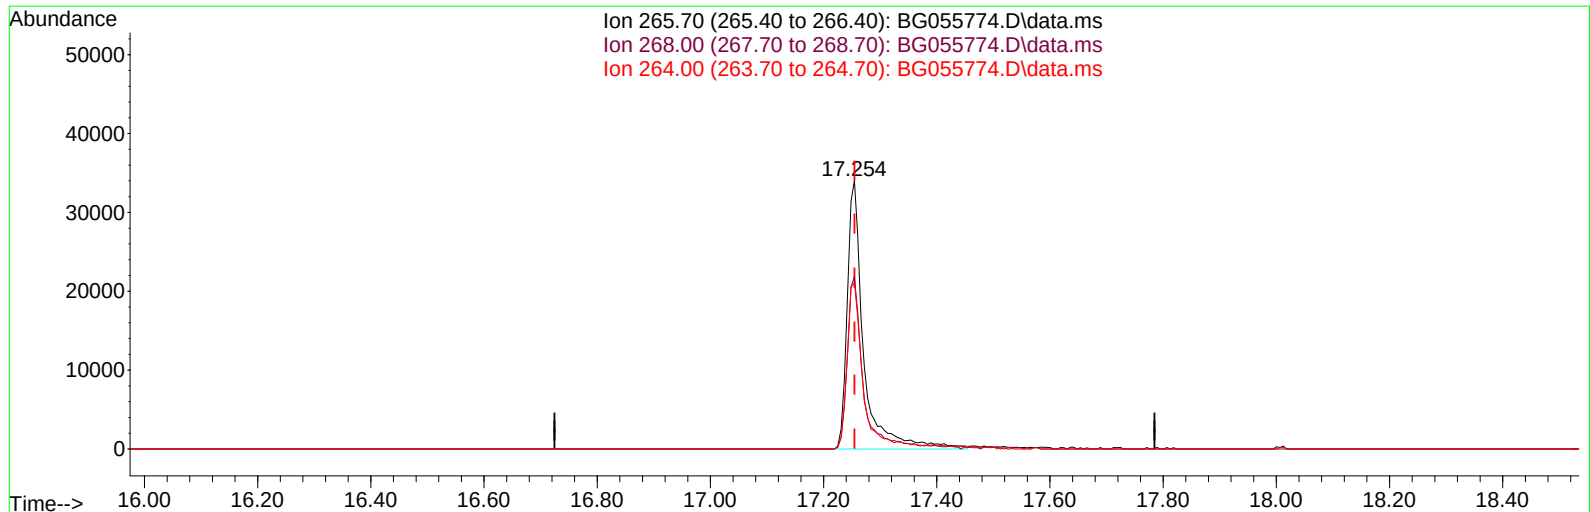

TIC: BG055774.D\data.ms

(70) Pentachlorophenol (C)




17.254min (0.000) 19259.57 ng

response 68768

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	64.23
264.00	61.90	61.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112522\
Data File : BG055774.D
Acq On : 25 Nov 2022 10:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 26 01:44:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 24 06:05:02 2022
Response via : Initial Calibration

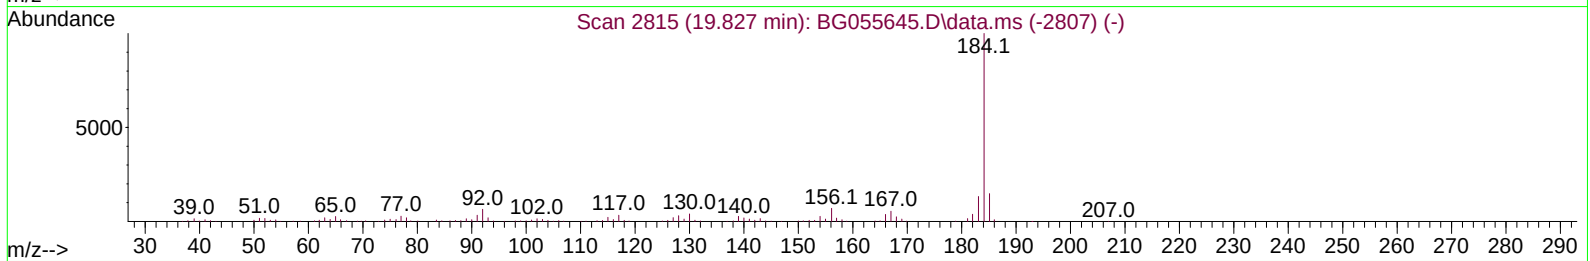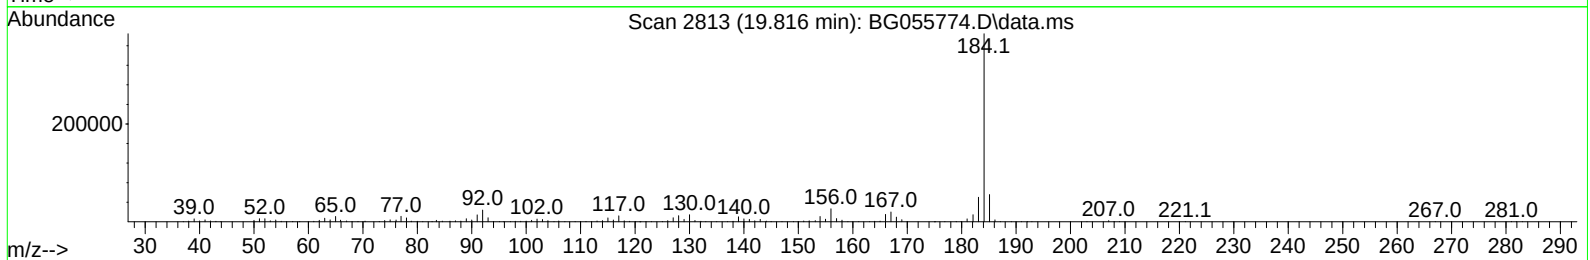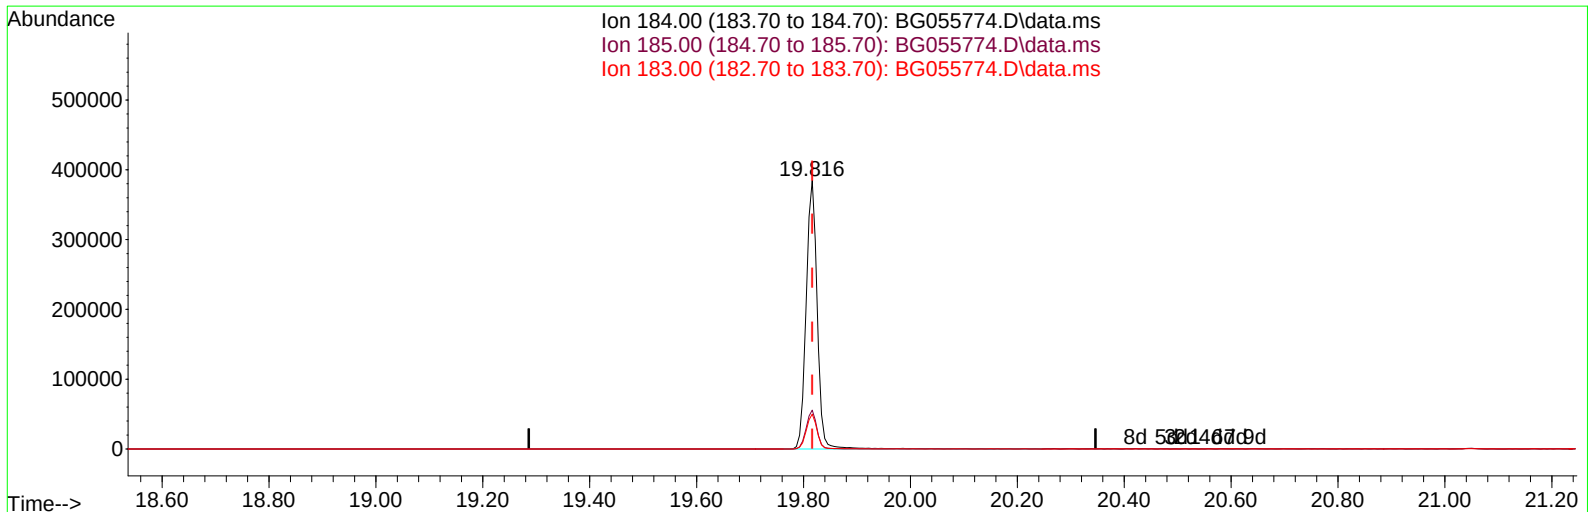

TIC: BG055774.D\data.ms

(77) Benzidine

19.816min (0.000) 451444.09 ng m

response 553528

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.49
183.00	13.20	13.00
0.00	0.00	0.00