
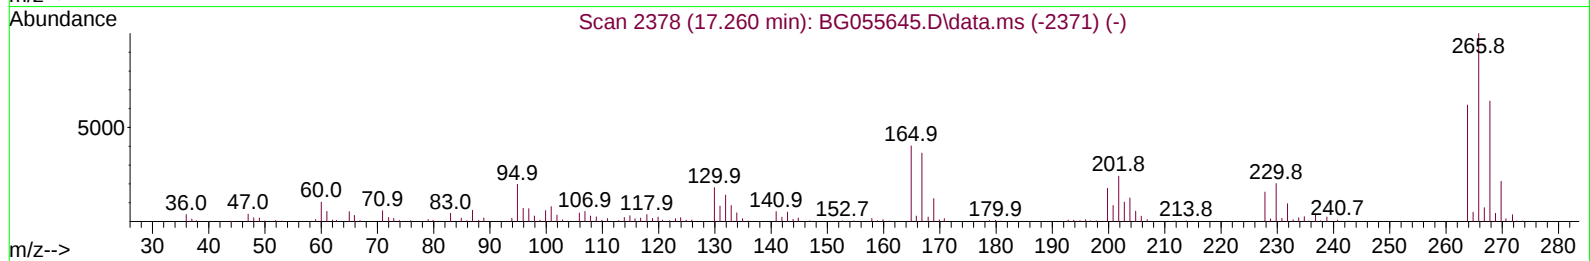
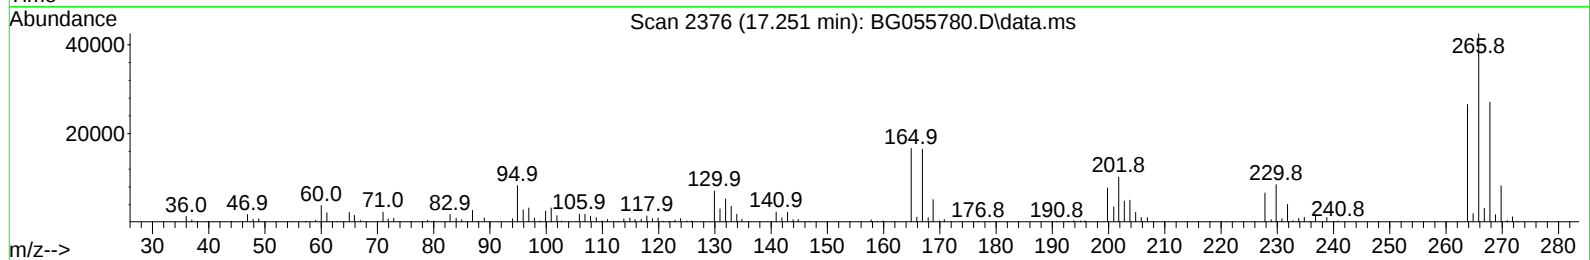


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG112522\  
Data File : BG055780.D  
Acq On : 25 Nov 2022 14:21  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 26 01:45:56 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG111622.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Nov 24 06:05:02 2022  
Response via : Initial Calibration

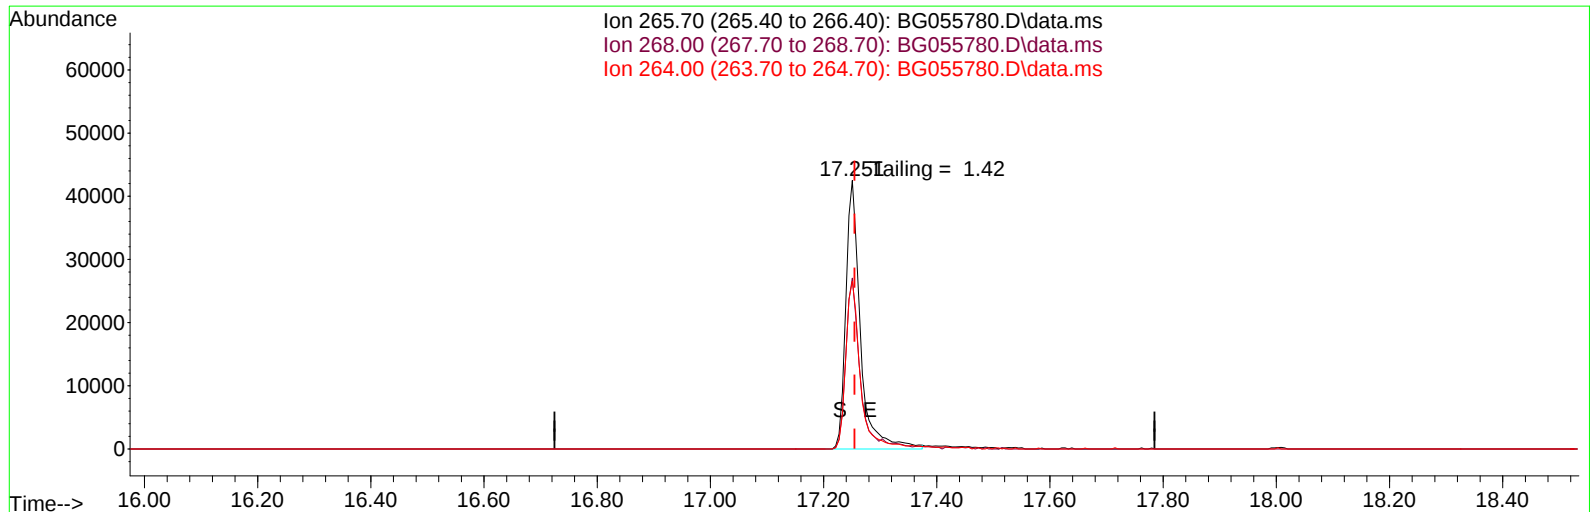

TIC: BG055780.D\data.ms

**(70) Pentachlorophenol (C)**




17.251min (-0.004) 23621.01 ng

response 76491

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 64.00  | 63.66  |
| 264.00 | 61.90  | 62.47  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG112522\  
Data File : BG055780.D  
Acq On : 25 Nov 2022 14:21  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 26 01:45:56 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG111622.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Nov 24 06:05:02 2022  
Response via : Initial Calibration

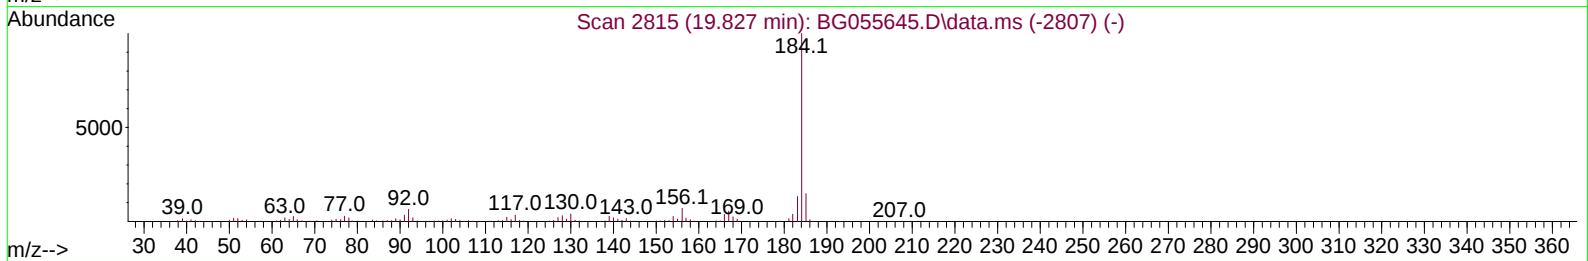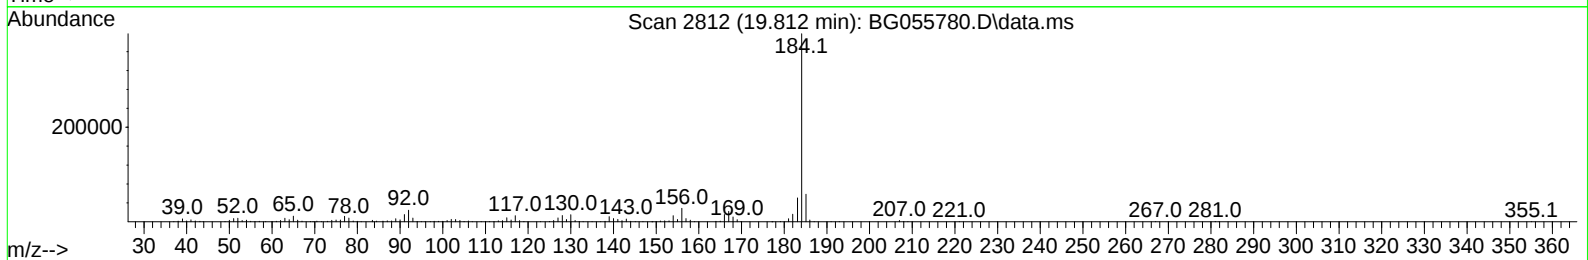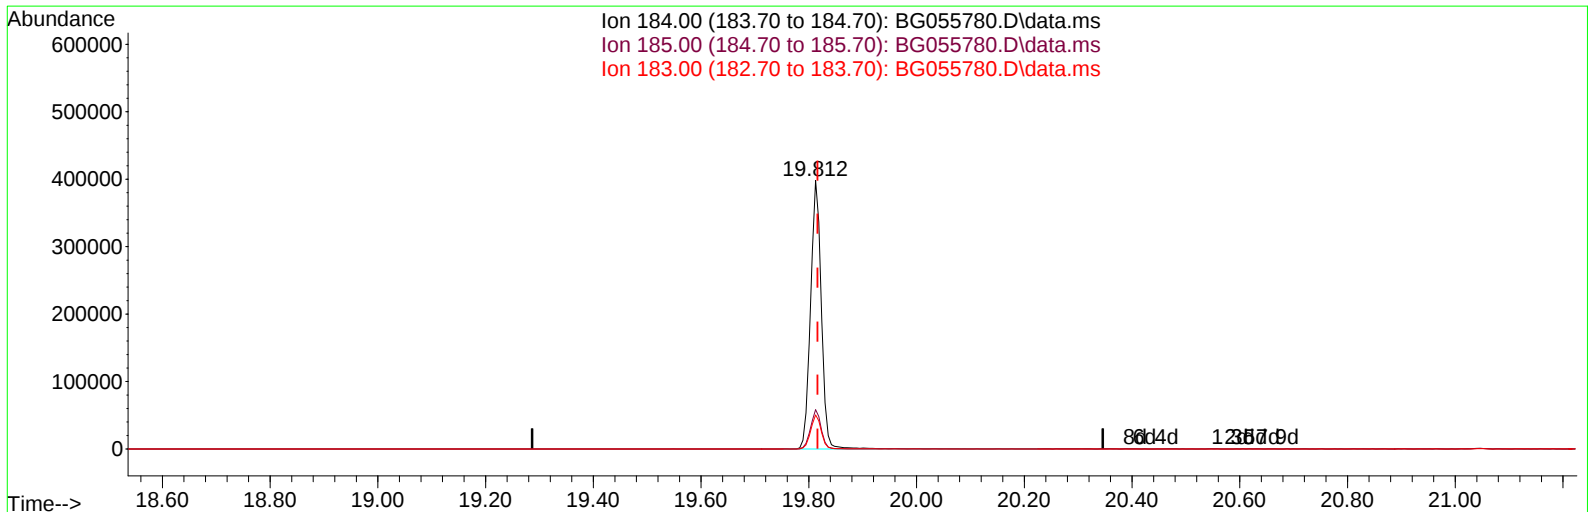

TIC: BG055780.D\data.ms

(77) Benzidine

19.812min (-0.004) 415453.91 ng m

response 557456

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.80  | 14.66  |
| 183.00 | 13.20  | 12.68  |
| 0.00   | 0.00   | 0.00   |