

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112522\
 Data File : BG055789.D
 Acq On : 25 Nov 2022 20:44
 Operator : CG/JU
 Sample : N5747-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 FB112122

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG055789.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.285	333	340	348	rBV	80360	123606	3.98%	1.030%
2	5.767	414	422	434	rBV	344166	556471	17.91%	4.639%
3	7.383	686	697	707	rBV	191151	344101	11.08%	2.869%
4	8.235	834	842	852	rBV	139994	242582	7.81%	2.022%
5	9.404	1031	1041	1052	rBV	481095	868133	27.95%	7.237%
6	11.061	1314	1323	1333	rBV	188967	340219	10.95%	2.836%
7	13.481	1728	1735	1745	rBV	1319187	2057595	66.24%	17.153%
8	14.856	1963	1969	1978	rVB	317656	487658	15.70%	4.065%
9	16.343	2215	2222	2237	rBV	1063030	1670836	53.79%	13.929%
10	17.600	2429	2436	2447	rBV	421899	645016	20.76%	5.377%
11	20.185	2870	2876	2882	rBV	2371362	3106312	100.00%	25.895%
12	21.889	3160	3166	3173	rVB2	434120	740579	23.84%	6.174%
13	25.285	3734	3744	3758	rVB2	264478	812536	26.16%	6.774%




Sum of corrected areas: 11995644

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112522\
Data File : BG055789.D
Acq On : 25 Nov 2022 20:44
Operator : CG/JU
Sample : N5747-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
FB112122

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

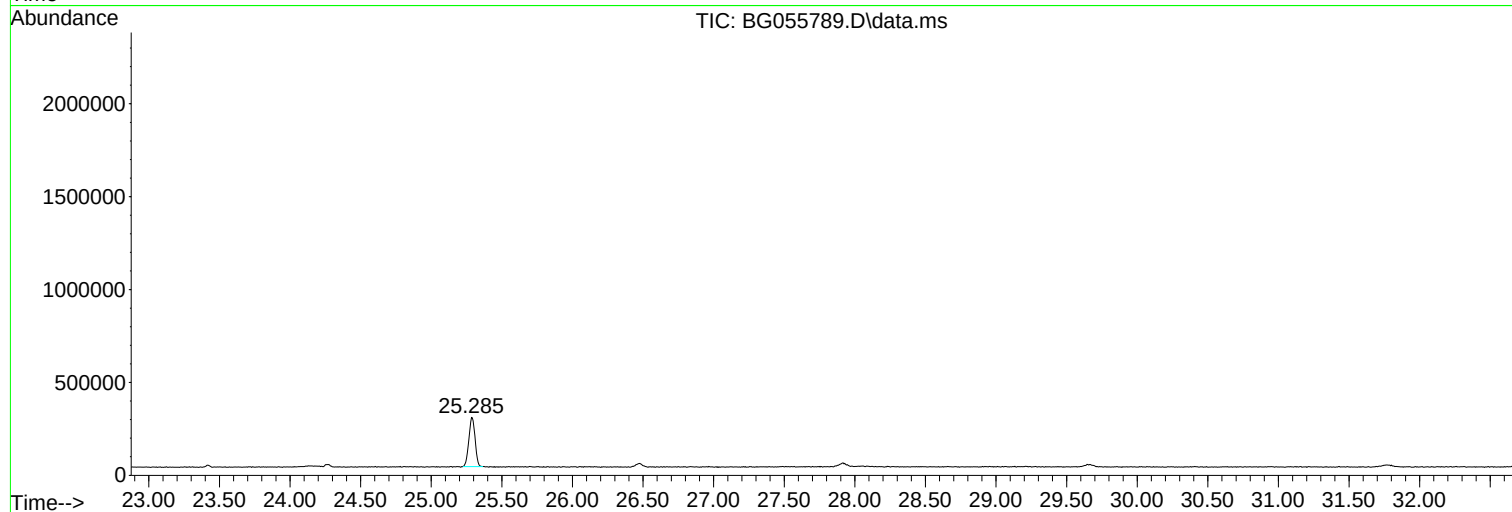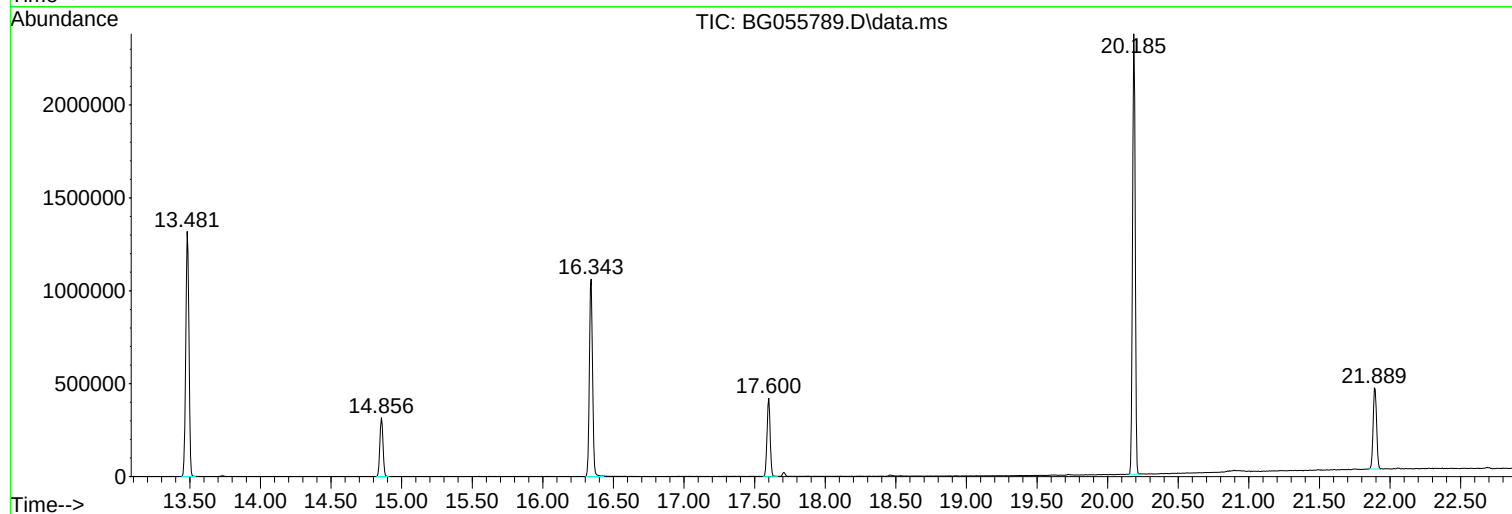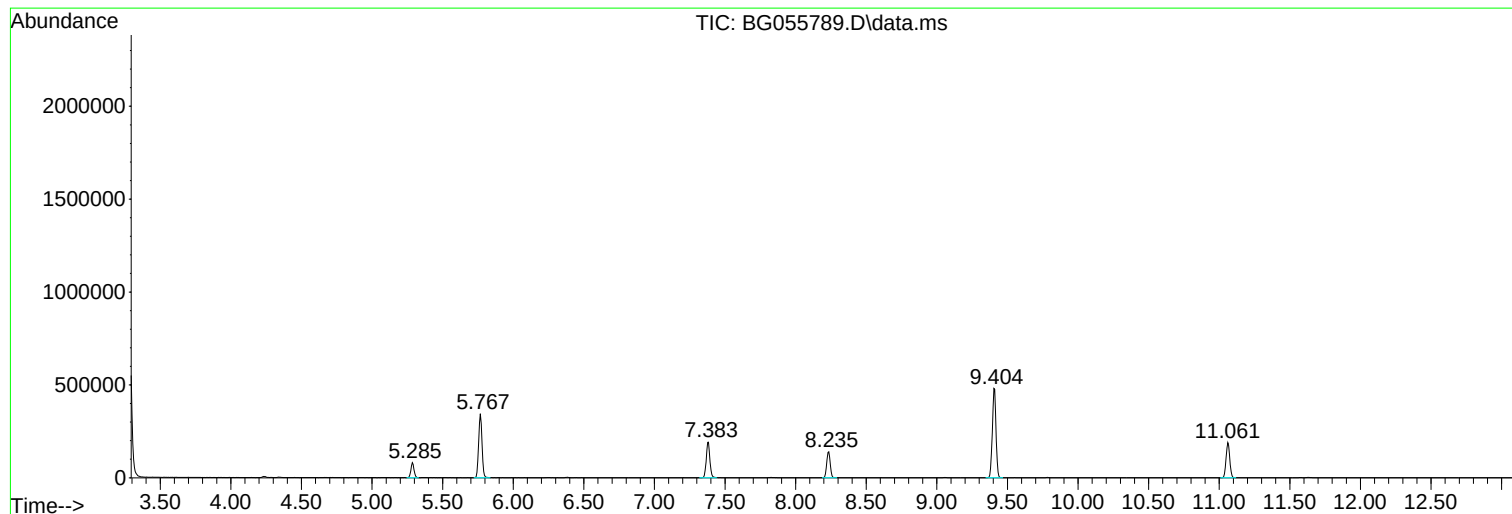

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112522\
Data File : BG055789.D
Acq On : 25 Nov 2022 20:44
Operator : CG/JU
Sample : N5747-06
Misc :
ALS Vial : 10 Sample Multiplier: 1










Instrument :
BNA_G
ClientSampleId :
FB112122

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG11622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
5.285	10.19 ng	123606	1,4-Dichlorobenzene-d4	8.235	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	72
2	3-Octanol	130	C8H18O	000589-98-0	36
3	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	25
4	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	23
5	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	12

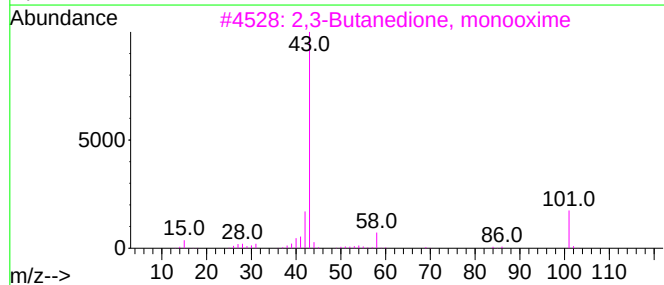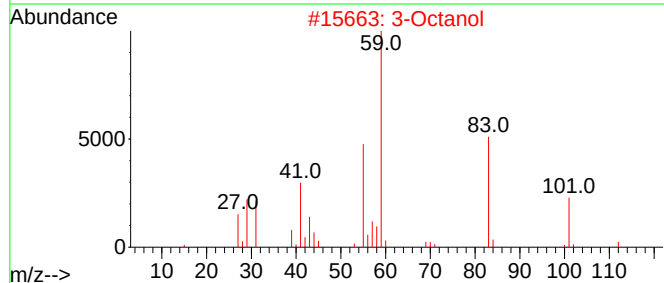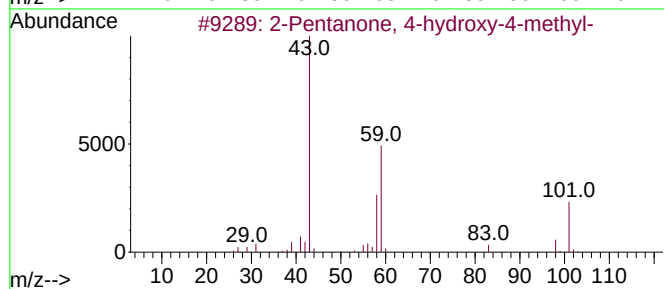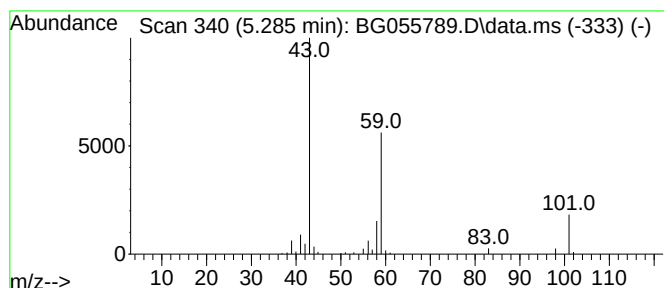

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112522\
Data File : BG055789.D
Acq On : 25 Nov 2022 20:44
Operator : CG/JU
Sample : N5747-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
FB112122

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.285	10.2	ng	123606	1	8.235	242582	20.0