

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112522\
 Data File : BG055790.D
 Acq On : 25 Nov 2022 21:25
 Operator : CG/JU
 Sample : N5769-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 COMP-218

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG055790.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.669	228	235	247	rBV	92083	142242	5.58%	1.123%
2	5.286	333	340	349	rBV	169069	260179	10.21%	2.055%
3	5.768	415	422	432	rBV	537620	862596	33.86%	6.812%
4	7.384	689	697	716	rVB	596378	1050842	41.25%	8.299%
5	8.235	836	842	848	rVB	158475	266424	10.46%	2.104%
6	9.405	1034	1041	1047	rBV	386324	693450	27.22%	5.476%
7	11.003	1307	1313	1317	rBV	42597	66693	2.62%	0.527%
8	11.062	1317	1323	1330	rVB	217039	394256	15.48%	3.114%
9	11.191	1340	1345	1351	rVB	32175	51701	2.03%	0.408%
10	11.943	1469	1473	1482	rVB2	13217	27276	1.07%	0.215%
11	12.049	1484	1491	1495	rBV	53236	88692	3.48%	0.700%
12	12.436	1550	1557	1565	rBV	72549	112502	4.42%	0.888%
13	12.654	1587	1594	1599	rVB4	15936	34874	1.37%	0.275%
14	12.842	1621	1626	1635	rBV8	7785	26129	1.03%	0.206%
15	13.059	1658	1663	1667	rBV5	14256	28665	1.13%	0.226%
16	13.235	1688	1693	1698	rBV2	17323	30161	1.18%	0.238%
17	13.318	1702	1707	1712	rVV2	18115	30465	1.20%	0.241%
18	13.376	1712	1717	1722	rVB	61057	88242	3.46%	0.697%
19	13.482	1728	1735	1741	rVB	1104572	1665213	65.37%	13.151%
20	13.658	1758	1765	1775	rBV	97959	164402	6.45%	1.298%
21	14.281	1866	1871	1873	rBV2	32463	51931	2.04%	0.410%
22	14.311	1873	1876	1880	rVV2	67790	90465	3.55%	0.714%
23	14.681	1934	1939	1942	rVV4	18841	34307	1.35%	0.271%
24	14.722	1942	1946	1955	rVB	77225	107145	4.21%	0.846%
25	14.857	1963	1969	1978	rVB	358488	572741	22.48%	4.523%
26	15.339	2045	2051	2058	rBV5	12882	26883	1.06%	0.212%
27	15.668	2097	2107	2112	rVB	45463	71818	2.82%	0.567%
28	16.073	2168	2176	2180	rBV2	16921	32503	1.28%	0.257%
29	16.338	2215	2221	2229	rBV	473438	742645	29.15%	5.865%
30	16.526	2249	2253	2255	rBV2	24293	32469	1.27%	0.256%
31	16.549	2255	2257	2265	rVB3	23057	29910	1.17%	0.236%
32	17.601	2429	2436	2442	rBV	443206	690067	27.09%	5.450%
33	18.453	2578	2581	2586	rVB3	26296	40873	1.60%	0.323%
34	20.186	2870	2876	2882	rBV	1989064	2547506	100.00%	20.119%
35	21.896	3161	3167	3173	rVB2	409369	707242	27.76%	5.585%
36	25.292	3736	3745	3758	rVB	254802	798899	31.36%	6.309%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112522\
Data File : BG055790.D
Acq On : 25 Nov 2022 21:25
Operator : CG/JU
Sample : N5769-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
COMP-218

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION




Sum of corrected areas: 12662408

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112522\
Data File : BG055790.D
Acq On : 25 Nov 2022 21:25
Operator : CG/JU
Sample : N5769-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
COMP-218

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

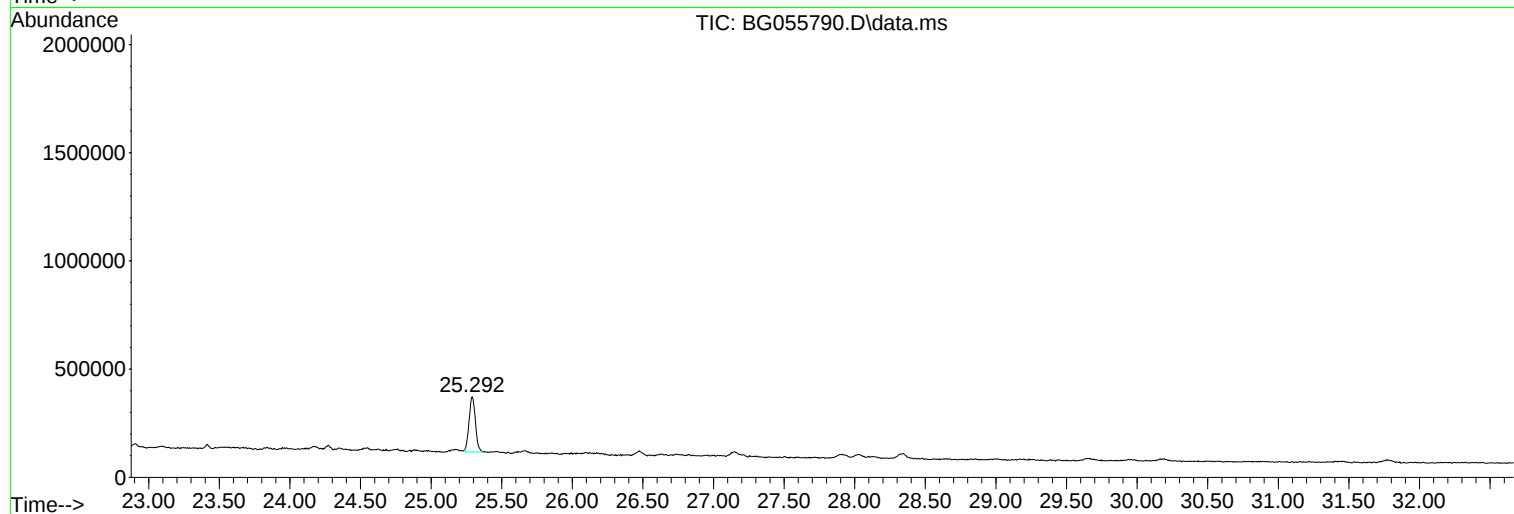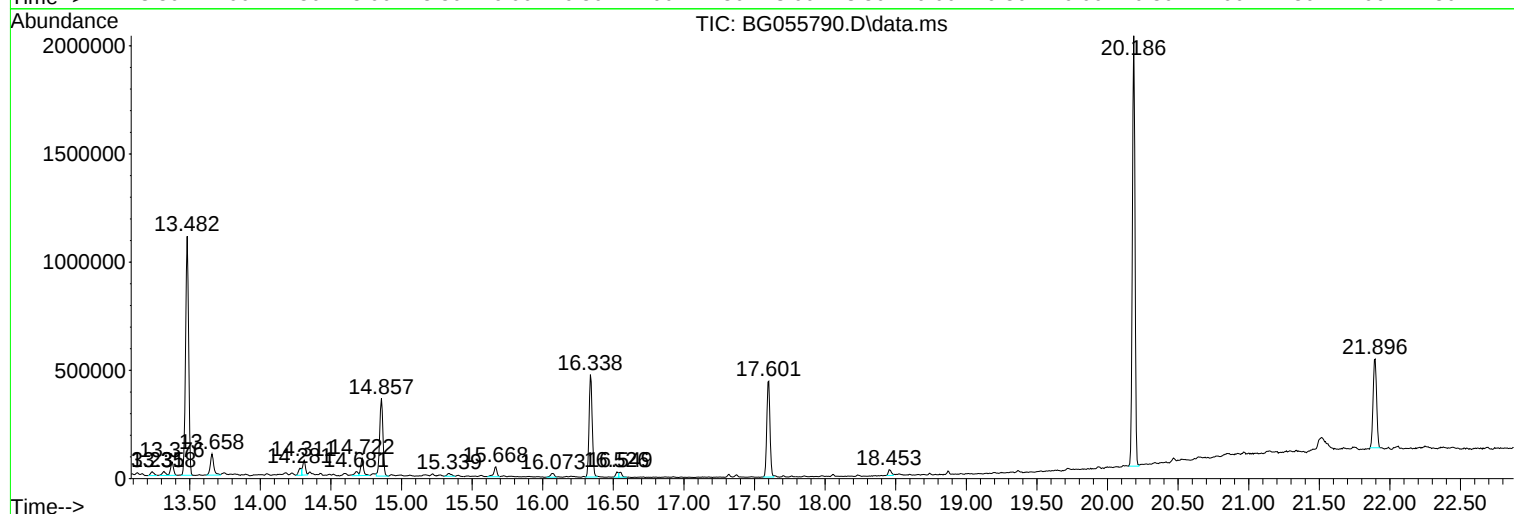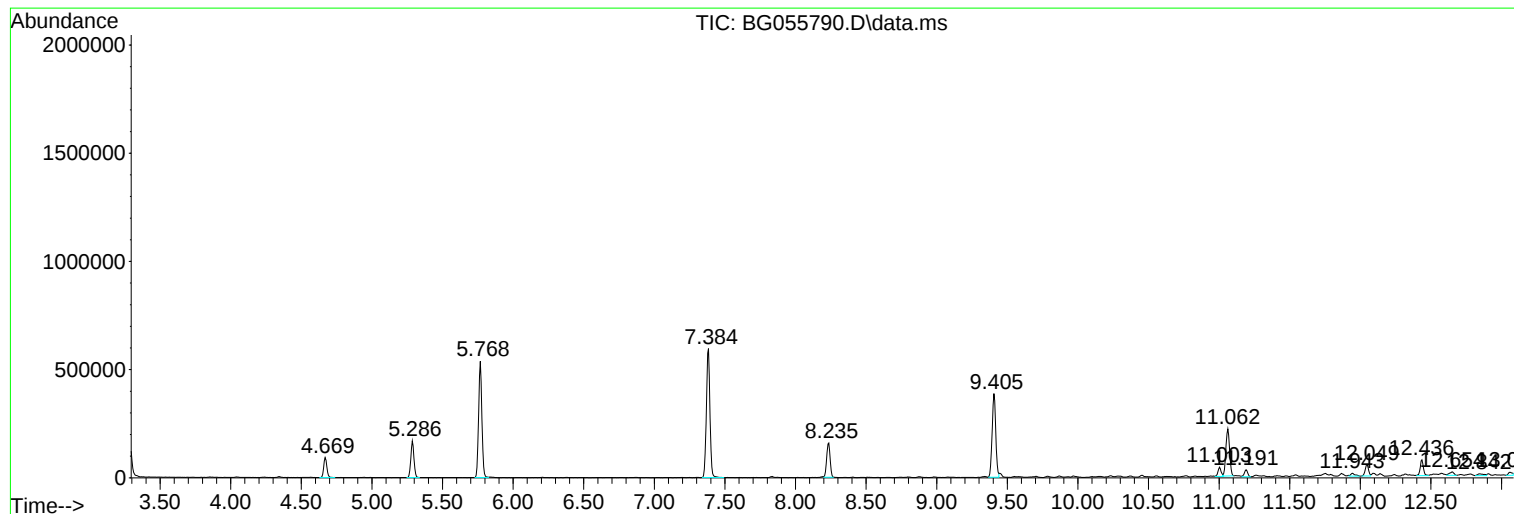

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112522\
Data File : BG055790.D
Acq On : 25 Nov 2022 21:25
Operator : CG/JU
Sample : N5769-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
COMP-218

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112522\
Data File : BG055790.D
Acq On : 25 Nov 2022 21:25
Operator : CG/JU
Sample : N5769-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
COMP-218

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------