


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112522\
 Data File : BG055774.D
 Acq On : 25 Nov 2022 10:00
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Nov 24 06:05:02 2022

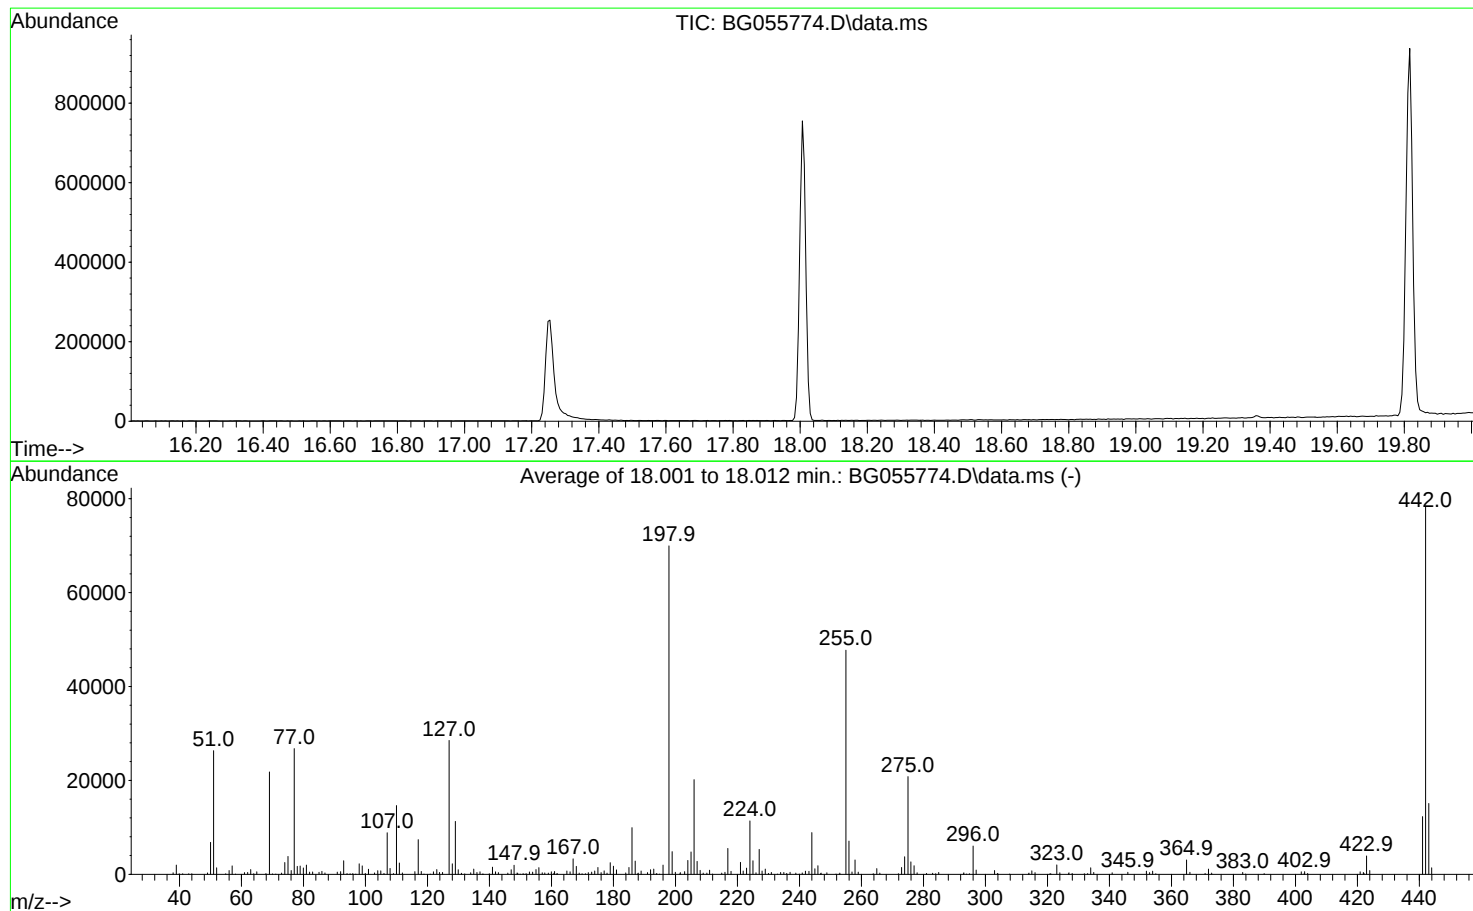




AutoFind: Scans 2504, 2505, 2506; Background Corrected with Scan 2498

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.6	26336	PASS
68	69	0.00	2	0.7	161	PASS
69	198	0.00	100	31.2	21808	PASS
70	69	0.00	2	0.3	73	PASS
127	198	10	80	40.7	28499	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	69971	PASS
199	198	5	9	6.9	4841	PASS
275	198	10	60	29.7	20797	PASS
365	198	1	100	4.4	3051	PASS
441	198	0.01	100	17.6	12304	PASS
442	442	50	100	100.0	78355	PASS
443	442	15	24	19.3	15089	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112522\
Data File : BG055774.D
Acq On : 25 Nov 2022 10:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 26 01:44:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 24 06:05:02 2022
Response via : Initial Calibration

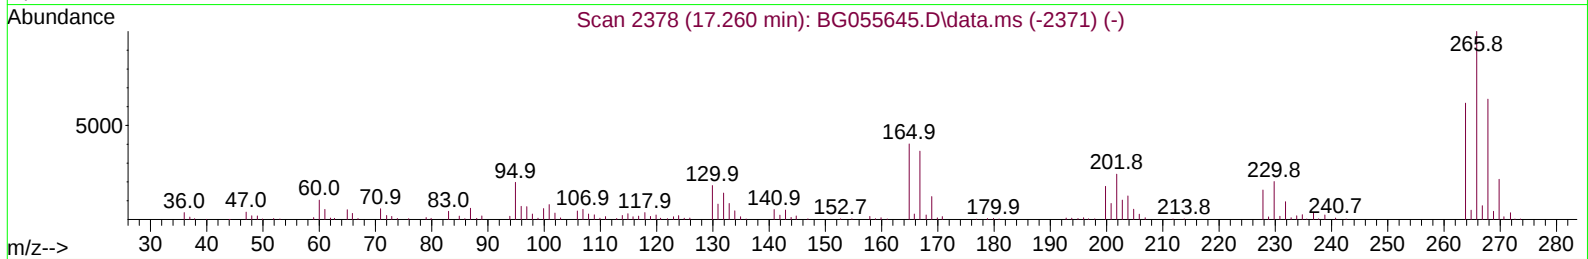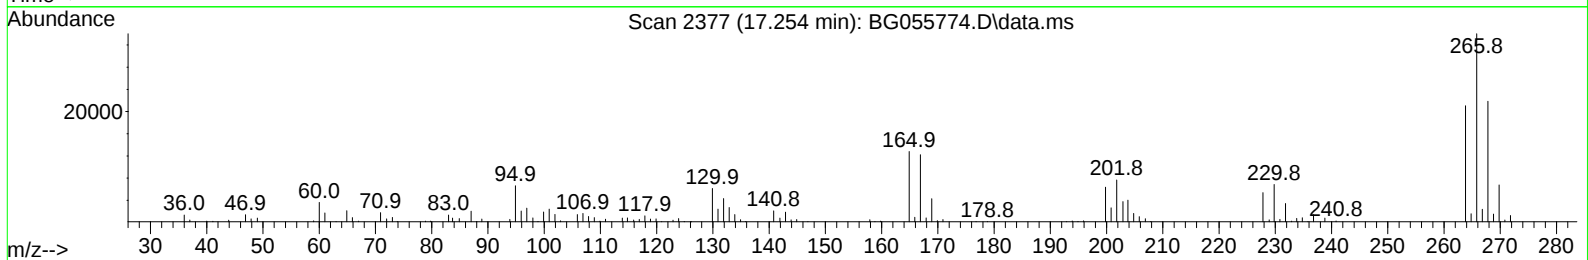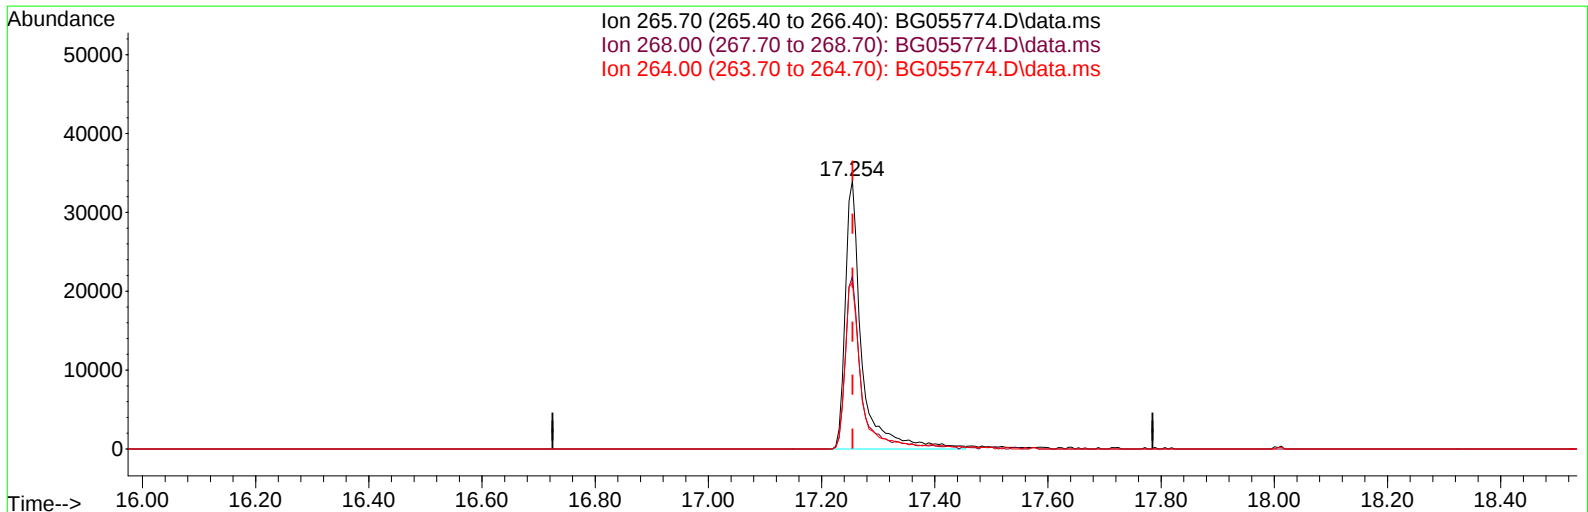

TIC: BG055774.D\data.ms

(70) Pentachlorophenol (C)

17.254min (0.000) 19259.57 ng




response 68768

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	64.23
264.00	61.90	61.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112522\
Data File : BG055774.D
Acq On : 25 Nov 2022 10:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 26 01:44:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 24 06:05:02 2022
Response via : Initial Calibration

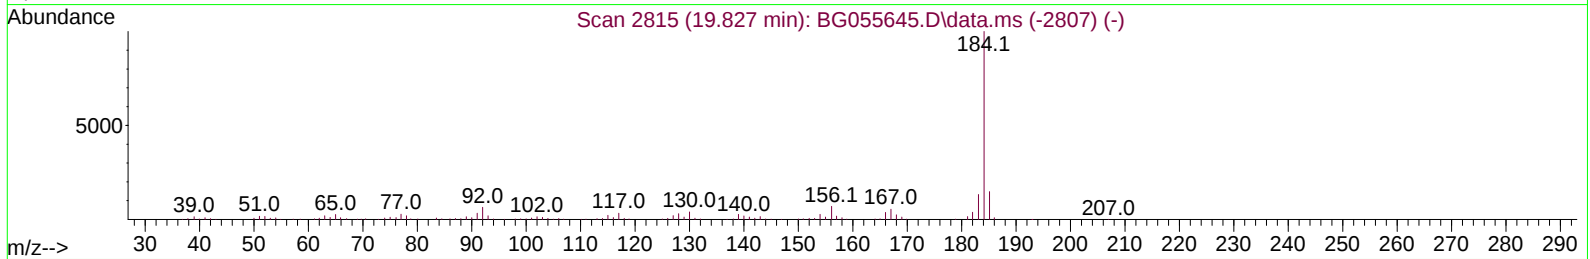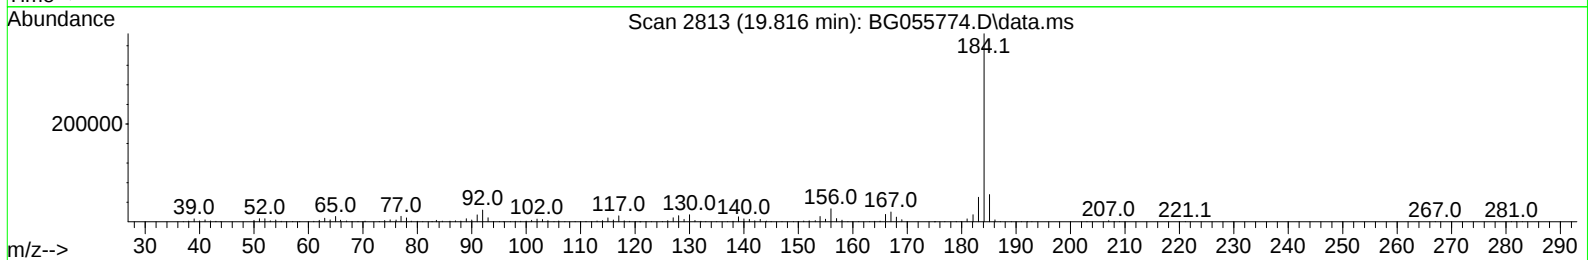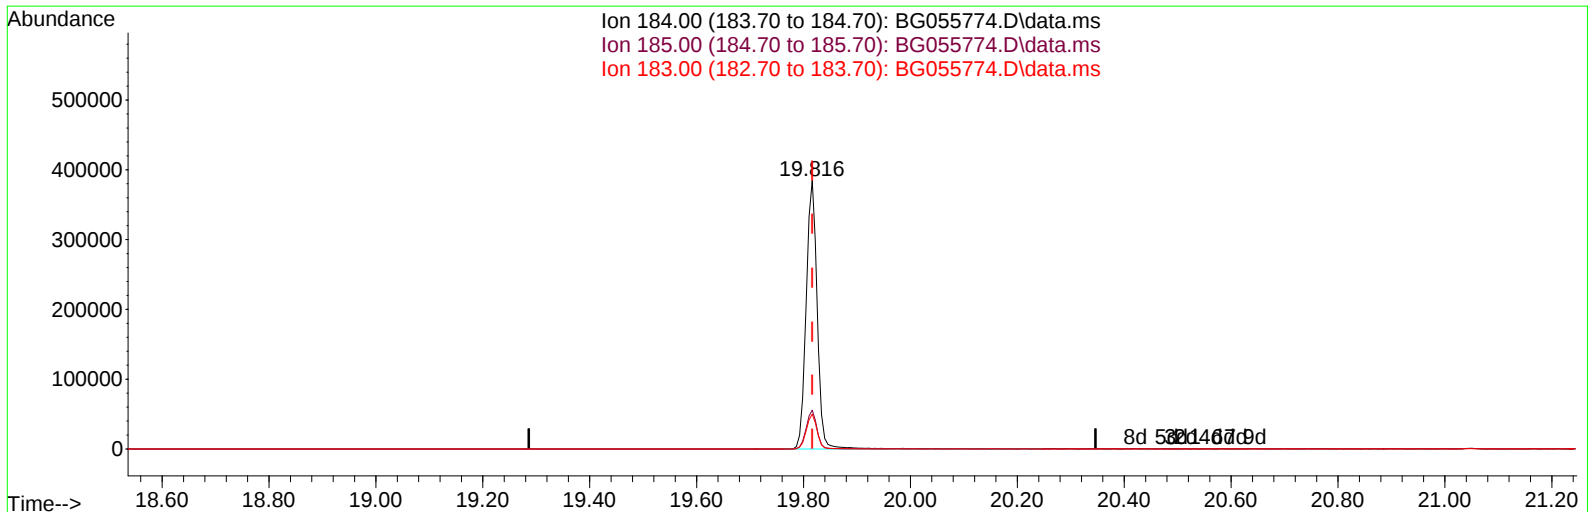

TIC: BG055774.D\data.ms

(77) Benzidine

19.816min (0.000) 451444.09 ng m

response 553528

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.49
183.00	13.20	13.00
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/25/2022	BNA_G	<u>BG055774.D</u>
Compound Name	Response	Retention Time
DDT	247143	21.05
DDD	3967	20.65
DDE	141	20.098
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4108	251251	1.64

Instrument :
BNA_G
ClientSampleId :
DFTPP