


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112522\
Data File : BG055780.D
Acq On : 25 Nov 2022 14:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Nov 24 06:05:02 2022

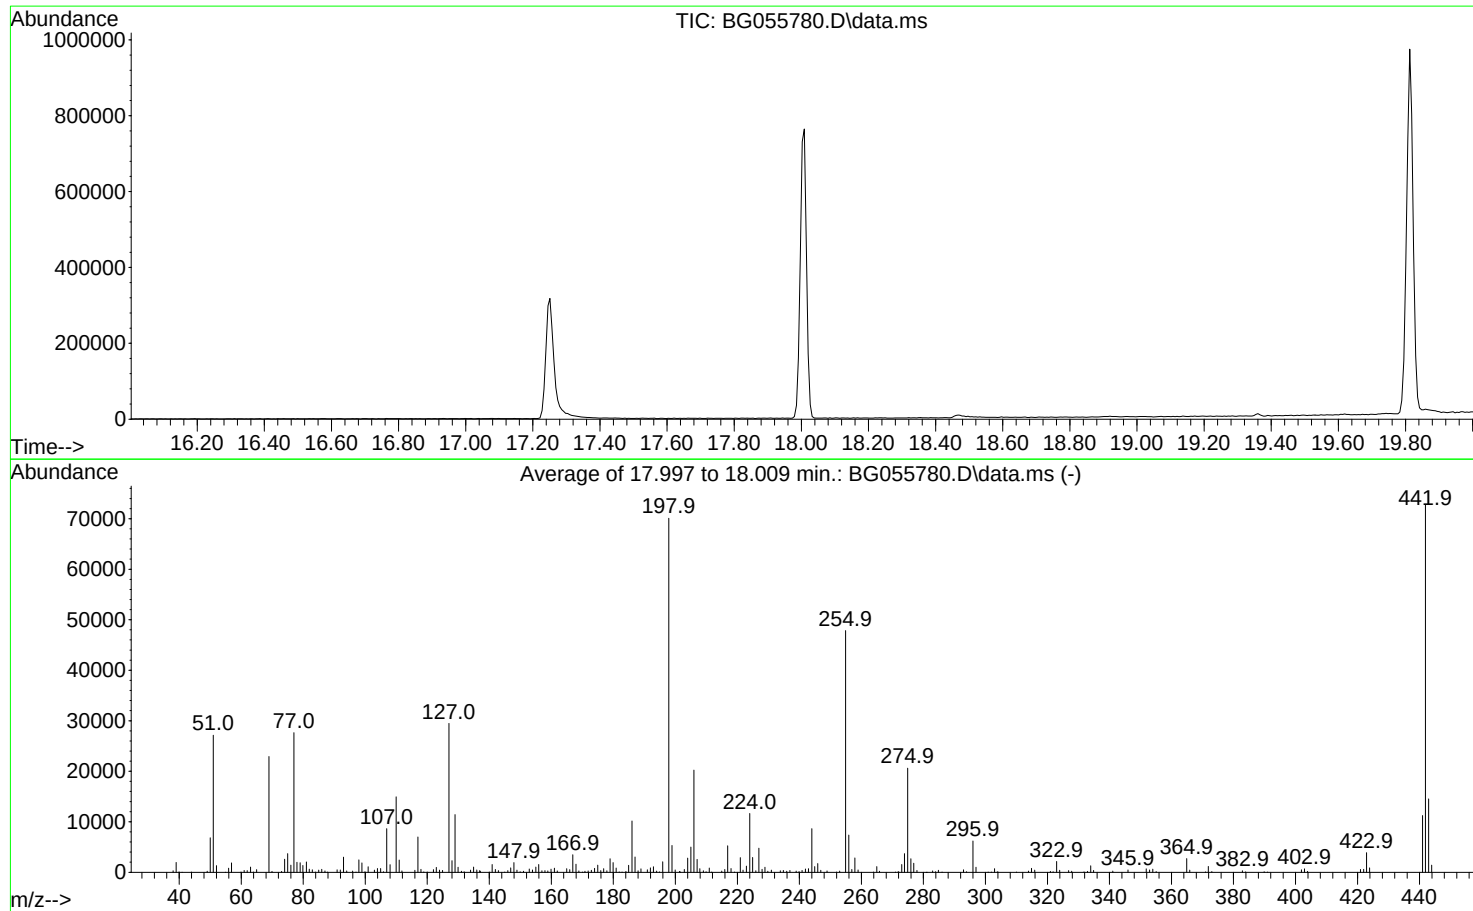




AutoFind: Scans 2503, 2504, 2505; Background Corrected with Scan 2497

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.7	27131	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	32.7	22928	PASS
70	69	0.00	2	0.8	180	PASS
127	198	10	80	42.1	29491	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	70099	PASS
199	198	5	9	7.6	5302	PASS
275	198	10	60	29.4	20612	PASS
365	198	1	100	3.9	2716	PASS
441	198	0.01	100	16.0	11236	PASS
442	442	50	100	100.0	72832	PASS
443	442	15	24	19.9	14521	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112522\
Data File : BG055780.D
Acq On : 25 Nov 2022 14:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 26 01:45:56 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 24 06:05:02 2022
Response via : Initial Calibration

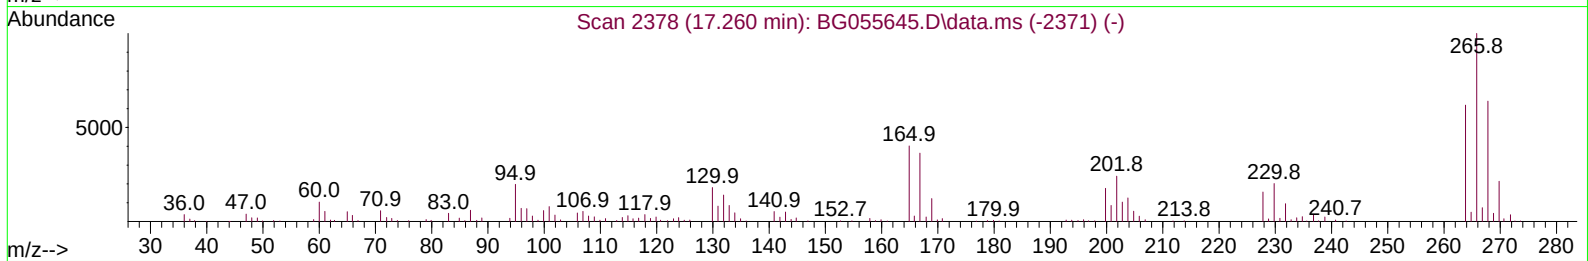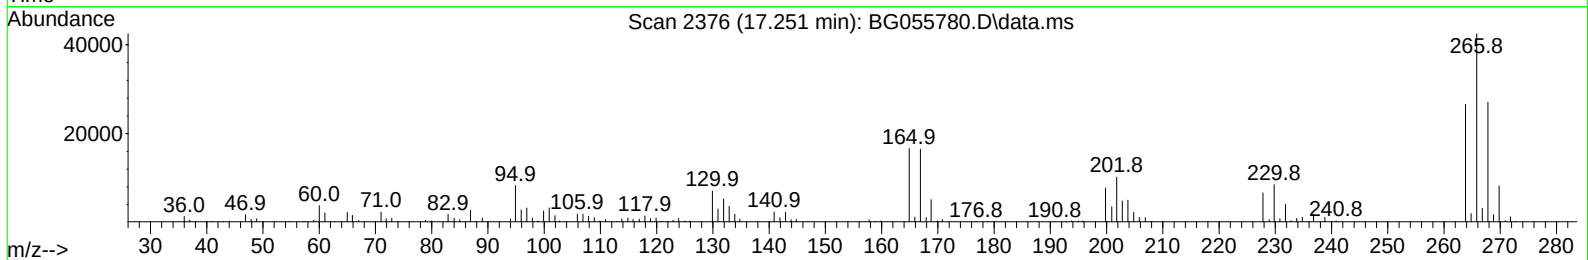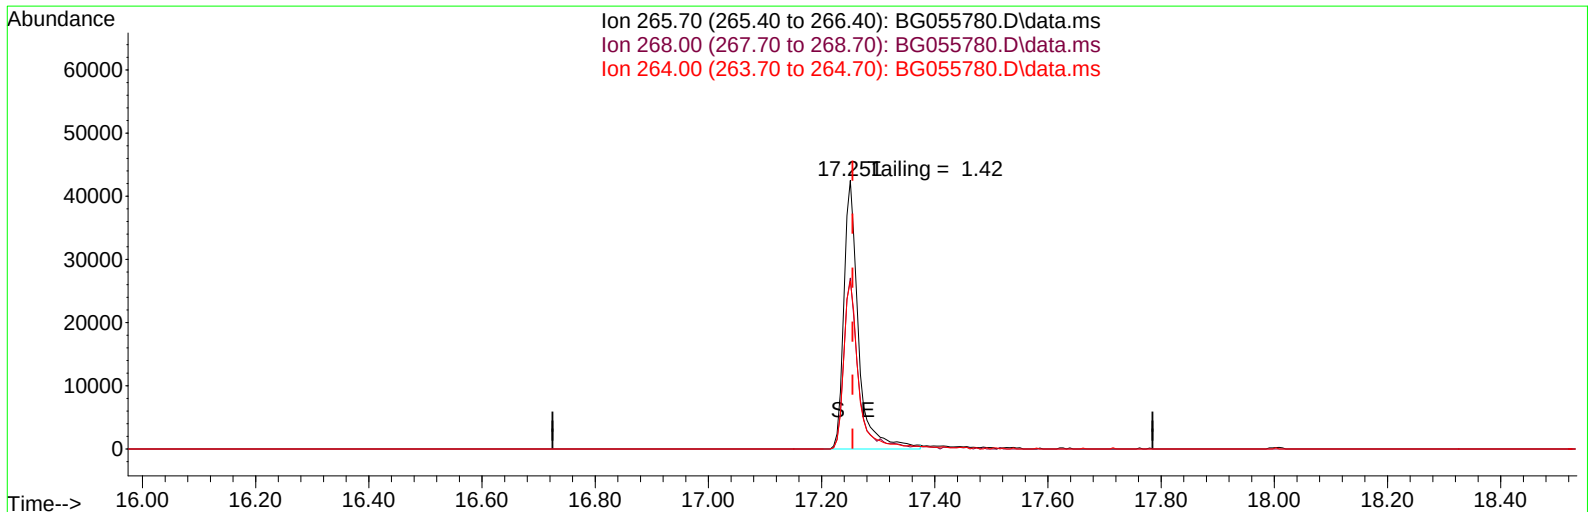

TIC: BG055780.D\data.ms

(70) Pentachlorophenol (C)

17.251min (-0.004) 23621.01 ng




response 76491

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	63.66
264.00	61.90	62.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112522\
Data File : BG055780.D
Acq On : 25 Nov 2022 14:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 26 01:45:56 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 24 06:05:02 2022
Response via : Initial Calibration

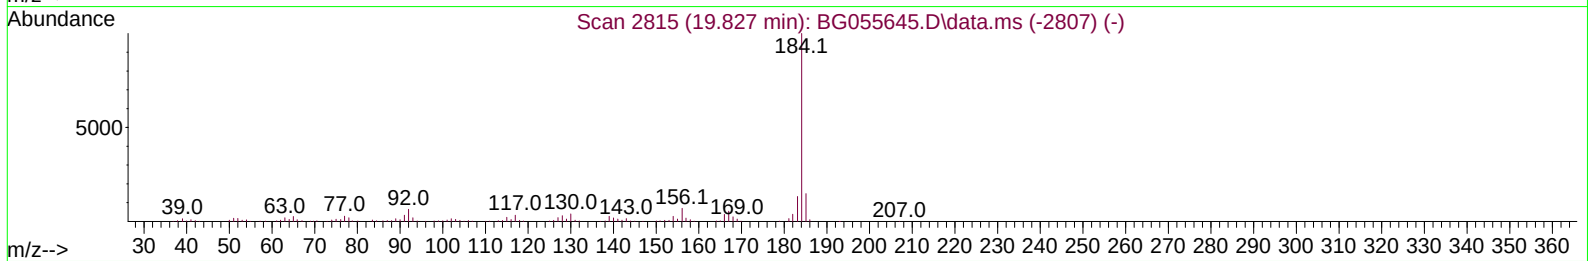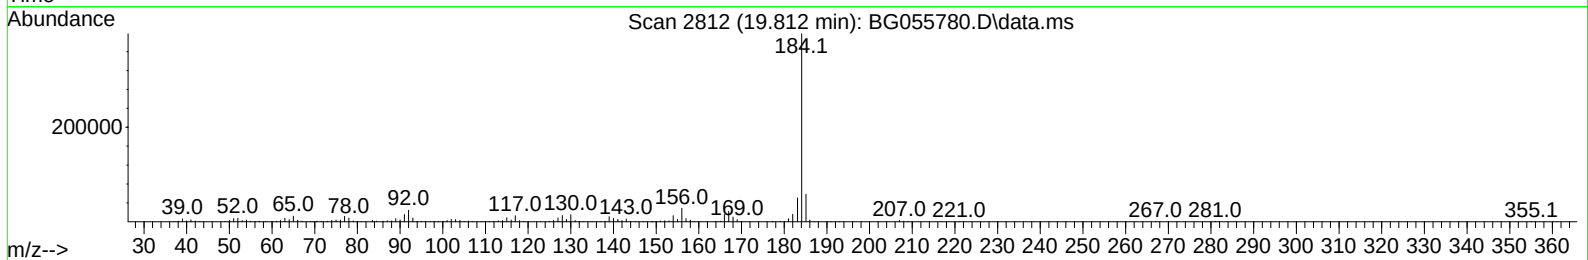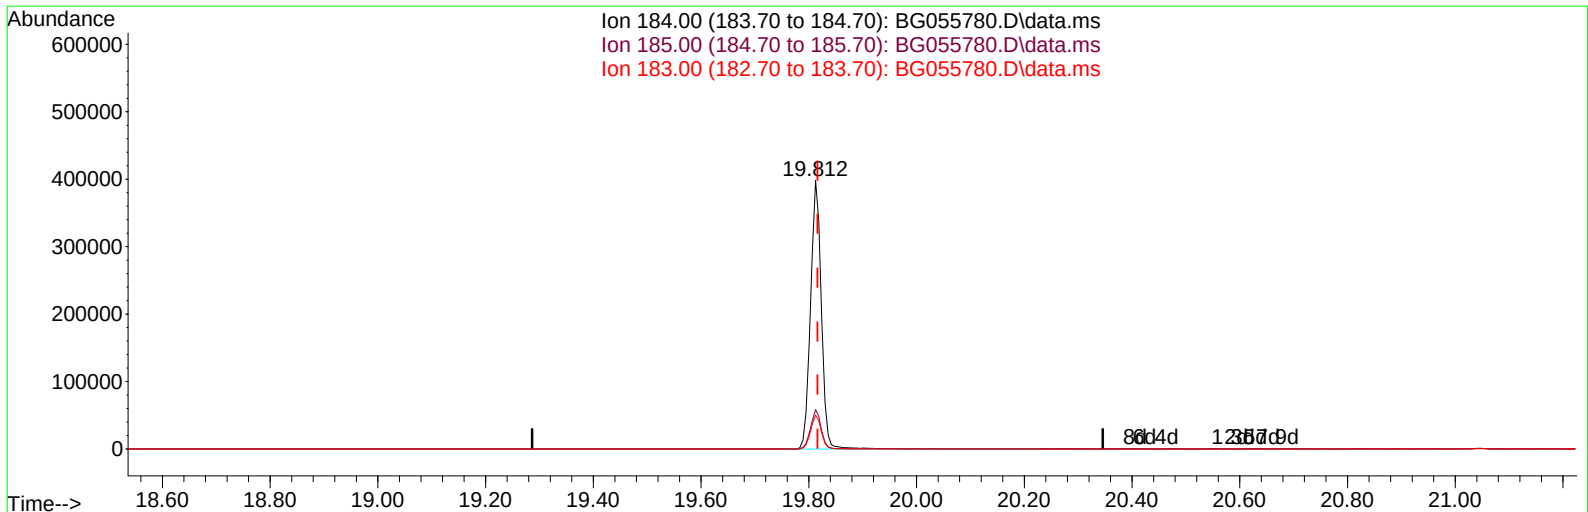

TIC: BG055780.D\data.ms

(77) Benzidine

19.812min (-0.004) 415453.91 ng m

response 557456

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.66
183.00	13.20	12.68
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/25/2022	BNA_G	BG055780.D
Compound Name	Response	Retention Time
DDT	264353	21.046
DDD	3909	20.653
DDE	53	20.089
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3962	268315	1.48

Instrument :
BNA_G
ClientSampleId :
DFTPP