




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112524\
Data File : BG063552.D
Acq On : 25 Nov 2024 16:33
Operator : RC/JU
Sample : PB165231BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK231

Manual IntegrationsAPPROVED

Quant Time: Nov 26 00:34:29 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 20 14:52:38 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/27/2024

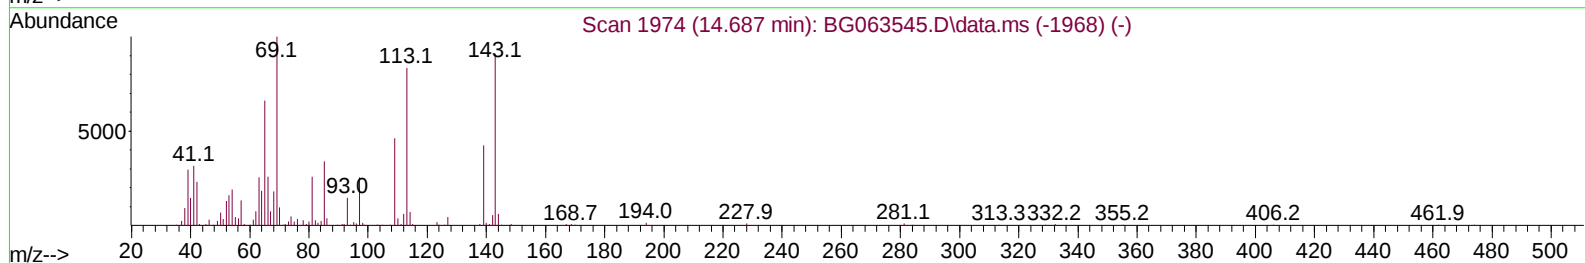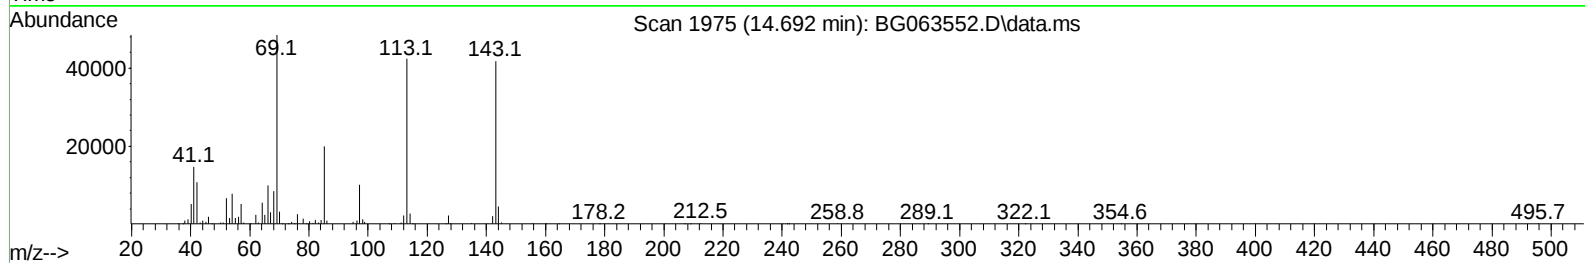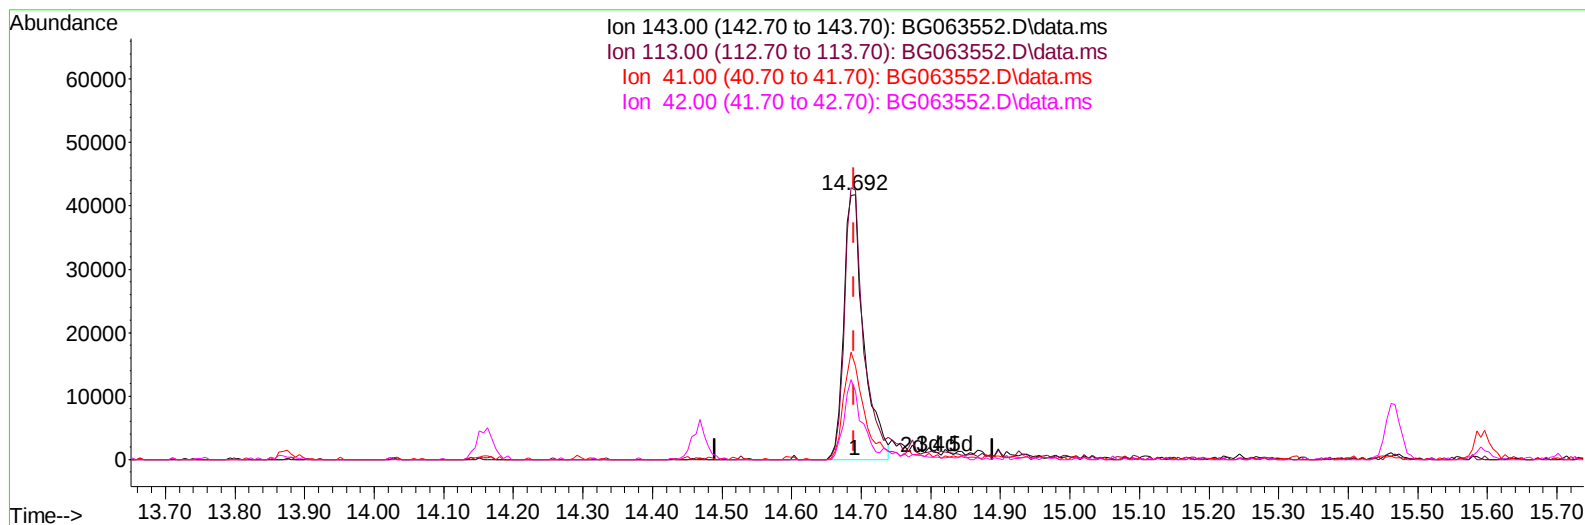

TIC: BG063552.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.692min (+ 0.002) 26.73 ng/u1

response 83253

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	103.10	101.49
41.00	38.80	35.29
42.00	26.30	25.72




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112524\
Data File : BG063552.D
Acq On : 25 Nov 2024 16:33
Operator : RC/JU
Sample : PB165231BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK231

Manual IntegrationsAPPROVED

Quant Time: Nov 26 00:34:29 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 20 14:52:38 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/27/2024

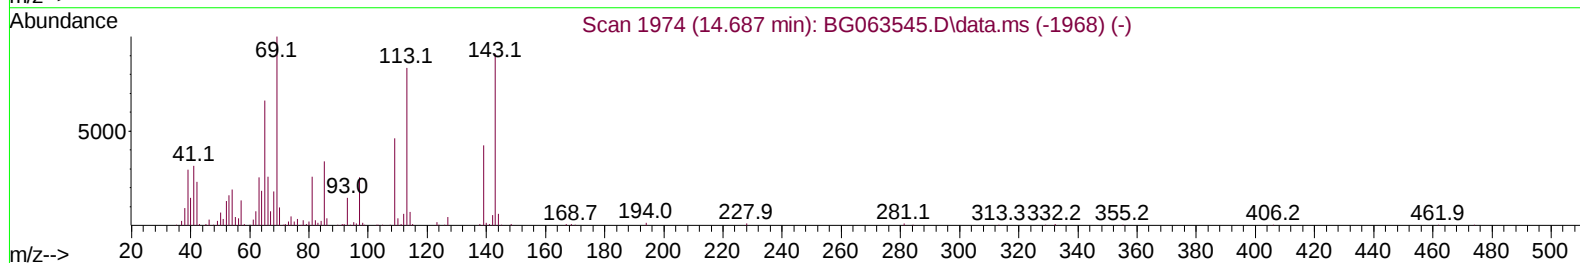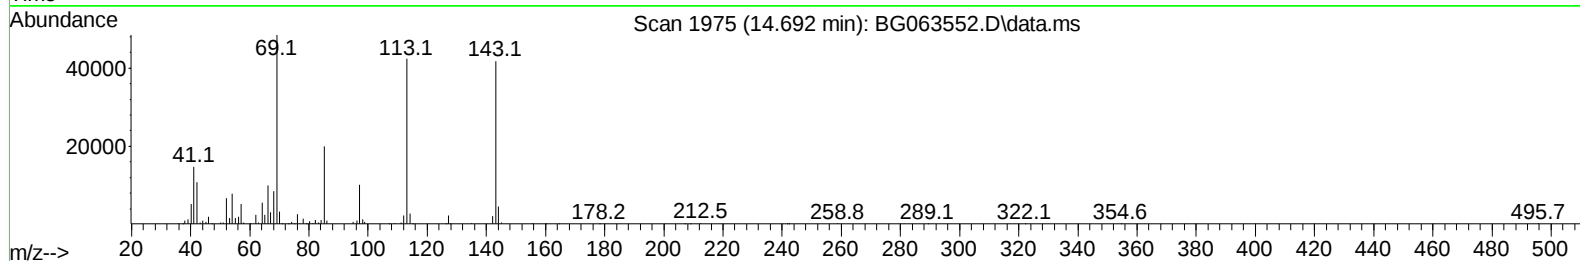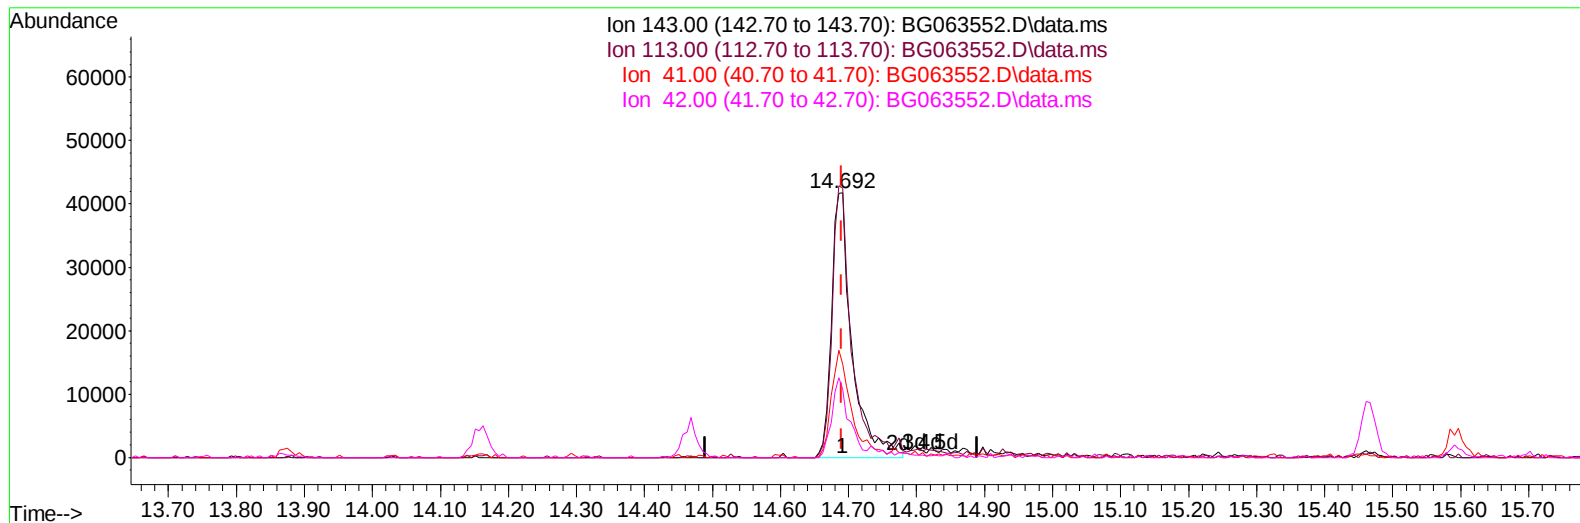

TIC: BG063552.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.692min (+ 0.002) 28.40 ng/ul m

response 88454

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	103.10	101.49
41.00	38.80	35.29
42.00	26.30	25.72

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112524\
 Data File : BG063552.D
 Acq On : 25 Nov 2024 16:33
 Operator : RC/JU
 Sample : PB165231BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK231

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/27/2024
 Supervised By :mohammad ahmed 11/27/2024

Quant Time: Nov 26 00:35:41 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 20 14:52:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.829	152	92541	20.000	ng/ul	0.00
20) Naphthalene-d8	10.614	136	386668	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.468	164	308767	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.224	188	780337	20.000	ng/ul	0.00
79) Chrysene-d12	21.478	240	850638	20.000	ng/ul	0.00
88) Perylene-d12	24.515	264	897028	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	14652	6.249	ng/uL	0.00
4) Pyridine-d5	3.699	84	191948	26.118	ng/ul	0.00
7) Phenol-d5	7.001	99	238605	31.350	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.159	67	153794	31.505	ng/ul	0.00
11) 2-Chlorophenol-d4	7.365	132	167644	31.081	ng/ul	0.00
15) 4-Methylphenol-d8	8.534	113	196839	30.949	ng/ul	0.00
21) Nitrobenzene-d5	8.981	128	90419	32.563	ng/ul	0.00
24) 2-Nitrophenol-d4	9.703	143	105162	30.657	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.244	165	193855	29.608	ng/ul	0.00
31) 4-Chloroaniline-d4	10.755	131	252068	30.438	ng/ul	0.00
46) Dimethylphthalate-d6	13.875	166	700131	33.402	ng/ul	0.00
49) Acenaphthylene-d8	14.157	160	769156	32.178	ng/ul	0.00
54) 4-Nitrophenol-d4	14.692	143	88454m	28.401	ng/ul	0.00
60) Fluorene-d10	15.461	176	645958	33.916	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.591	200	123939	28.251	ng/ul	0.00
73) Anthracene-d10	17.318	188	1144331	33.754	ng/ul	0.00
81) Pyrene-d10	19.621	212	1487401	34.883	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.310	264	1486077	34.155	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112524\
Data File : BG063552.D
Acq On : 25 Nov 2024 16:33
Operator : RC/JU
Sample : PB165231BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK231

Manual IntegrationsAPPROVED

Quant Time: Nov 26 00:35:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 20 14:52:38 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/27/2024

