

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112524\
 Data File : BG063546.D
 Acq On : 25 Nov 2024 10:28
 Operator : RC/JU
 Sample : PB165212BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK212

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063546.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.294	32	35	43	rVB	30984	41368	1.08%	0.124%
2	3.693	99	103	114	rBV	312562	543698	14.23%	1.625%
3	4.034	159	161	166	rVB2	13323	15283	0.40%	0.046%
4	4.398	220	223	224	rBV3	4643	4976	0.13%	0.015%
5	4.416	224	226	229	rVB3	5322	6574	0.17%	0.020%
6	7.001	658	666	675	rBV	417040	732543	19.17%	2.189%
7	7.154	684	692	702	rBV	326614	544336	14.24%	1.627%
8	7.360	720	727	736	rBV	411329	709134	18.56%	2.119%
9	7.824	800	806	813	rBV2	324038	540931	14.15%	1.617%
10	8.006	835	837	839	rBV	5918	5639	0.15%	0.017%
11	8.188	864	868	870	rVB3	4133	5641	0.15%	0.017%
12	8.535	919	927	936	rBV	544668	923514	24.16%	2.760%
13	8.981	995	1003	1013	rBV	411123	727753	19.04%	2.175%
14	9.704	1117	1126	1134	rBV	371551	670543	17.55%	2.004%
15	9.851	1150	1151	1154	rBV2	4858	5127	0.13%	0.015%
16	10.244	1212	1218	1230	rBV	531470	953852	24.96%	2.851%
17	10.615	1272	1281	1288	rBV	459704	823128	21.54%	2.460%
18	10.756	1298	1305	1315	rBV	464569	904406	23.66%	2.703%
19	10.938	1333	1336	1339	rBV2	5098	6954	0.18%	0.021%
20	11.261	1388	1391	1395	rVB3	3820	5418	0.14%	0.016%
21	11.654	1455	1458	1461	rBV2	4353	5974	0.16%	0.018%
22	12.224	1551	1555	1557	rBV3	4733	6233	0.16%	0.019%
23	13.258	1725	1731	1735	rVB3	4446	10147	0.27%	0.030%
24	13.370	1747	1750	1752	rBV	3980	5448	0.14%	0.016%
25	13.564	1780	1783	1786	rVB	4216	5081	0.13%	0.015%
26	13.593	1786	1788	1792	rBV3	4339	5906	0.15%	0.018%
27	13.875	1829	1836	1845	rBV	1033959	1507688	39.45%	4.506%
28	14.163	1877	1885	1895	rBV	1092808	1751090	45.82%	5.234%
29	14.469	1930	1937	1944	rBV	796790	1226748	32.10%	3.667%
30	14.686	1968	1974	1990	rBV	313690	648229	16.96%	1.937%
31	14.915	2010	2013	2015	rBV4	4752	5717	0.15%	0.017%
32	15.080	2038	2041	2044	rBV3	5429	6093	0.16%	0.018%
33	15.215	2063	2064	2069	rVB2	4003	5829	0.15%	0.017%
34	15.256	2069	2071	2075	rBV3	4846	6720	0.18%	0.020%
35	15.468	2098	2107	2115	rBV	1567692	2311939	60.49%	6.910%
36	15.597	2122	2129	2138	rBV	443549	717363	18.77%	2.144%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112524\
 Data File : BG063546.D
 Acq On : 25 Nov 2024 10:28
 Operator : RC/JU
 Sample : PB165212BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK212

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
 Title : SVOA CALIBRATION

37	15.985	2192	2195	2197	rBV3	8177	8439	0.22%	0.025%
38	16.249	2236	2240	2241	rBV2	5913	6856	0.18%	0.020%
39	16.513	2283	2285	2288	rVB3	6610	4905	0.13%	0.015%
40	16.560	2291	2293	2298	rVV2	4107	6280	0.16%	0.019%
41	16.613	2300	2302	2305	rBV2	5235	7161	0.19%	0.021%
42	16.966	2357	2362	2363	rBV2	5119	5601	0.15%	0.017%
43	17.224	2398	2406	2414	rBV	1143373	1722178	45.06%	5.147%
44	17.324	2416	2423	2437	rVB	1897500	2837476	74.25%	8.481%
45	17.583	2464	2467	2470	rBV	6069	8275	0.22%	0.025%
46	17.771	2494	2499	2500	rVB3	4651	5460	0.14%	0.016%
47	17.894	2515	2520	2526	rVB5	10581	14360	0.38%	0.043%
48	18.670	2650	2652	2655	rVB2	5546	6350	0.17%	0.019%
49	18.734	2660	2663	2665	rBV5	5350	6844	0.18%	0.020%
50	18.823	2675	2678	2680	rBV4	4878	6427	0.17%	0.019%
51	18.981	2702	2705	2709	rBV3	5120	8249	0.22%	0.025%
52	19.181	2735	2739	2746	rBV2	30824	48740	1.28%	0.146%
53	19.257	2748	2752	2756	rBV2	28824	43194	1.13%	0.129%
54	19.557	2799	2803	2807	rBV6	9685	16272	0.43%	0.049%
55	19.622	2808	2814	2820	rBV	2537623	3707356	97.01%	11.081%
56	19.833	2848	2850	2852	rBV3	5433	4985	0.13%	0.015%
57	19.886	2857	2859	2860	rBV2	9353	6046	0.16%	0.018%
58	20.691	2994	2996	2998	rBV3	9841	5564	0.15%	0.017%
59	21.484	3124	3131	3143	rBV	1383316	2269496	59.38%	6.783%
60	22.595	3316	3320	3325	rVB6	73312	126952	3.32%	0.379%
61	24.316	3603	3613	3628	rVB	1508565	3821749	100.00%	11.423%
62	24.528	3639	3649	3662	rVB	857510	2355423	61.63%	7.040%




Sum of corrected areas: 33457661

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112524\
Data File : BG063546.D
Acq On : 25 Nov 2024 10:28
Operator : RC/JU
Sample : PB165212BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK212

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

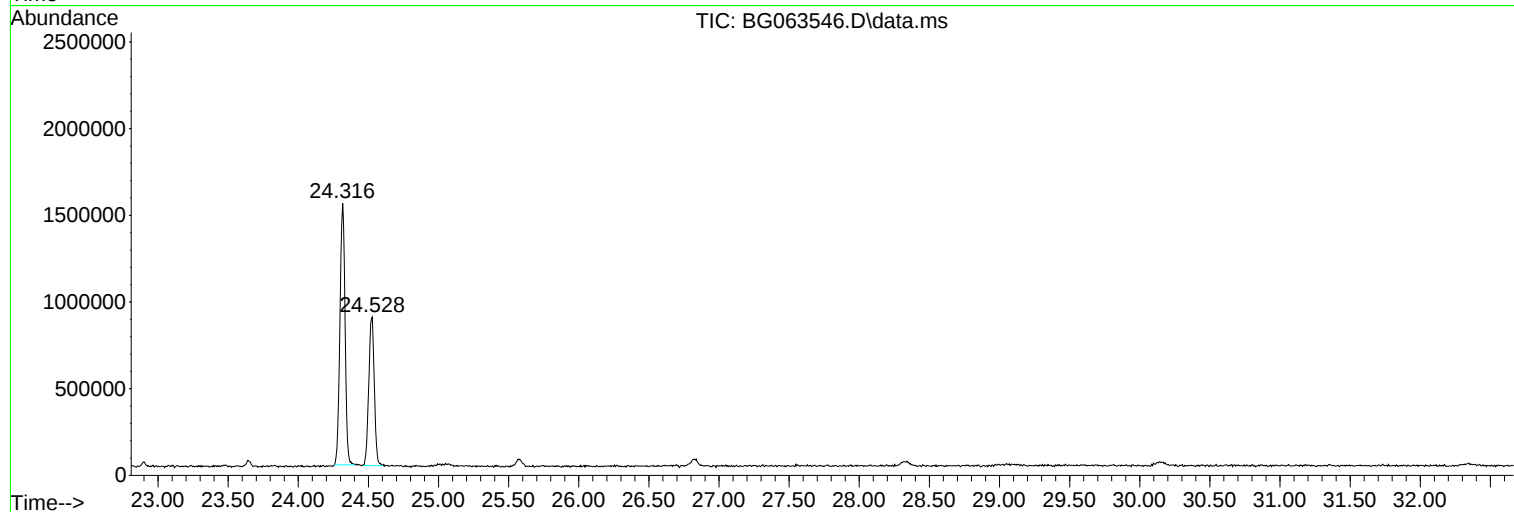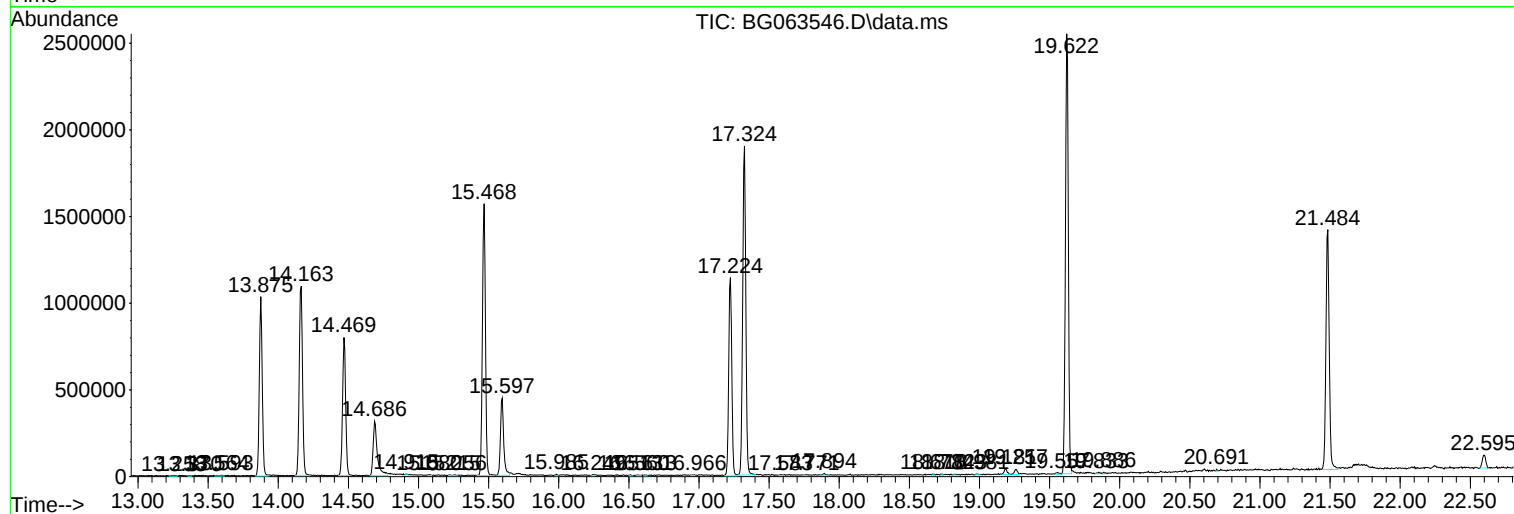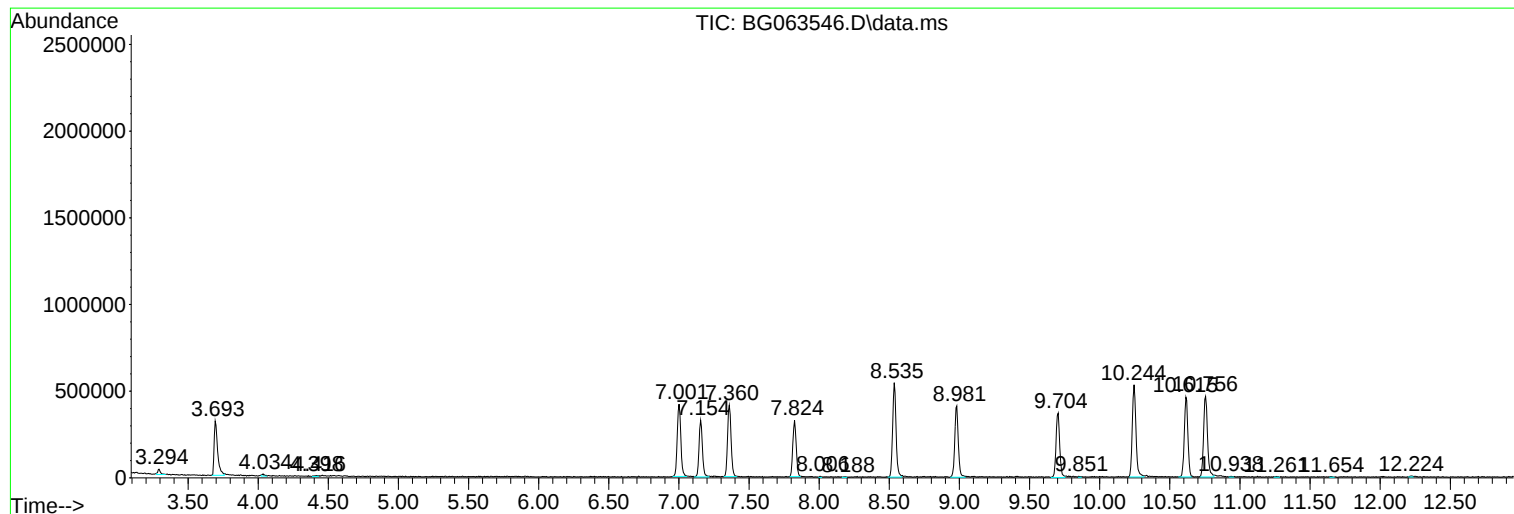

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112524\
Data File : BG063546.D
Acq On : 25 Nov 2024 10:28
Operator : RC/JU
Sample : PB165212BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK212

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112524\
Data File : BG063546.D
Acq On : 25 Nov 2024 10:28
Operator : RC/JU
Sample : PB165212BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK212

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc