

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112524\
 Data File : BG063551.D
 Acq On : 25 Nov 2024 15:52
 Operator : RC/JU
 Sample : P4965-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E1PJ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063551.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.293	31	35	39	rVB2	19633	26353	0.60%	0.076%
2	3.564	79	81	87	rVB	11655	10566	0.24%	0.031%
3	3.699	100	104	113	rBV	85594	149255	3.41%	0.432%
4	4.034	157	161	165	rBV2	40385	56810	1.30%	0.165%
5	4.474	231	236	240	rBV3	17300	27181	0.62%	0.079%
6	4.933	311	314	317	rVB5	6424	6192	0.14%	0.018%
7	5.661	437	438	443	rBV5	5030	6118	0.14%	0.018%
8	7.001	655	666	676	rVB	118156	230522	5.26%	0.668%
9	7.154	686	692	701	rBV	344283	560626	12.79%	1.624%
10	7.359	720	727	737	rBV	390493	658033	15.01%	1.907%
11	7.823	800	806	813	rBV	344700	556532	12.70%	1.613%
12	8.534	921	927	938	rBV	342247	585847	13.37%	1.698%
13	8.981	996	1003	1013	rBV	434846	785151	17.91%	2.275%
14	9.410	1074	1076	1079	rVB2	9948	6462	0.15%	0.019%
15	9.704	1118	1126	1135	rBV	397197	714736	16.31%	2.071%
16	10.244	1210	1218	1227	rBV2	563095	1007499	22.99%	2.919%
17	10.614	1271	1281	1289	rBV	464295	822848	18.78%	2.384%
18	10.755	1297	1305	1316	rBV2	429099	812818	18.55%	2.355%
19	11.384	1406	1412	1413	rBV2	5596	7959	0.18%	0.023%
20	11.419	1416	1418	1423	rVB4	5630	8075	0.18%	0.023%
21	11.913	1498	1502	1504	rVB4	6891	10117	0.23%	0.029%
22	12.212	1549	1553	1555	rBV3	9630	13472	0.31%	0.039%
23	12.671	1626	1631	1633	rVB2	5109	6406	0.15%	0.019%
24	12.724	1638	1640	1644	rBV2	4516	6289	0.14%	0.018%
25	13.311	1734	1740	1746	rVB2	42870	63564	1.45%	0.184%
26	13.875	1829	1836	1844	rBV	1182483	1680749	38.35%	4.870%
27	14.163	1875	1885	1893	rBV	1245410	1993541	45.49%	5.777%
28	14.469	1930	1937	1946	rBV2	802737	1251597	28.56%	3.627%
29	14.698	1969	1976	1986	rBV4	74999	186724	4.26%	0.541%
30	14.892	2005	2009	2010	rBV3	7382	7244	0.17%	0.021%
31	15.062	2036	2038	2042	rBV4	4465	6545	0.15%	0.019%
32	15.338	2080	2085	2086	rBV4	4962	7050	0.16%	0.020%
33	15.467	2100	2107	2117	rBV	1786843	2677414	61.09%	7.758%
34	15.591	2122	2128	2137	rBV	601543	925156	21.11%	2.681%
35	15.708	2145	2148	2151	rBV4	10260	10785	0.25%	0.031%
36	15.826	2167	2168	2173	rVB3	10290	12656	0.29%	0.037%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112524\
 Data File : BG063551.D
 Acq On : 25 Nov 2024 15:52
 Operator : RC/JU
 Sample : P4965-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E1PJ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
 Title : SVOA CALIBRATION

37	16.090	2210	2213	2218	rVB3	8472	14738	0.34%	0.043%
38	16.255	2238	2241	2244	rVB4	5350	6996	0.16%	0.020%
39	16.425	2268	2270	2276	rVB4	3275	6265	0.14%	0.018%
40	16.713	2317	2319	2323	rVB3	4542	6263	0.14%	0.018%
41	17.224	2399	2406	2412	rBV	1170780	1725789	39.38%	5.001%
42	17.324	2416	2423	2430	rVV	2284196	3383576	77.20%	9.804%
43	17.618	2471	2473	2476	rVB3	9077	9521	0.22%	0.028%
44	17.894	2517	2520	2524	rVB6	10203	13340	0.30%	0.039%
45	18.476	2618	2619	2622	rBV3	7754	8720	0.20%	0.025%
46	18.693	2654	2656	2660	rBV5	6599	6717	0.15%	0.019%
47	18.887	2687	2689	2692	rBV4	6816	6918	0.16%	0.020%
48	19.040	2711	2715	2718	rBV5	9635	16976	0.39%	0.049%
49	19.181	2736	2739	2747	rVB6	38008	59583	1.36%	0.173%
50	19.257	2749	2752	2757	rVB	35138	50123	1.14%	0.145%
51	19.621	2808	2814	2821	rBV	3131356	4382651	100.00%	12.699%
52	21.478	3124	3130	3144	rVB2	1387259	2260755	51.58%	6.551%
53	24.310	3602	3612	3625	rBV	1647244	4363203	99.56%	12.643%
54	24.516	3639	3647	3660	rVB	860749	2290176	52.26%	6.636%




Sum of corrected areas: 34511202

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112524\
Data File : BG063551.D
Acq On : 25 Nov 2024 15:52
Operator : RC/JU
Sample : P4965-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E1PJ0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

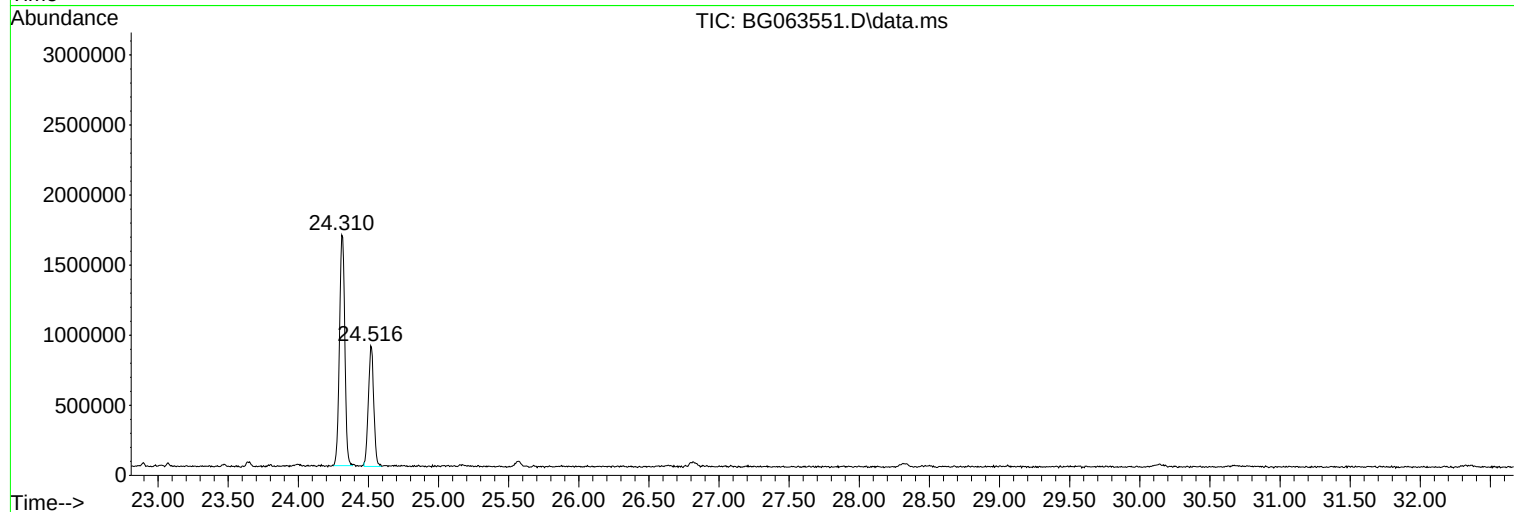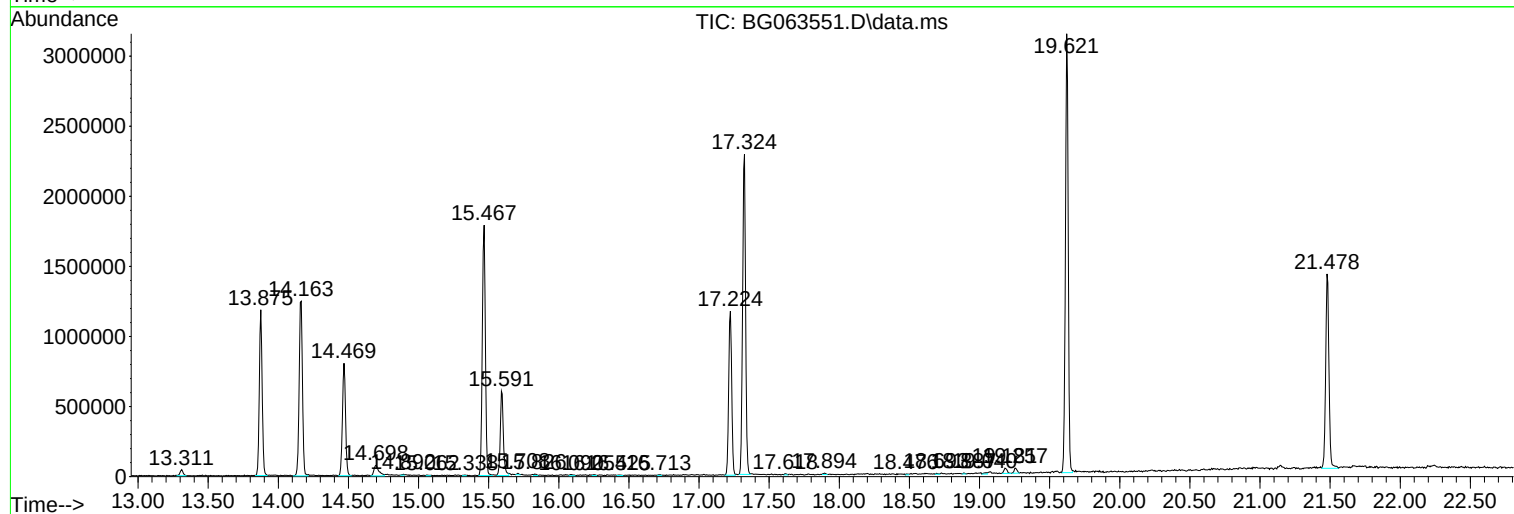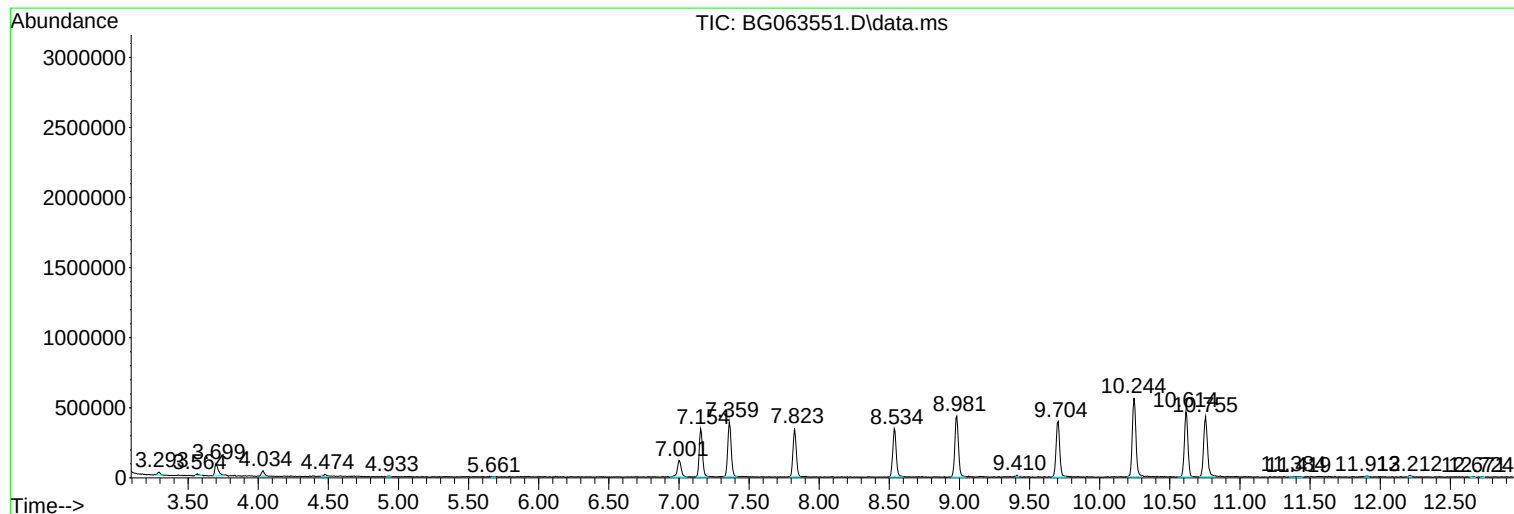

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112524\
Data File : BG063551.D
Acq On : 25 Nov 2024 15:52
Operator : RC/JU
Sample : P4965-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E1PJ0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112524\
Data File : BG063551.D
Acq On : 25 Nov 2024 15:52
Operator : RC/JU
Sample : P4965-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E1PJ0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------