
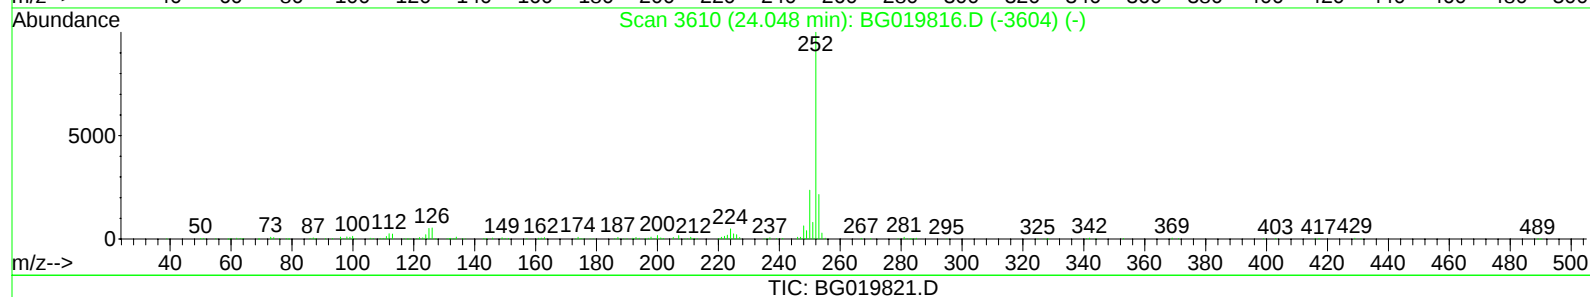
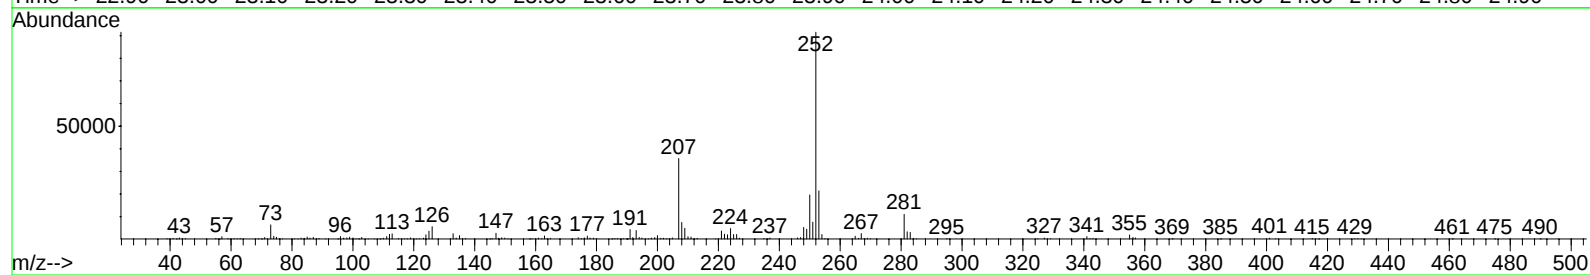


Data Path : Z:\HPCHEM1\BNA G\Data\BG112615\
Data File : BG019821.D
Acq On : 26 Nov 2015 12:00
Operator : UM/NP
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Nov 26 17:01:31 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG111615.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Nov 26 00:35:50 2015
Response via : Initial Calibration

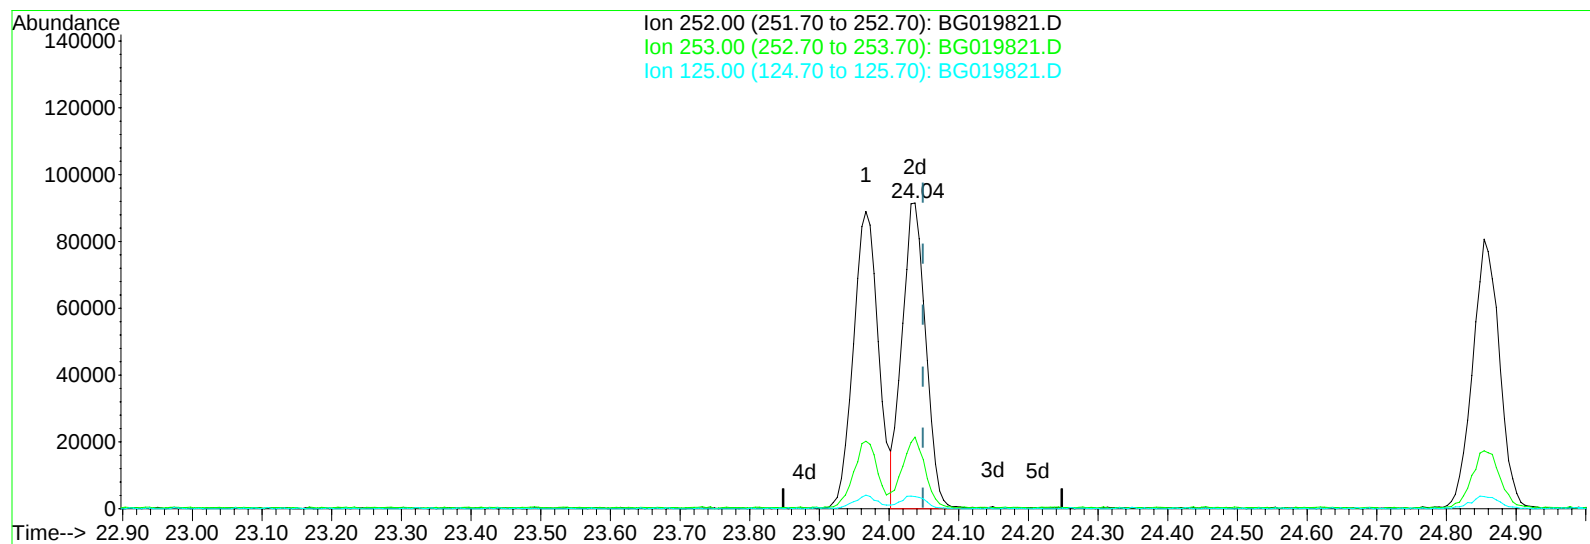

(89) Benzo(k)fluoranthene




24.037min (-0.011) 19.44ng/ul m

response 215147

Ion	Exp%	Act%
252.00	100	100
253.00	21.40	23.45
125.00	5.50	3.99#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\Data\BG112615\
Data File : BG019821.D
Acq On : 26 Nov 2015 12:00
Operator : UM/NP
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Nov 26 17:01:31 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG111615.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Nov 26 00:35:50 2015
Response via : Initial Calibration

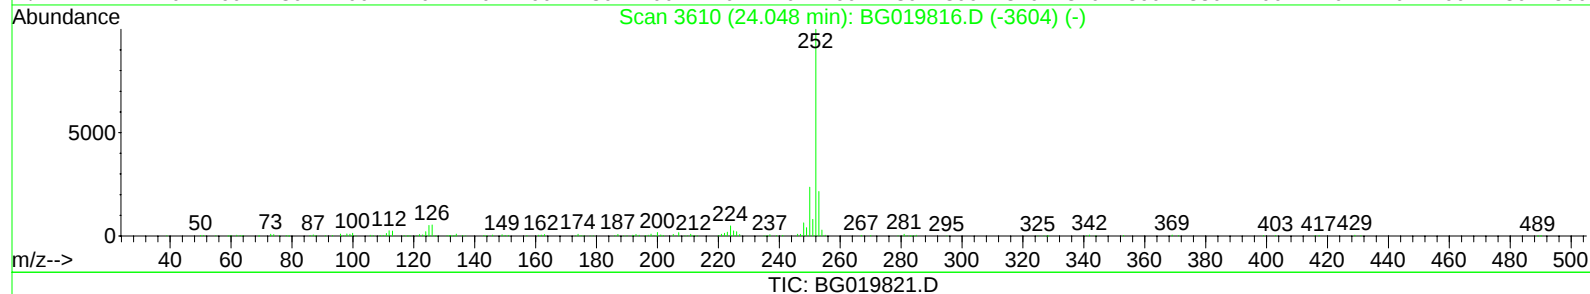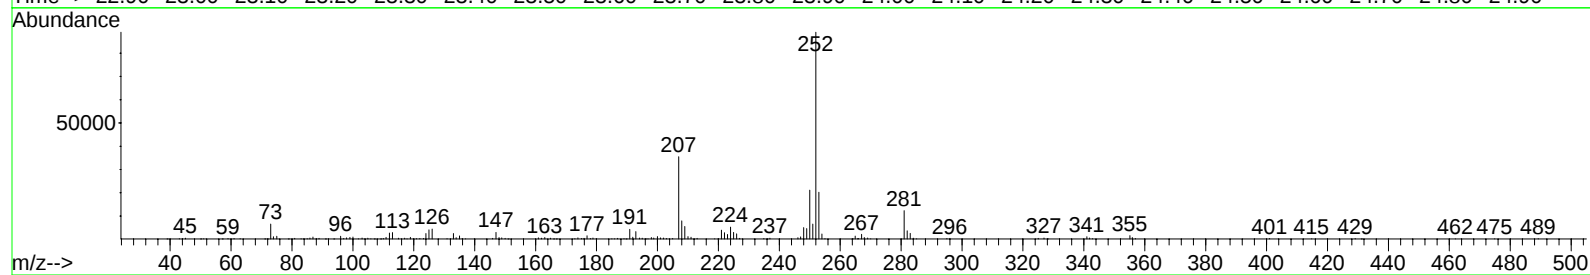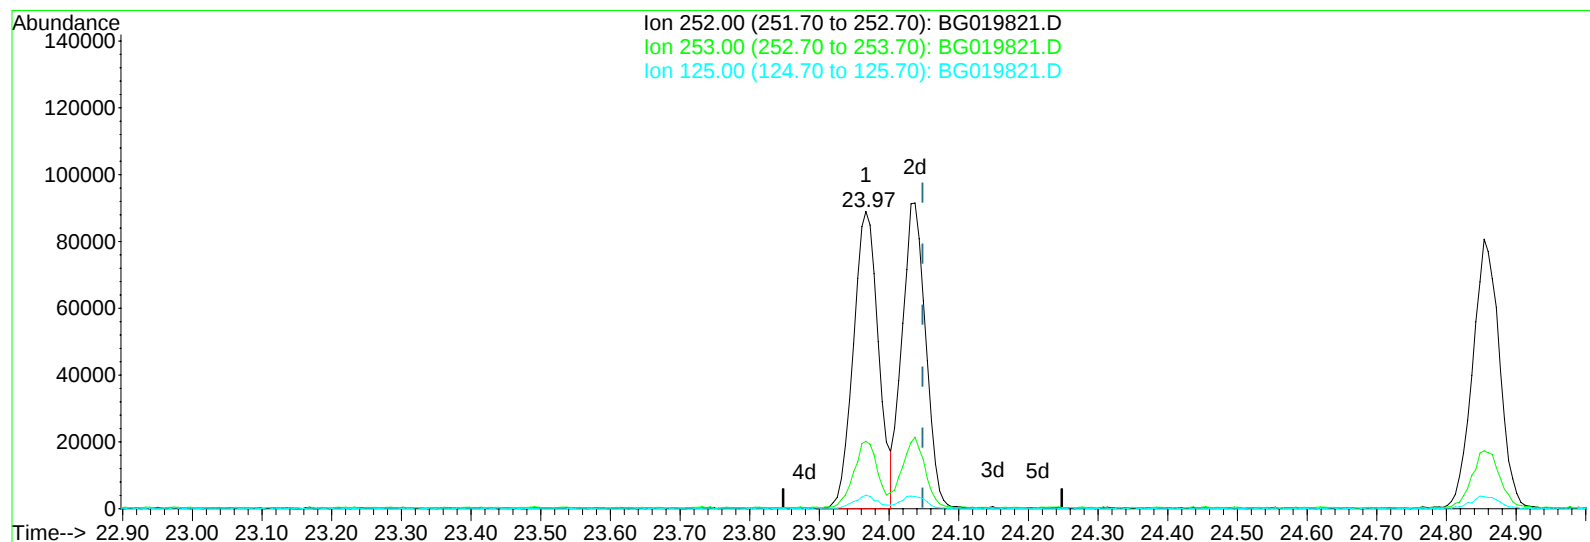

(89) Benzo(k)fluoranthene

23.967min (-0.081) 20.16ng/ul

response 223135

Ion	Exp%	Act%
252.00	100	100
253.00	21.40	22.70
125.00	5.50	4.61
0.00	0.00	0.00