


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG112615\
 Data File : BG019820.D
 Acq On : 26 Nov 2015 10:04
 Operator : UM/NP
 Sample : DFTPP03
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP03

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG111615.M
 Title : SVOA CALIBRATION
 Last Update : Thu Nov 26 00:35:50 2015

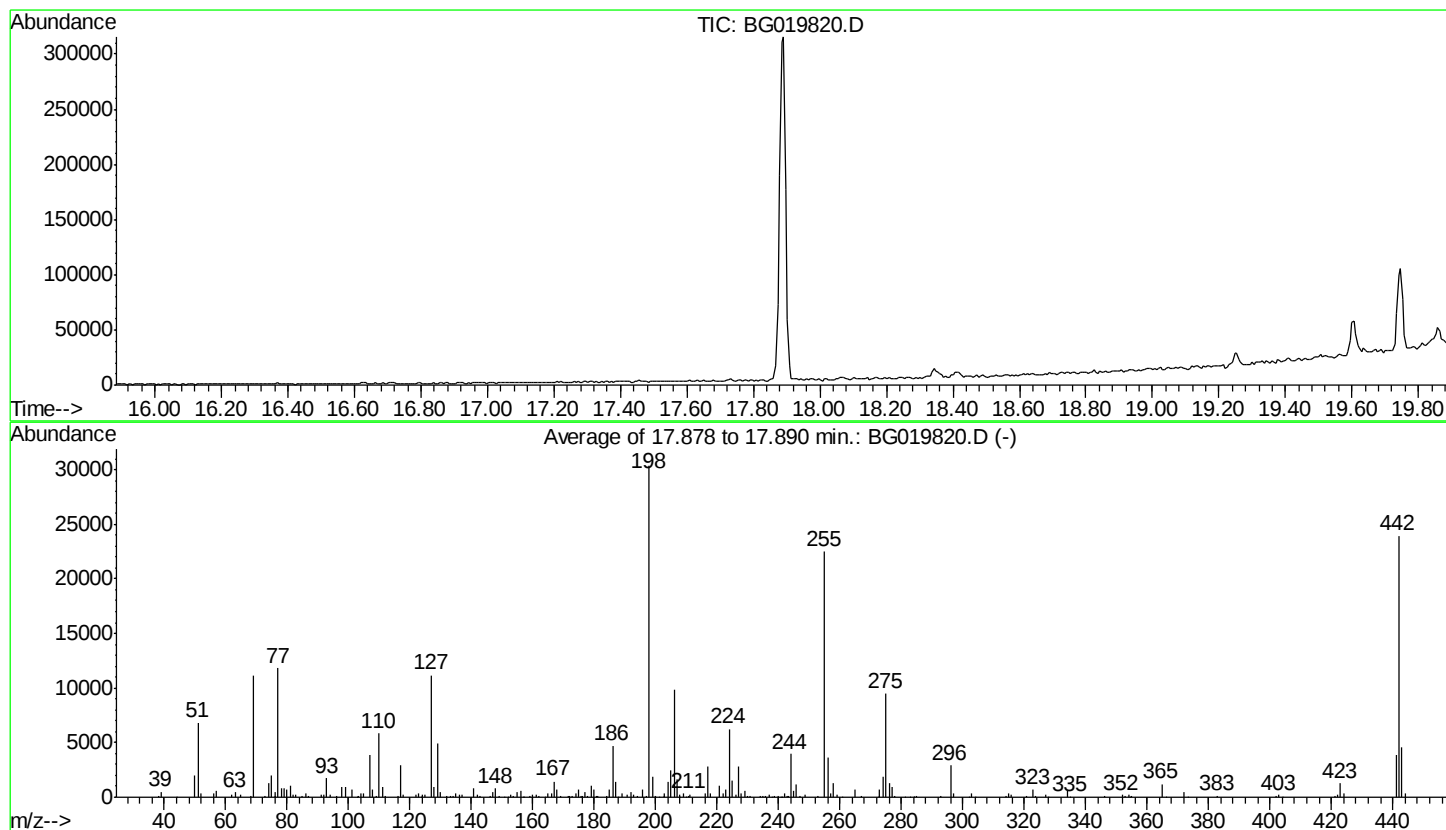

AutoFind: Scans 2560, 2561, 2562; Background Corrected with Scan 2555

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.6	6856	PASS
68	69	0.00	2	0.6	65	PASS
69	198	0.00	100	36.5	11089	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	36.7	11141	PASS
197	198	0.00	2	0.4	112	PASS
198	198	100	100	100.0	30360	PASS
199	198	5	9	6.4	1936	PASS
275	198	10	60	31.1	9453	PASS
365	198	1	100	3.9	1184	PASS
441	442	0.01	24	16.0	3821	PASS
442	198	50	100	78.8	23924	PASS
443	442	15	24	19.2	4596	PASS

m/z	Abundance
39.00	422.0
50.00	1436.0
51.00	6037.0
52.00	167.0
55.90	330.0
57.00	624.0
62.00	334.0
63.00	372.0
65.00	234.0
69.00	8673.0
73.00	573.0
74.00	1164.0
75.00	1641.0
76.00	901.0
77.00	10110.0
78.00	606.0
78.90	608.0
79.90	792.0
80.90	818.0
81.80	231.0
83.00	261.0
85.00	215.0
85.90	162.0
86.80	236.0
91.90	233.0
93.00	1256.0
94.00	212.0
96.00	196.0
98.00	696.0
98.90	1046.0
100.90	399.0
103.90	420.0
105.00	222.0
107.00	3193.0
107.90	504.0
108.90	154.0
110.00	4506.0
111.00	831.0
116.90	2356.0
121.90	262.0
123.00	288.0
123.80	175.0
124.80	250.0
127.00	8293.0
128.00	655.0
128.90	4365.0
130.00	387.0
131.90	202.0
133.00	185.0
133.90	193.0
134.90	399.0
136.00	284.0
137.00	205.0
140.90	691.0
142.00	156.0
147.00	544.0
147.90	478.0
150.80	167.0
152.00	163.0
152.90	265.0
155.00	397.0
156.00	458.0
156.90	162.0
160.90	263.0
164.00	158.0
165.00	344.0
165.90	396.0
167.00	1200.0
168.00	621.0
169.00	184.0
171.70	212.0
174.00	257.0
175.00	604.0
177.00	247.0
178.90	817.0
179.90	645.0
185.10	434.0
186.00	3508.0
187.00	1157.0
188.90	254.0
190.90	390.0
191.90	342.0
192.90	539.0
195.90	462.0
197.90	20392.0
198.90	1481.0
202.80	233.0
203.90	958.0
205.00	1736.0
206.00	6148.0
207.00	2542.0

Instrument :
BNA_G
ClientSampleId :
DFTPP03

207.80	630.0
208.90	193.0
209.70	179.0
210.80	270.0
216.00	408.0
216.90	1755.0
218.00	262.0
220.90	757.0
221.90	203.0
223.00	440.0
224.00	4779.0
225.00	921.0
226.90	1837.0
227.80	188.0
229.00	531.0
230.80	198.0
241.90	315.0
243.10	260.0
244.00	2924.0
245.00	387.0
245.80	1037.0
254.90	14772.0
256.00	2631.0
256.90	176.0
258.00	878.0
264.90	737.0
272.80	491.0
274.00	1036.0
275.00	6536.0
275.90	837.0
276.90	549.0
281.00	473.0
283.00	181.0
284.00	175.0
296.00	1822.0
296.90	180.0
302.90	399.0
314.90	204.0
322.90	387.0
326.90	295.0
333.80	354.0
354.70	156.0
355.20	155.0
364.90	798.0
371.90	437.0
422.10	169.0
423.00	705.0
423.90	199.0
441.00	2082.0
442.00	11604.0
443.00	2634.0
443.90	201.0

Instrument :
BNA_G
ClientSampleId :
DFTPP03

m/z	Abundance
38.90	567.0
50.00	2705.0
51.00	7480.0
52.00	549.0
56.00	367.0
56.90	685.0
63.10	450.0
65.00	275.0
68.00	197.0
69.00	12552.0
73.00	690.0
73.90	1544.0
75.00	2234.0
76.00	586.0
77.00	13632.0
78.00	980.0
79.00	745.0
80.00	589.0
80.90	1186.0
81.90	412.0
82.90	227.0
84.90	268.0
86.00	428.0
86.80	261.0
91.00	378.0
91.90	228.0
92.90	2076.0
94.00	220.0
95.90	287.0
97.90	960.0
98.90	841.0
101.00	775.0
102.80	157.0
103.90	392.0
104.90	392.0
107.00	4340.0
108.00	924.0
109.00	214.0
110.00	6911.0
110.90	1106.0
112.00	220.0
117.00	3380.0
117.90	334.0
121.90	233.0
123.00	579.0
124.00	224.0
124.90	266.0
127.00	13269.0
127.90	1128.0
128.90	5609.0
129.90	511.0
134.00	280.0
135.00	536.0
135.90	313.0
137.00	259.0
140.90	846.0
141.90	337.0
143.00	240.0
146.00	213.0
147.00	638.0
147.90	982.0
149.00	216.0
152.90	273.0
155.00	424.0
156.00	623.0
160.00	402.0
161.00	395.0
162.00	213.0
164.90	275.0
166.00	266.0
167.00	2158.0
167.90	816.0
168.90	224.0
171.90	202.0
173.00	159.0
174.10	413.0
175.00	780.0
175.90	343.0
176.90	566.0
178.00	152.0
179.00	1537.0
180.00	654.0
180.80	429.0
183.90	163.0
184.90	747.0
186.00	5577.0
187.00	1303.0
187.90	166.0
188.90	374.0
190.80	348.0
192.00	474.0

Instrument :
BNA_G
ClientSampleId :
DFTPP03

193.00	484.0
193.90	213.0
195.90	621.0
197.90	35408.0
198.90	2210.0
199.80	155.0
201.00	162.0
203.00	534.0
204.00	1523.0
205.00	2846.0
206.00	11911.0
207.00	3784.0
208.00	882.0
209.00	272.0
211.00	357.0
216.00	280.0
216.90	3180.0
217.90	476.0
221.00	1647.0
222.00	440.0
223.00	800.0
224.00	6246.0
225.00	1896.0
225.90	338.0
226.90	3186.0
227.90	574.0
229.00	446.0
230.00	199.0
234.90	212.0
235.90	228.0
236.90	278.0
237.80	152.0
238.80	261.0
239.90	248.0
240.90	175.0
241.90	464.0
242.80	157.0
244.00	4362.0
245.00	864.0
245.90	1149.0
246.90	269.0
248.80	236.0
252.90	211.0
255.00	26432.0
256.00	4374.0
256.90	505.0
257.90	1260.0
259.00	367.0
260.80	169.0
265.00	787.0
273.00	1108.0
274.00	2160.0
275.00	10317.0
276.00	1505.0
276.90	898.0
277.80	185.0
281.00	543.0
283.00	306.0
284.20	188.0
285.10	211.0
292.90	211.0
295.90	3265.0
297.00	533.0
302.90	282.0
303.90	160.0
313.90	154.0
314.90	415.0
315.90	323.0
321.00	190.0
323.00	903.0
327.90	158.0
333.90	502.0
335.10	164.0
346.00	221.0
352.00	204.0
353.00	323.0
354.00	318.0
364.90	1267.0
372.00	387.0
383.00	209.0
402.10	167.0
403.10	321.0
403.90	152.0
421.10	184.0
421.90	268.0
423.00	1273.0
424.00	356.0
441.00	4198.0
442.00	25984.0
443.00	4774.0
443.90	397.0

Instrument :
BNA_G
ClientSampleId :
DFTPP03

m/z	Abundance
38.00	192.0
39.00	603.0
43.90	154.0
50.00	1884.0
51.00	7053.0
52.00	205.0
55.90	241.0
56.90	594.0
62.00	323.0
63.00	517.0
65.00	232.0
68.90	12044.0
73.00	688.0
74.00	1527.0
75.00	2064.0
76.20	431.0
77.00	11635.0
78.00	828.0
79.00	981.0
80.00	840.0
81.00	1067.0
83.00	266.0
85.90	322.0
90.90	209.0
91.90	374.0
93.00	1795.0
93.90	158.0
98.00	1296.0
98.90	1008.0
101.00	790.0
103.00	332.0
103.90	252.0
104.90	399.0
107.00	3911.0
108.00	704.0
109.90	6062.0
111.00	874.0
116.10	194.0
117.00	2913.0
117.90	272.0
121.90	395.0
122.90	345.0
124.00	319.0
125.00	181.0
127.00	11863.0
128.00	1203.0
129.00	4691.0
129.90	570.0
133.00	187.0
134.90	211.0
136.10	223.0
137.00	308.0
140.90	779.0
142.00	281.0
143.00	248.0
145.90	210.0
147.00	735.0
148.00	933.0
149.00	248.0
152.80	260.0
153.80	229.0
154.90	442.0
155.90	664.0
157.10	166.0
158.90	224.0
159.90	364.0
160.90	196.0
161.90	174.0
164.90	290.0
166.10	441.0
166.90	1564.0
167.90	519.0
173.00	327.0
174.00	448.0
174.90	685.0
176.10	213.0
176.90	573.0
177.80	201.0
178.90	915.0
180.00	970.0
181.00	460.0
184.00	250.0
185.00	936.0
186.00	5097.0
186.90	1811.0
188.90	284.0
190.90	521.0
191.90	487.0
193.00	777.0
195.90	1116.0
196.80	337.0

Instrument :
BNA_G
ClientSampleId :
DFTPP03

197.90	35280.0
198.90	2117.0
200.00	211.0
203.00	480.0
203.90	1875.0
205.00	2697.0
206.00	11474.0
207.00	3467.0
207.90	770.0
209.00	429.0
211.00	458.0
216.10	510.0
216.90	3539.0
217.80	441.0
221.00	1619.0
221.90	539.0
222.90	912.0
224.00	7671.0
225.00	1834.0
226.00	204.0
227.00	3383.0
227.90	232.0
228.90	684.0
230.80	223.0
234.00	194.0
235.00	163.0
235.80	186.0
237.00	465.0
238.80	169.0
241.10	157.0
241.90	332.0
242.90	320.0
244.00	4518.0
245.00	679.0
245.90	1312.0
248.90	341.0
253.00	231.0
255.00	26168.0
256.00	3816.0
257.00	259.0
257.90	1749.0
258.90	243.0
264.90	573.0
266.90	254.0
273.00	1186.0
274.00	2537.0
275.00	11506.0
276.00	1409.0
276.90	1251.0
277.80	237.0
280.90	512.0
283.00	259.0
284.90	164.0
293.00	270.0
296.00	3597.0
296.90	361.0
302.00	173.0
303.00	499.0
314.00	259.0
315.00	355.0
315.80	228.0
320.90	276.0
323.00	813.0
323.80	197.0
327.00	277.0
334.00	784.0
346.00	190.0
351.90	350.0
353.00	160.0
353.90	237.0
355.00	166.0
364.90	1489.0
366.00	179.0
371.90	442.0
373.20	175.0
382.80	164.0
401.90	305.0
402.90	355.0
420.90	210.0
422.00	177.0
423.00	1879.0
424.00	368.0
441.00	5184.0
442.00	34184.0
443.00	6381.0
444.00	557.0

Instrument :
BNA_G
ClientSampleId :
DFTPP03

Scan 2555 (17.849 min): BG019820.D
DFTPP03

m/z	Abundance
72.90	549.0
74.10	164.0
146.90	189.0
167.10	184.0
190.90	220.0
192.90	312.0
207.00	1672.0
207.90	493.0
208.70	261.0
220.90	249.0
281.00	455.0
282.00	175.0
283.00	219.0

Instrument :
BNA_G
ClientSampleId :
DFTPP03