
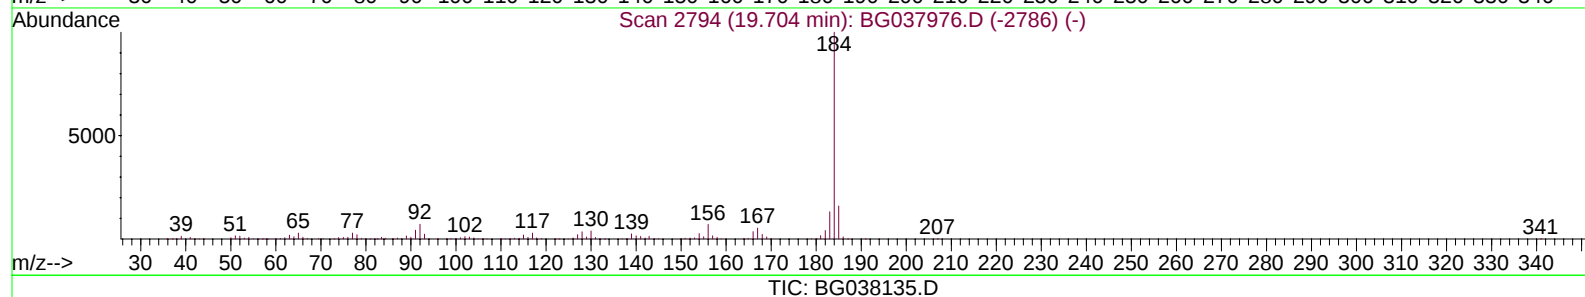
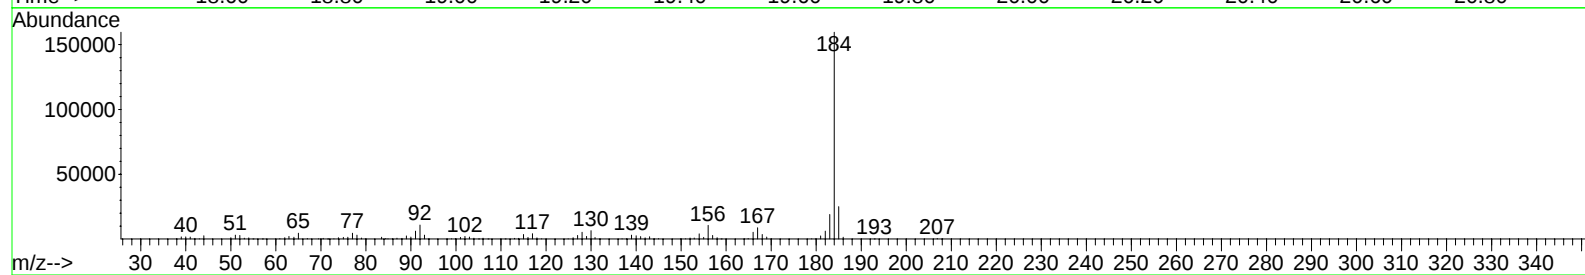


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG112618\
Data File : BG038135.D
Acq On : 26 Nov 2018 14:09
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 26 17:10:15 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG111318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 13 16:39:28 2018
Response via : Initial Calibration

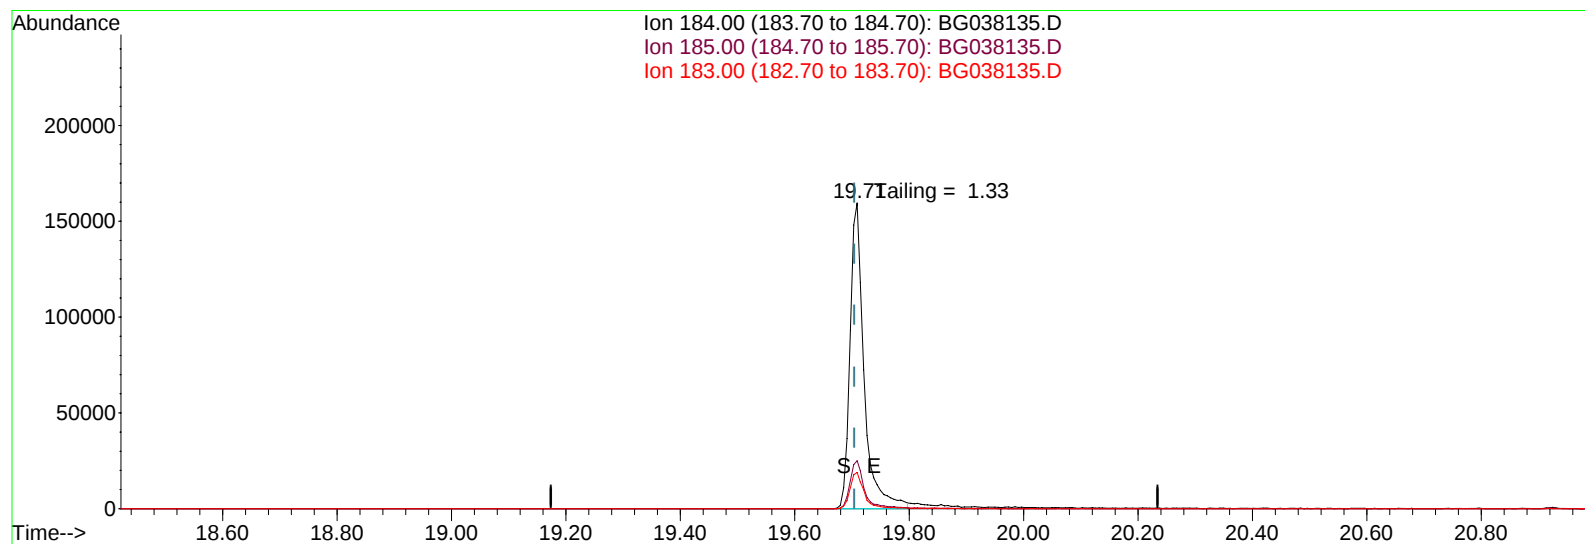

(77) Benzidine




19.709min (+0.005) 136330.48ng

response 282240

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.68
183.00	12.70	11.90
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG112618\
Data File : BG038135.D
Acq On : 26 Nov 2018 14:09
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 26 17:10:15 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG111318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 13 16:39:28 2018
Response via : Initial Calibration

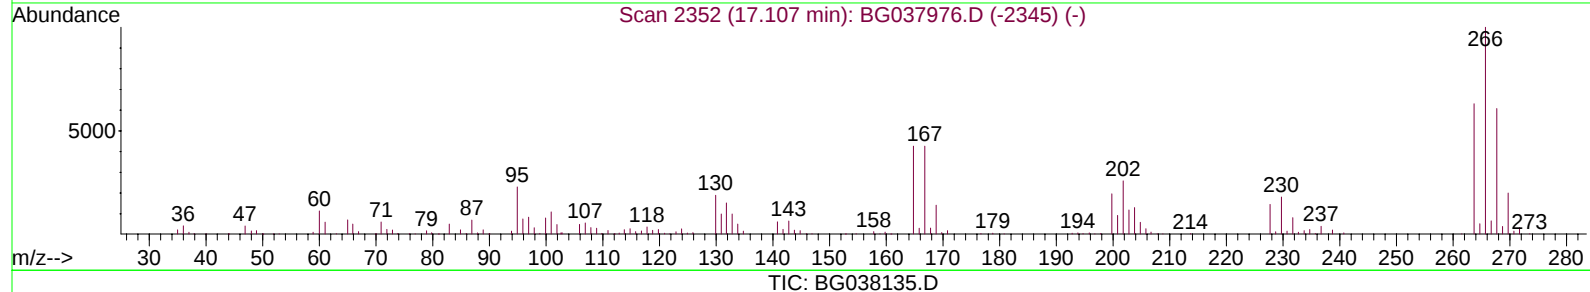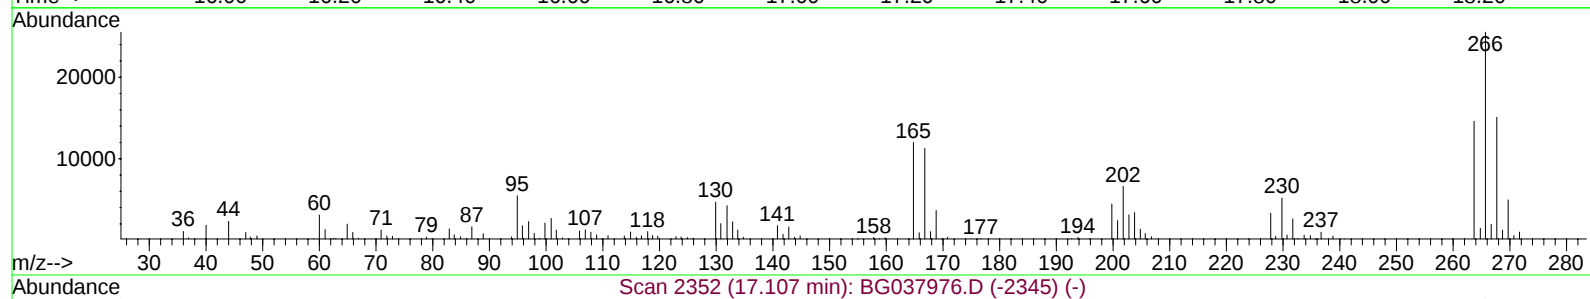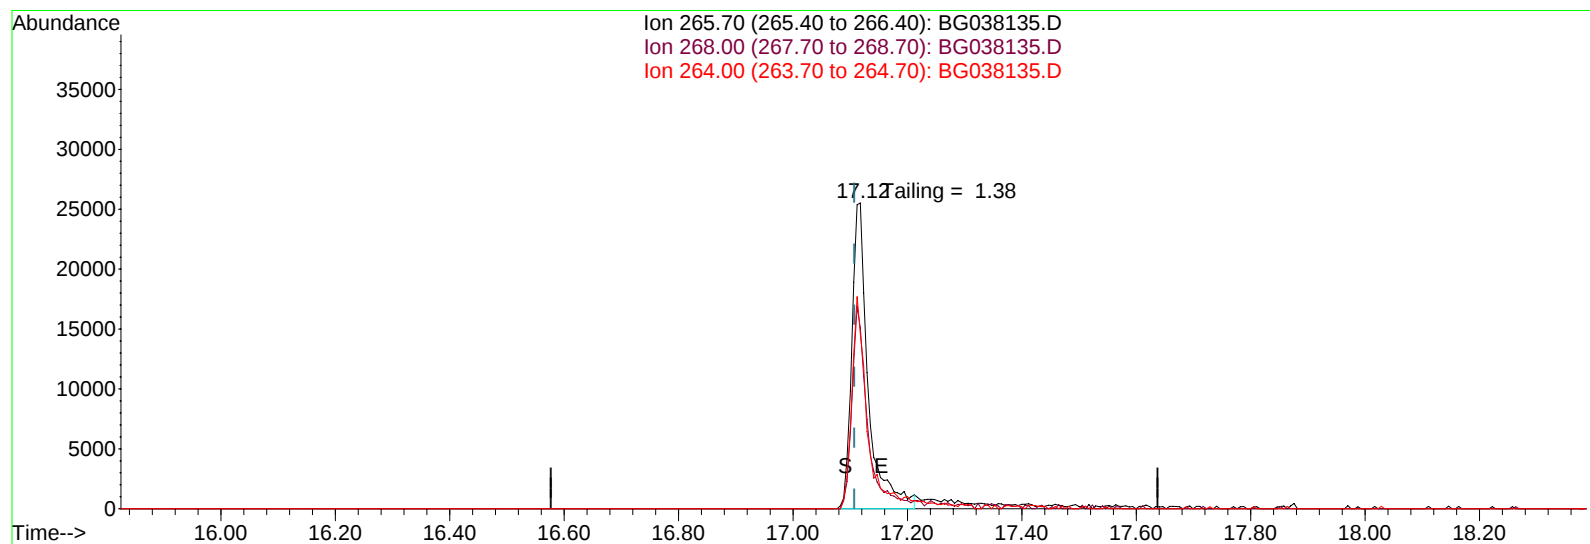

(70) Pentachlorophenol (C)

17.118min (+0.011) 121419.31ng

response 51384

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	64.00
264.00	73.60	57.24#
0.00	0.00	0.00