

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG112618\
 Data File : BG038157.D
 Acq On : 27 Nov 2018 6:17
 Operator : JU/SJ
 Sample : J6061-04
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 112018-JETT-E-U-B

Quant Time: Nov 27 07:30:39 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG111318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 13 16:39:28 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.09	152	37882	20.00	ng	0.00
21) Naphthalene-d8	10.91	136	169752	20.00	ng	0.00
39) Acenaphthene-d10	14.72	164	107483	20.00	ng	0.00
64) Phenanthrene-d10	17.47	188	244058	20.00	ng	0.00
76) Chrysene-d12	21.76	240	223019	20.00	ng	0.00
87) Perylene-d12	25.08	264	219368	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.63	112	116019	52.88	ng	0.00
7) Phenol-d6	7.23	99	109046	34.82	ng	0.00
23) Nitrobenzene-d5	9.27	82	335213	105.71	ng	0.00
42) 2,4,6-Tribromophenol	16.21	330	120073	97.95	ng	0.00
45) 2-Fluorobiphenyl	13.34	172	754045	102.21	ng	0.00
79) Terphenyl-d14	20.07	244	959180	101.20	ng	0.00
Target Compounds						
10) Phenol	7.26	94	9789	2.951	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG112618\
Data File : BG038157.D
Acq On : 27 Nov 2018 6:17
Operator : JU/SJ
Sample : J6061-04
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
112018-JETT-E-U-B

Quant Time: Nov 27 07:30:39 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG111318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 13 16:39:28 2018
Response via : Initial Calibration

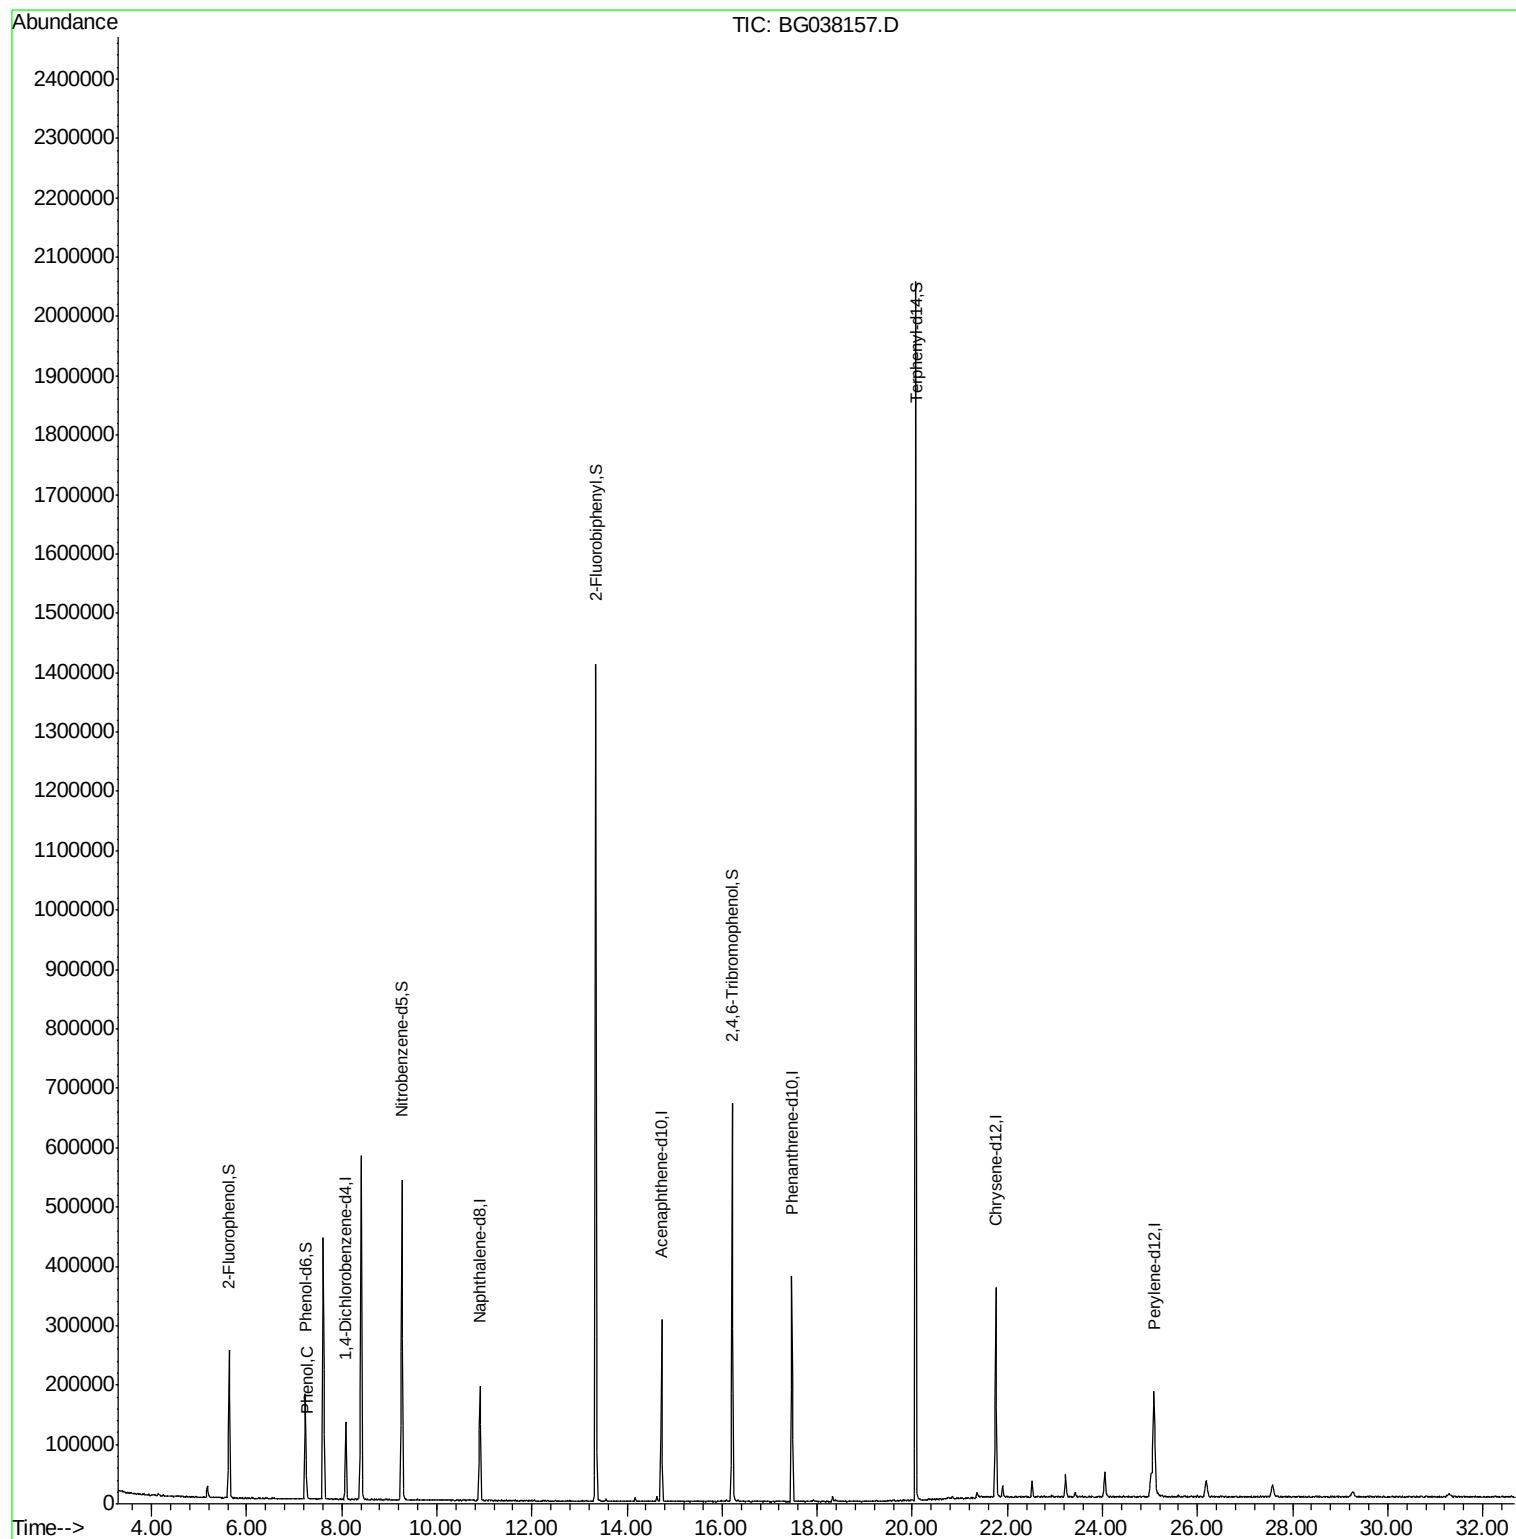

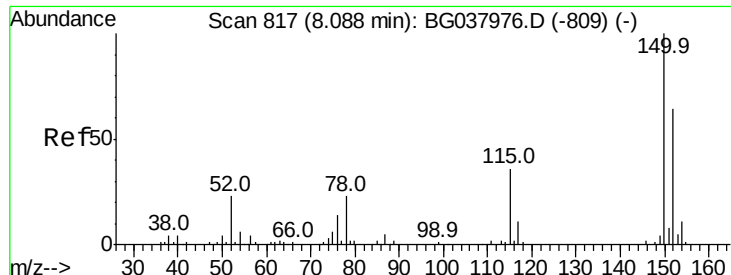


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.09 min Scan# 816
Delta R.T. -0.00 min
Lab File: BG038157.D
Acq: 27 Nov 2018 6:17

Instrument :
BNA_G
ClientSampleId :
112018-JETT-E-U-B

Tot Ion:152 Resp: 37882
Ion Ratio Lower Upper
152 100
150 158.2 126.0 189.0
115 60.6 45.5 68.3

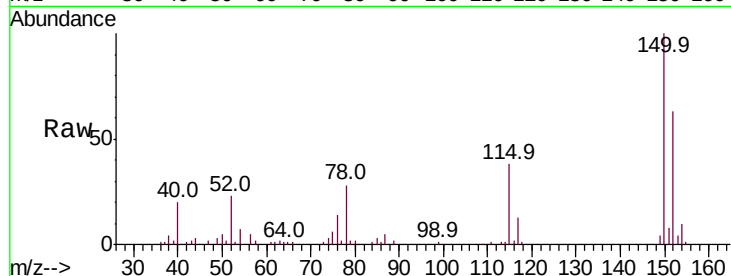


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

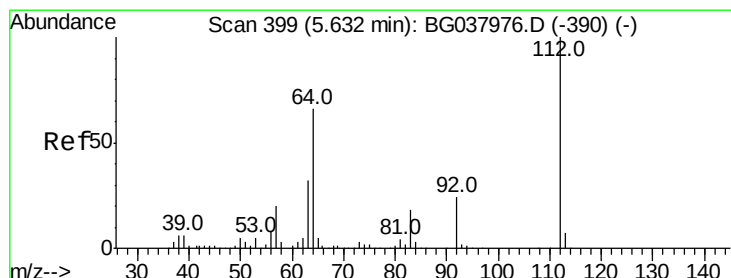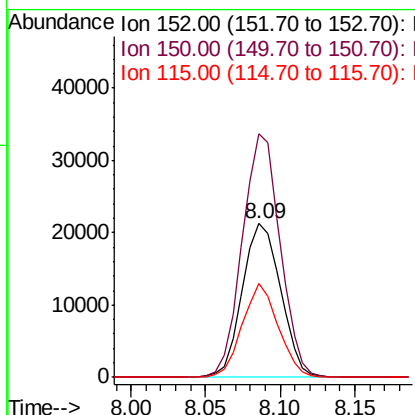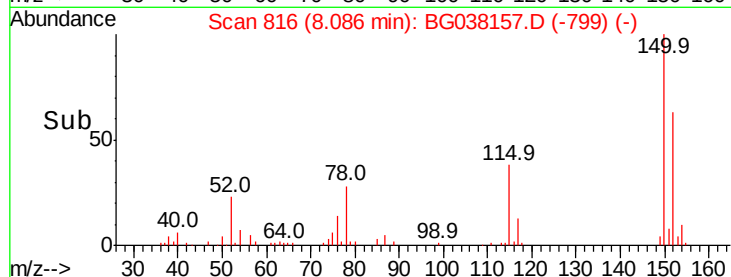



#5


2-Fluorophenol
Concen: 52.879 ng
RT: 5.63 min Scan# 398
Delta R.T. -0.00 min
Lab File: BG038157.D
Acq: 27 Nov 2018 6:17

Tgt Ion:112 Resp: 116019
Ion Ratio Lower Upper
112 100
64 68.2 53.1 79.7
63 33.4 27.3 40.9

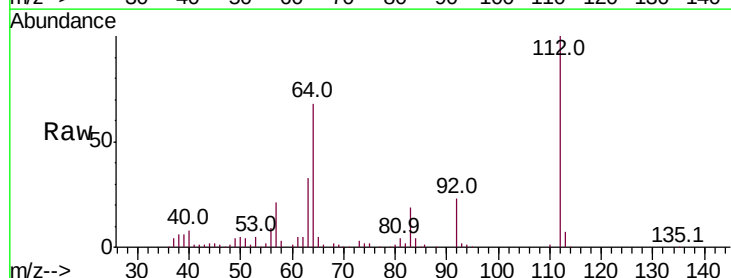

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

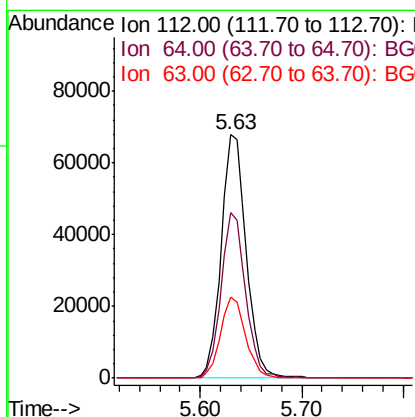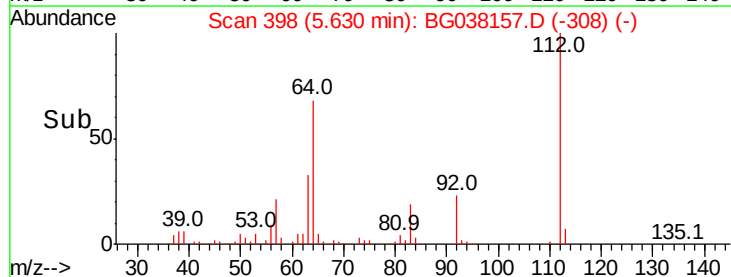

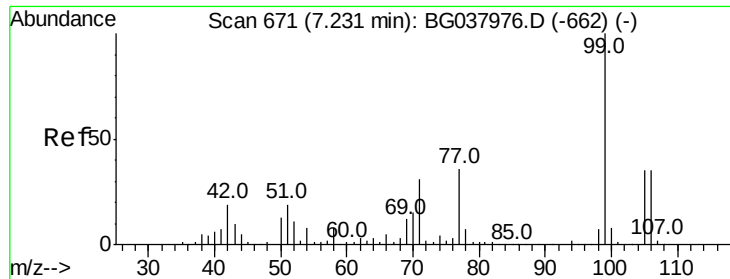

#7

Phenol-d6

Concen: 34.818 ng

RT: 7.23 min Scan# 671

Delta R.T. 0.00 min

Lab File: BG038157.D

Acq: 27 Nov 2018 6:17

Instrument :

BNA_G

ClientSampleId :

112018-JETT-E-U-B


Tot Ion: 99 Resp: 109046

Ion Ratio Lower Upper




99 100

42 21.0 15.0 22.4

71 31.5 25.5 38.3

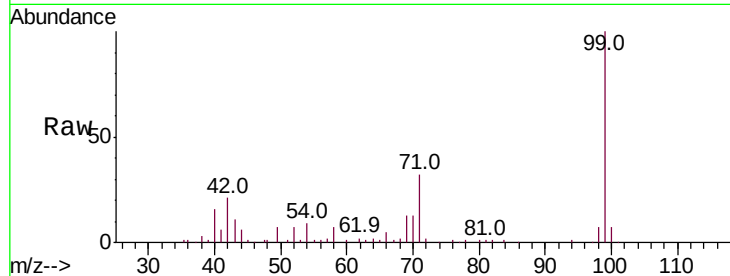

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

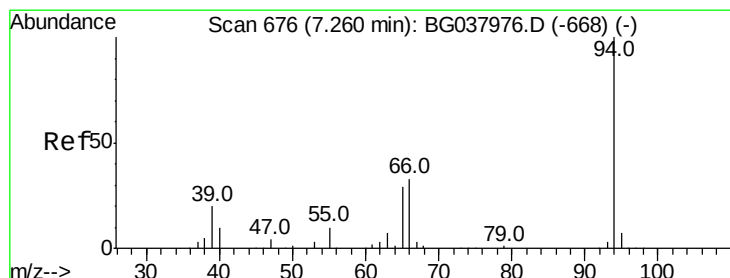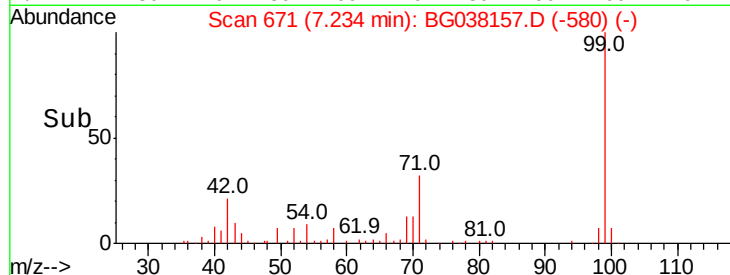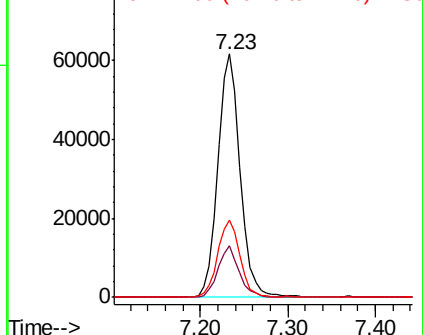

#10

Phenol

Concen: 2.951 ng

RT: 7.26 min Scan# 676

Delta R.T. 0.00 min

Lab File: BG038157.D

Acq: 27 Nov 2018 6:17


Tgt Ion: 94 Resp: 9789

Ion Ratio Lower Upper



94 100


65 29.5 9.7 49.7

66 37.1 15.9 55.9

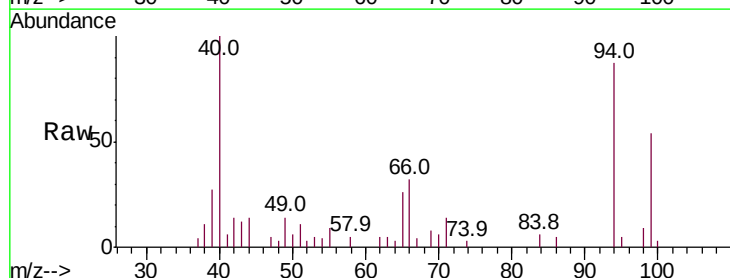

Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC

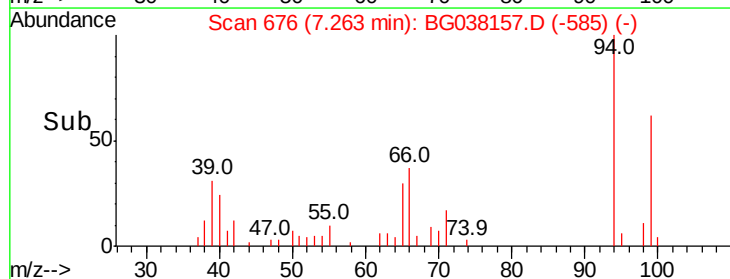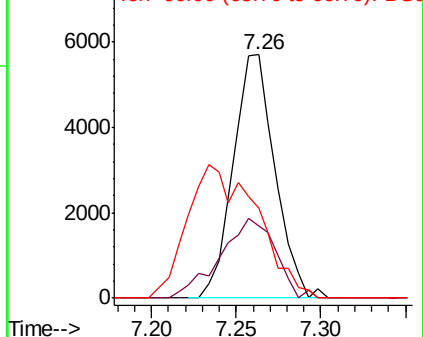


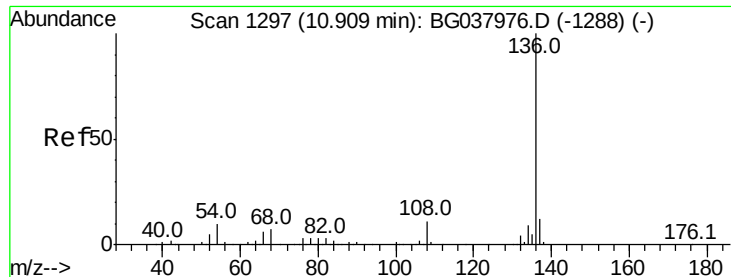




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.91 min Scan# 1296
Delta R.T. -0.00 min
Lab File: BG038157.D
Acq: 27 Nov 2018 6:17

Instrument :
BNA_G
ClientSampleId :
112018-JETT-E-U-B

Tot Ion:136	Resp: 169752
Ion Ratio	Lower Upper
136 100	
137 11.8	9.6 14.4
54 11.1	7.9 11.9
68 6.5	4.8 7.2

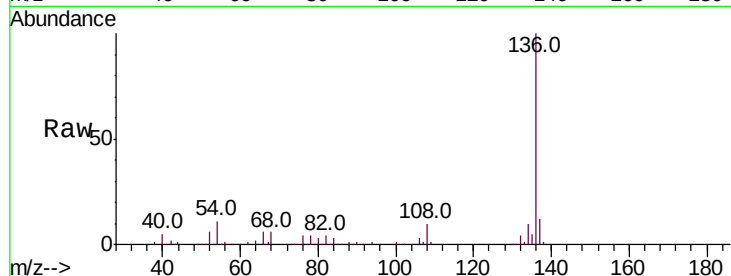


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

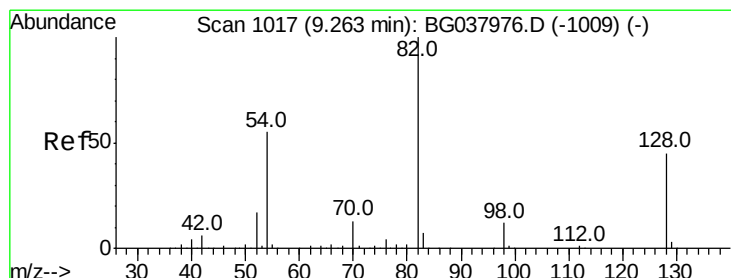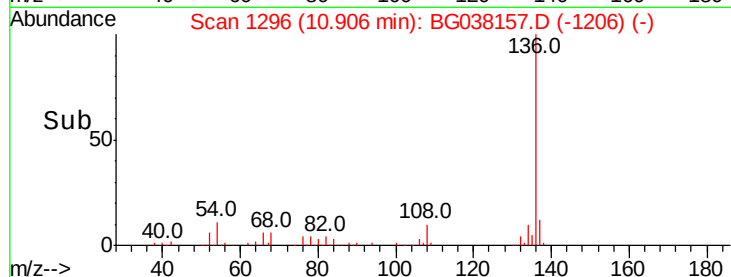
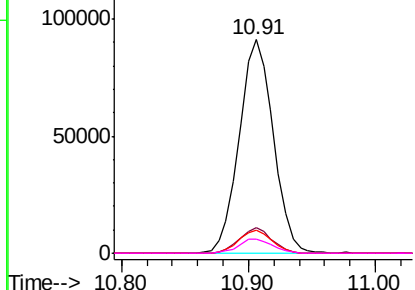



#23
Nitrobenzene-d5
Concen: 105.708 ng
RT: 9.27 min Scan# 1017
Delta R.T. 0.00 min
Lab File: BG038157.D
Acq: 27 Nov 2018 6:17

Tgt Ion: 82	Resp: 335213
Ion Ratio	Lower Upper
82 100	
128 42.7	34.6 51.8
54 58.4	45.3 67.9

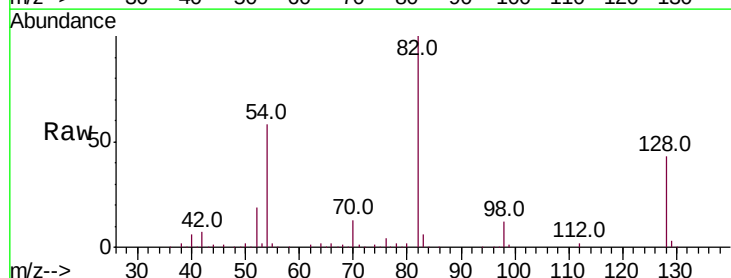

Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BGC

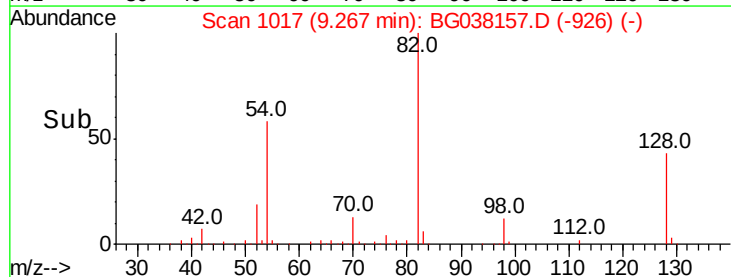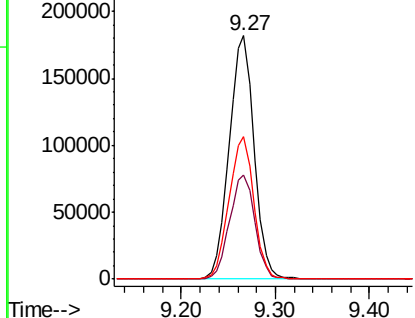

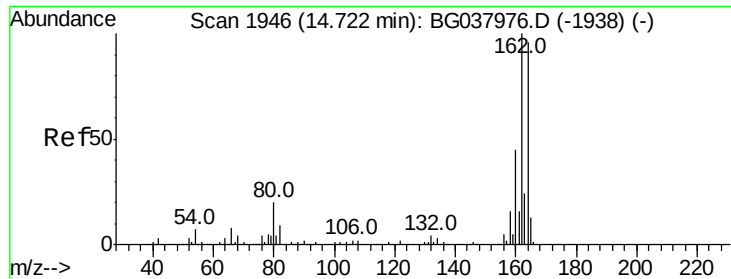

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.72 min Scan# 1946

Delta R.T. 0.00 min

Lab File: BG038157.D

Acq: 27 Nov 2018 6:17

Instrument :

BNA_G

ClientSampleId :

112018-JETT-E-U-B


Tot Ion:164 Resp: 107483

Ion Ratio Lower Upper

164 100

162 105.0 81.3 121.9




160 44.7 36.3 54.5

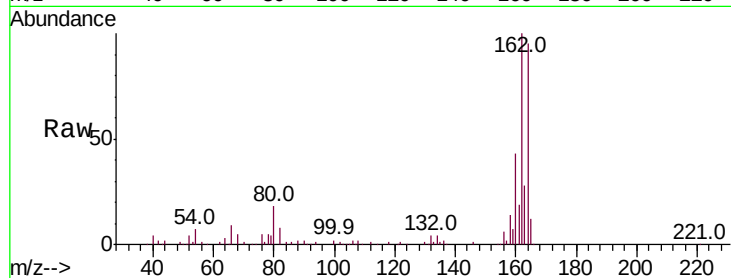

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

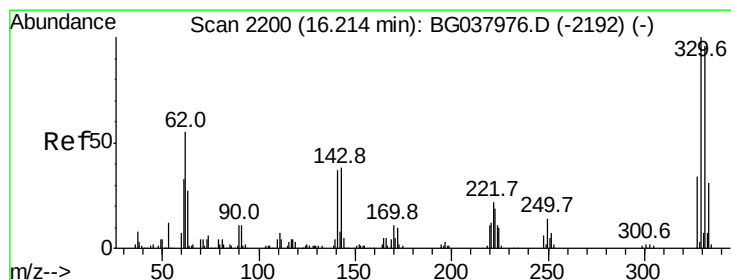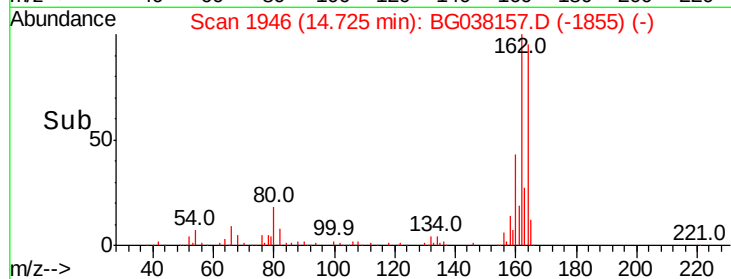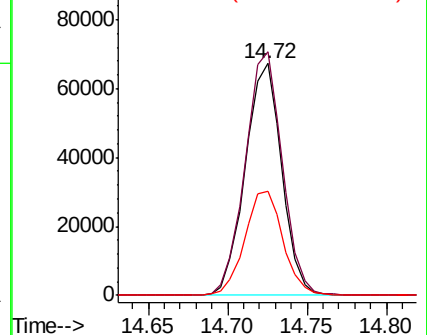

#42

2,4,6-Tribromophenol

Concen: 97.953 ng

RT: 16.21 min Scan# 2199

Delta R.T. -0.00 min

Lab File: BG038157.D

Acq: 27 Nov 2018 6:17


Tgt Ion:330 Resp: 120073

Ion Ratio Lower Upper

330 100

332 96.8 78.4 117.6



141 41.0 32.2 48.2

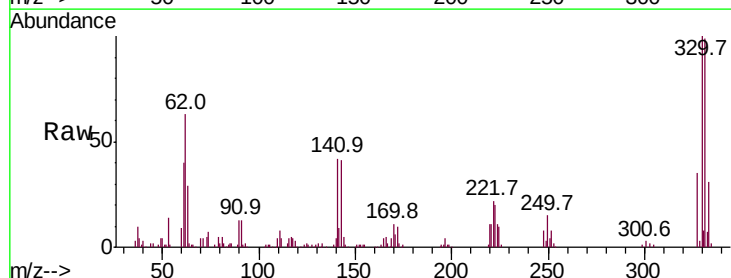


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



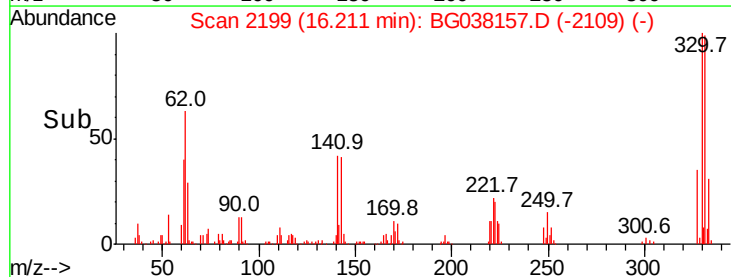
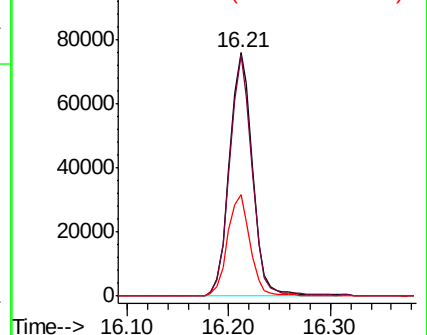


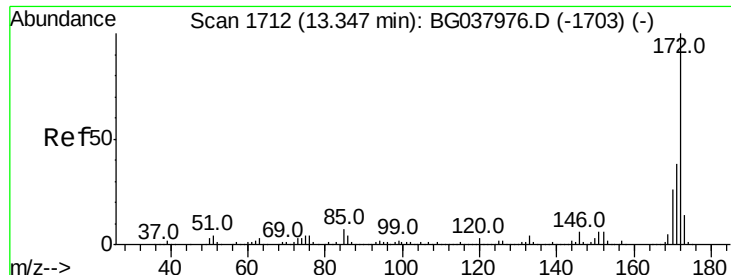

#45
 2-Fluorobiphenyl
 Concen: 102.205 ng
 RT: 13.34 min Scan# 1711
 Delta R.T. -0.00 min
 Lab File: BG038157.D
 Acq: 27 Nov 2018 6:17




Instrument :
 BNA_G
 ClientSampleId :
 112018-JETT-E-U-B


Tot Ion	Ratio	Lower	Upper
172	100		
171	38.1	31.0	46.4
170	25.0	20.2	30.2

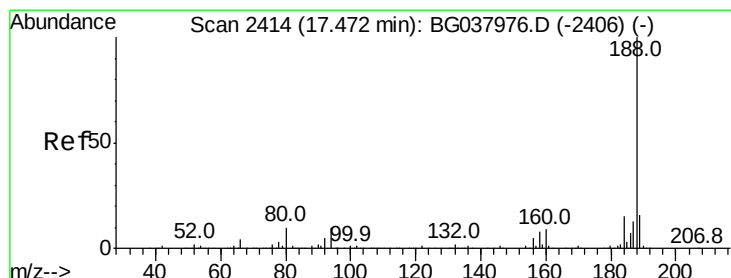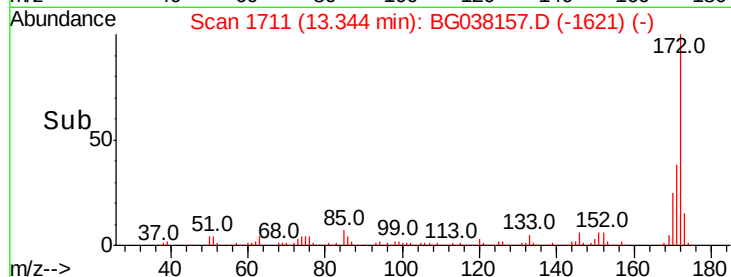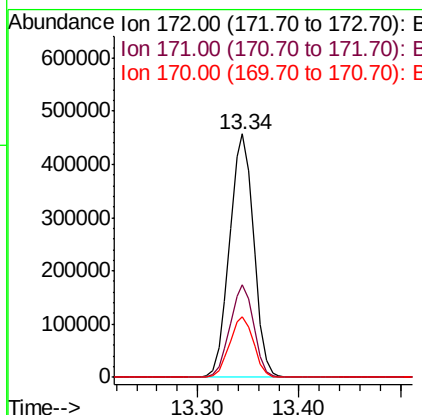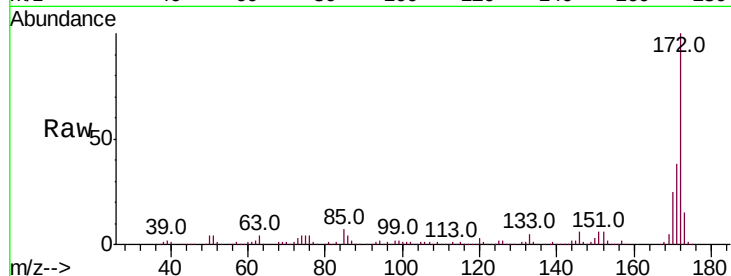

#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.47 min Scan# 2413
 Delta R.T. -0.00 min
 Lab File: BG038157.D
 Acq: 27 Nov 2018 6:17

Tgt Ion	Ratio	Lower	Upper
188	100		
94	8.3	7.2	10.8
80	9.9	7.7	11.5

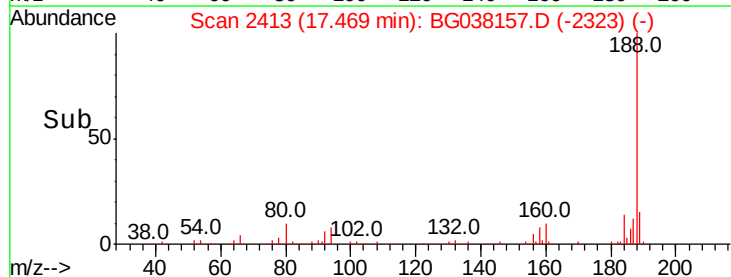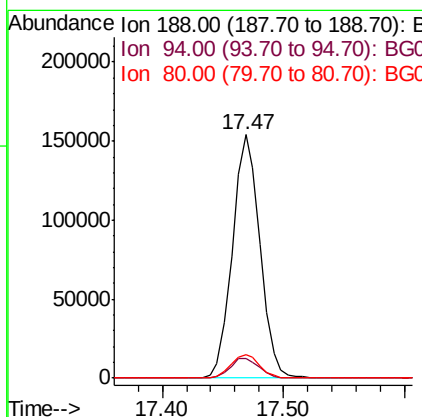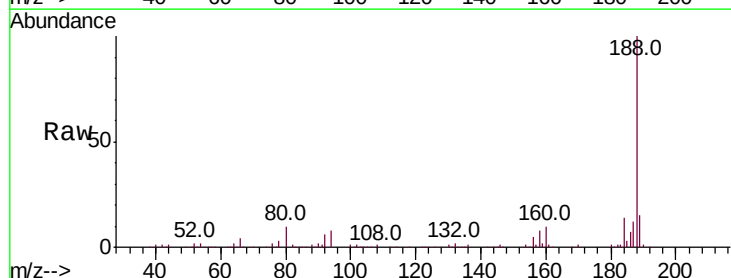

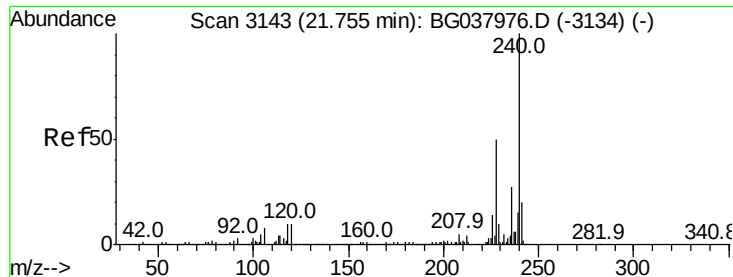

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.76 min Scan# 3143

Delta R.T. 0.00 min

Lab File: BG038157.D

Acq: 27 Nov 2018 6:17

Instrument :

BNA_G

ClientSampleId :

112018-JETT-E-U-B


Tot Ion:240 Resp: 223019

Ion Ratio Lower Upper

240 100

120 10.4 8.1 12.1




236 28.1 21.4 32.0

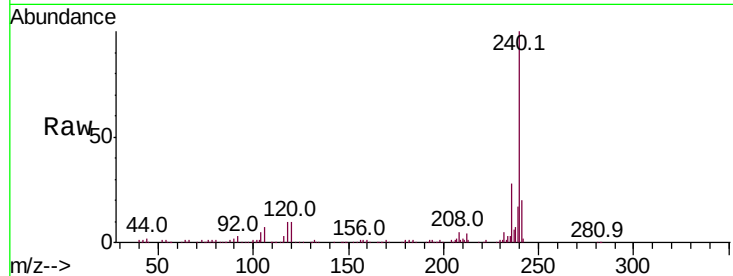

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

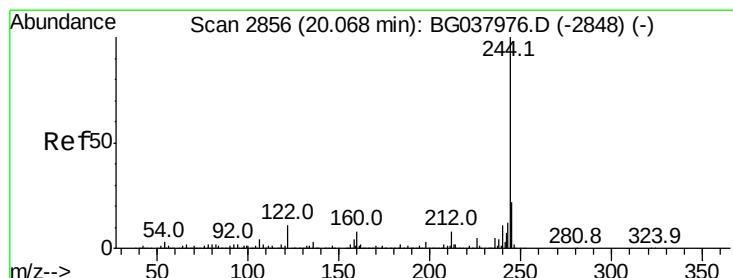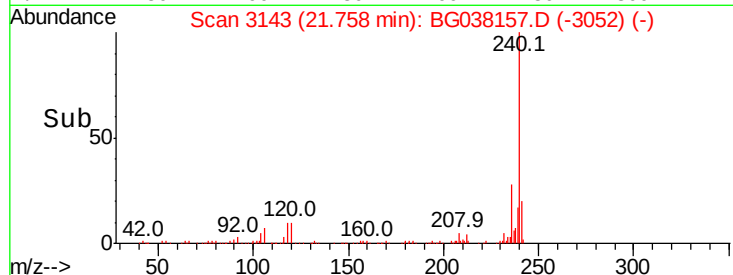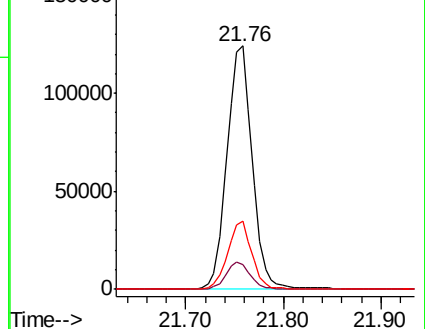

#79

Terphenyl-d14

Concen: 101.200 ng

RT: 20.07 min Scan# 2856

Delta R.T. 0.00 min

Lab File: BG038157.D

Acq: 27 Nov 2018 6:17


Tgt Ion:244 Resp: 959180

Ion Ratio Lower Upper

244 100

212 8.0 6.5 9.7



122 10.3 9.0 13.4

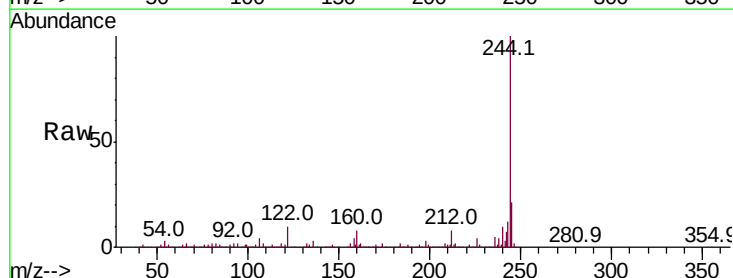


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

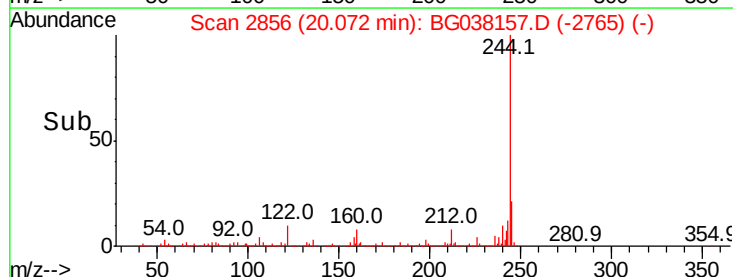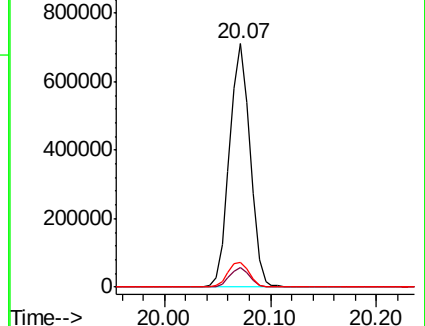

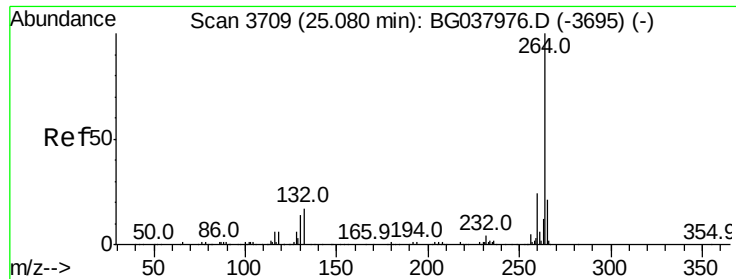

#87
 Pervlene-d12
 Concen: 20.000 ng
 RT: 25.08 min Scan# 3709
 Delta R.T. 0.00 min
 Lab File: BG038157.D
 Acq: 27 Nov 2018 6:17

Instrument :
 BNA_G
 ClientSampleId :
 112018-JETT-E-U-B

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.5	18.2	27.4
265	22.3	17.9	26.9

