

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG112618\
 Data File : BG038145.D
 Acq On : 26 Nov 2018 21:23
 Operator : JU/SJ
 Sample : J6032-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MMTW-02

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG111318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.633	392	399	410	rBV	332070	550302	21.22%	4.192%
2	7.231	665	671	684	rVB	222060	419836	16.19%	3.198%
3	7.613	728	736	744	rBV	576684	1023380	39.46%	7.796%
4	8.089	810	817	829	rBV	146079	255308	9.85%	1.945%
5	8.412	864	872	880	rBV	497024	912662	35.19%	6.952%
6	9.264	1009	1017	1031	rBV	457065	869168	33.52%	6.621%
7	10.909	1290	1297	1307	rVB	209194	394609	15.22%	3.006%
8	13.341	1703	1711	1723	rBV	1187623	1956346	75.44%	14.903%
9	14.722	1936	1946	1956	rBV3	331678	557337	21.49%	4.246%
10	16.209	2190	2199	2211	rBV	840932	1337595	51.58%	10.189%
11	16.414	2229	2234	2243	rVB2	19239	35980	1.39%	0.274%
12	17.472	2408	2414	2420	rBV	405232	636512	24.55%	4.849%
13	18.324	2554	2559	2564	rBV3	20030	29733	1.15%	0.226%
14	19.734	2794	2799	2804	rBV	51347	63968	2.47%	0.487%
15	20.069	2850	2856	2866	rBV	1856994	2593186	100.00%	19.754%
16	21.755	3136	3143	3155	rBV2	398631	688221	26.54%	5.243%
17	23.224	3389	3393	3399	rVB2	20324	35239	1.36%	0.268%
18	24.047	3527	3533	3542	rVB4	20715	47893	1.85%	0.365%
19	25.081	3692	3709	3720	rBV2	198223	675235	26.04%	5.144%
20	26.191	3887	3898	3905	rBV6	14848	44902	1.73%	0.342%


Sum of corrected areas: 13127412

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG112618\
Data File : BG038145.D
Acq On : 26 Nov 2018 21:23
Operator : JU/SJ
Sample : J6032-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MMTW-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG111318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

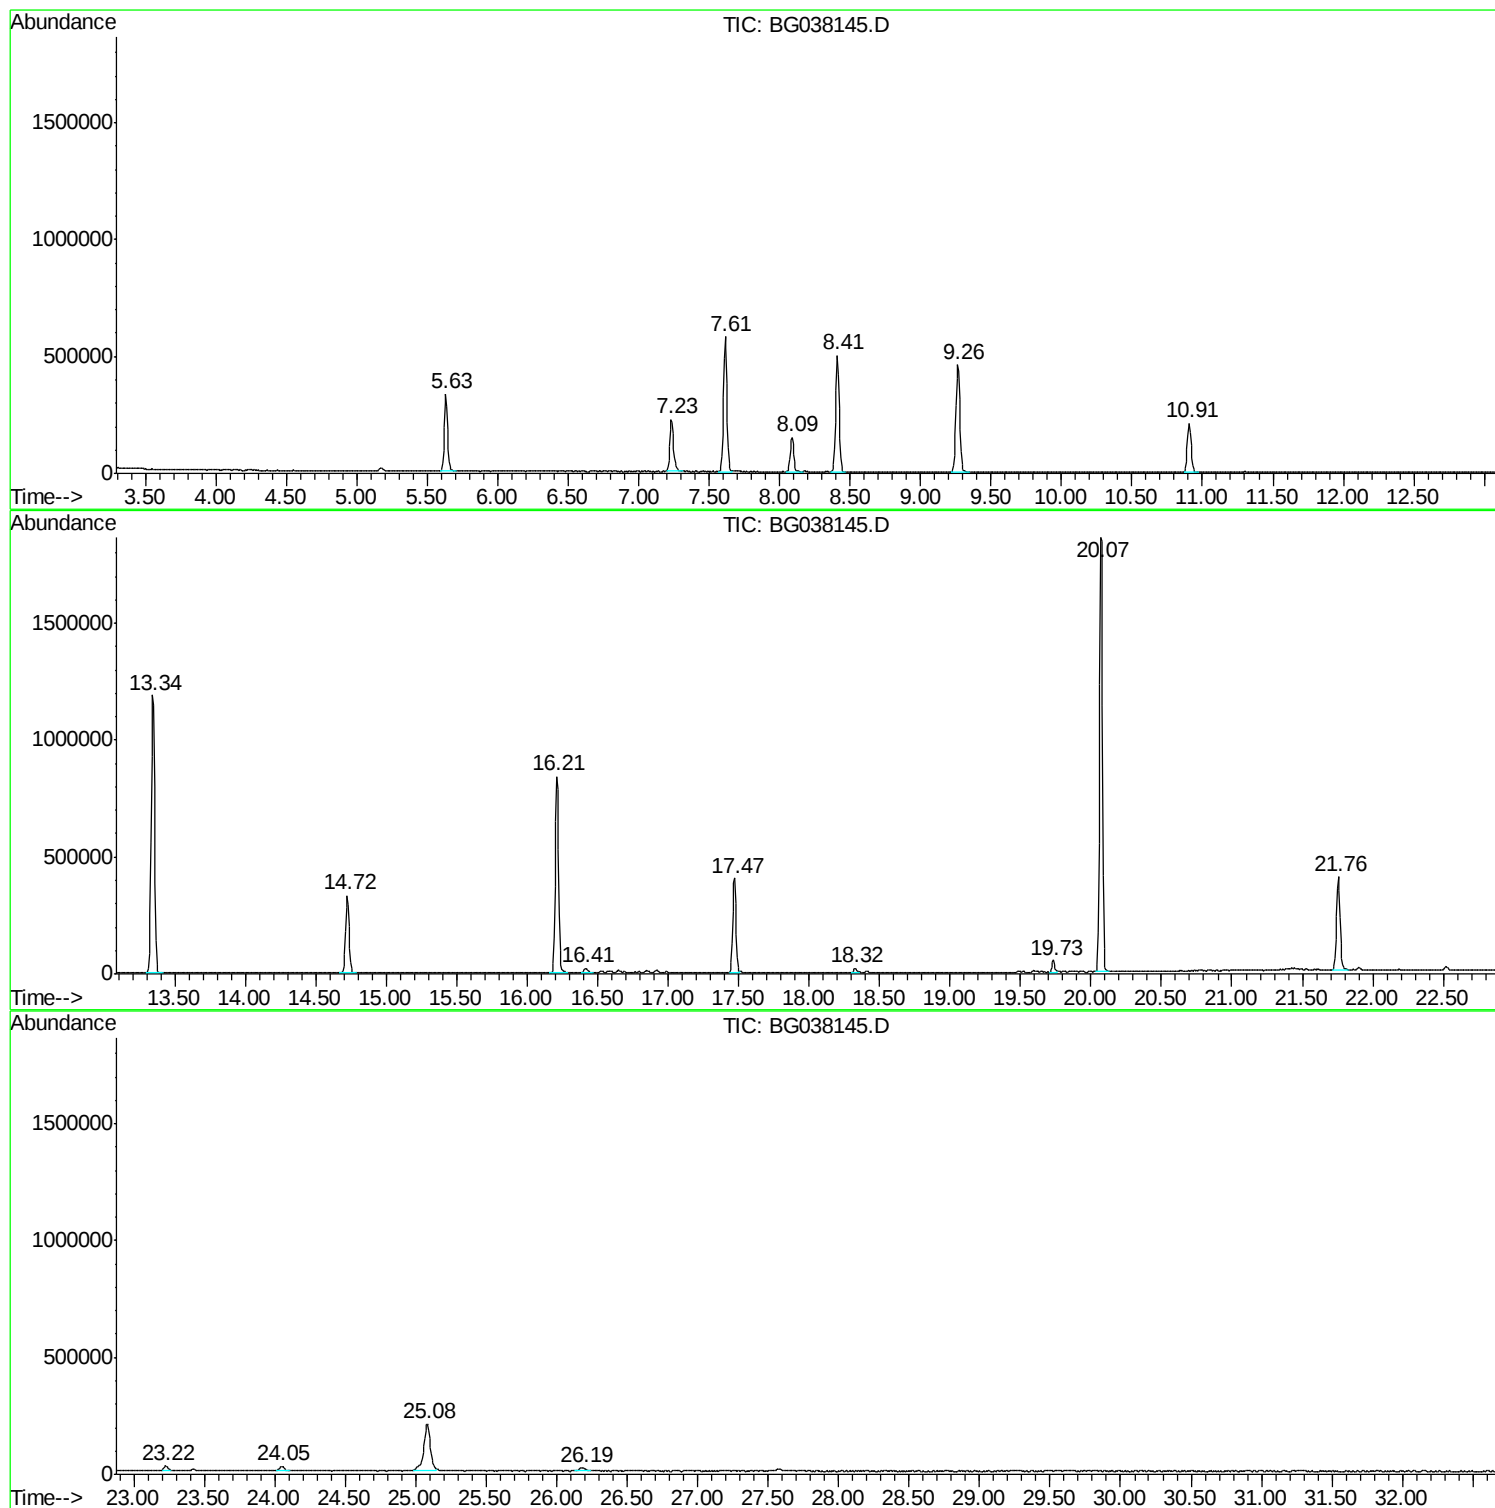

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG112618\
Data File : BG038145.D
Acq On : 26 Nov 2018 21:23
Operator : JU/SJ
Sample : J6032-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MMTW-02










Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG111318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.61 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.61	80.17 ng	1023380	1,4-Dichlorobenzene-d4	8.09

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Tranvlcvpromine-propionyl	189	C12H15NO	1000123-86-3	22
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
3		1,2,4-Trifluorobenzene	132	C6H3F3	000367-23-7	9
4		1,3,5-Trifluorobenzene	132	C6H3F3	000372-38-3	9
5		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	9

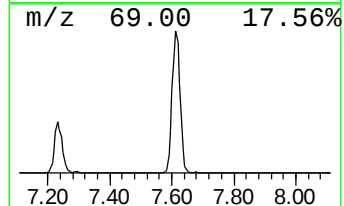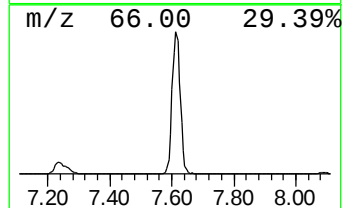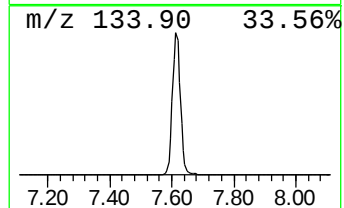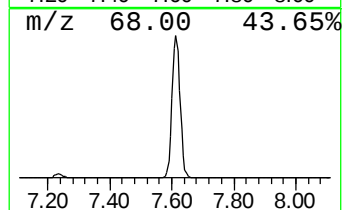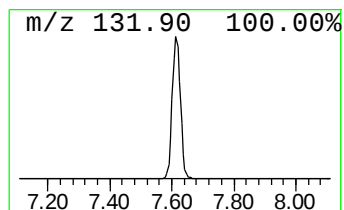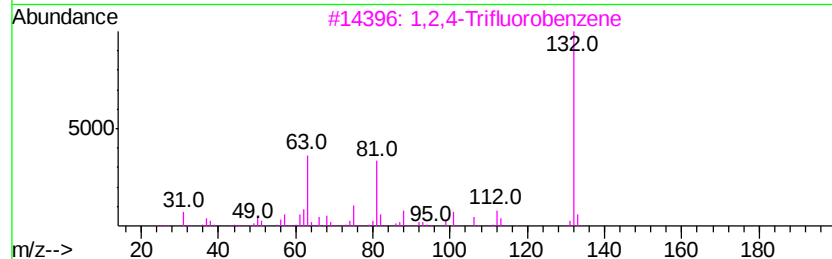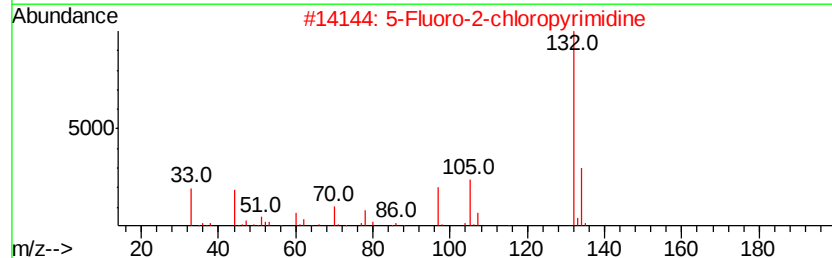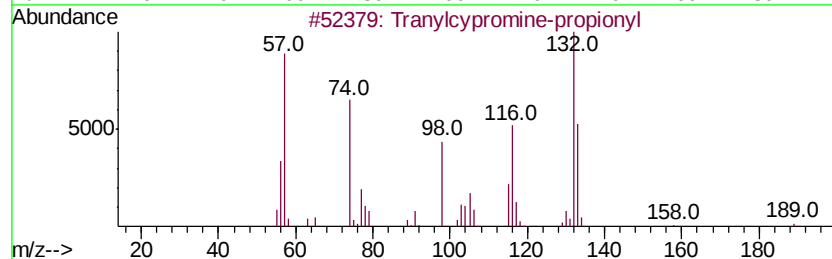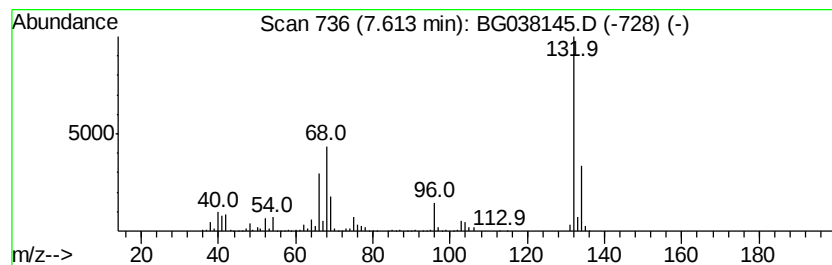

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG112618\
Data File : BG038145.D
Acq On : 26 Nov 2018 21:23
Operator : JU/SJ
Sample : J6032-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MMTW-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG111318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.61	7.61	80.2	ng	1023380	1	8.09	255308	20.0