


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG112618\
 Data File : BG038153.D
 Acq On : 27 Nov 2018 3:18
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG111318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 13 16:39:28 2018

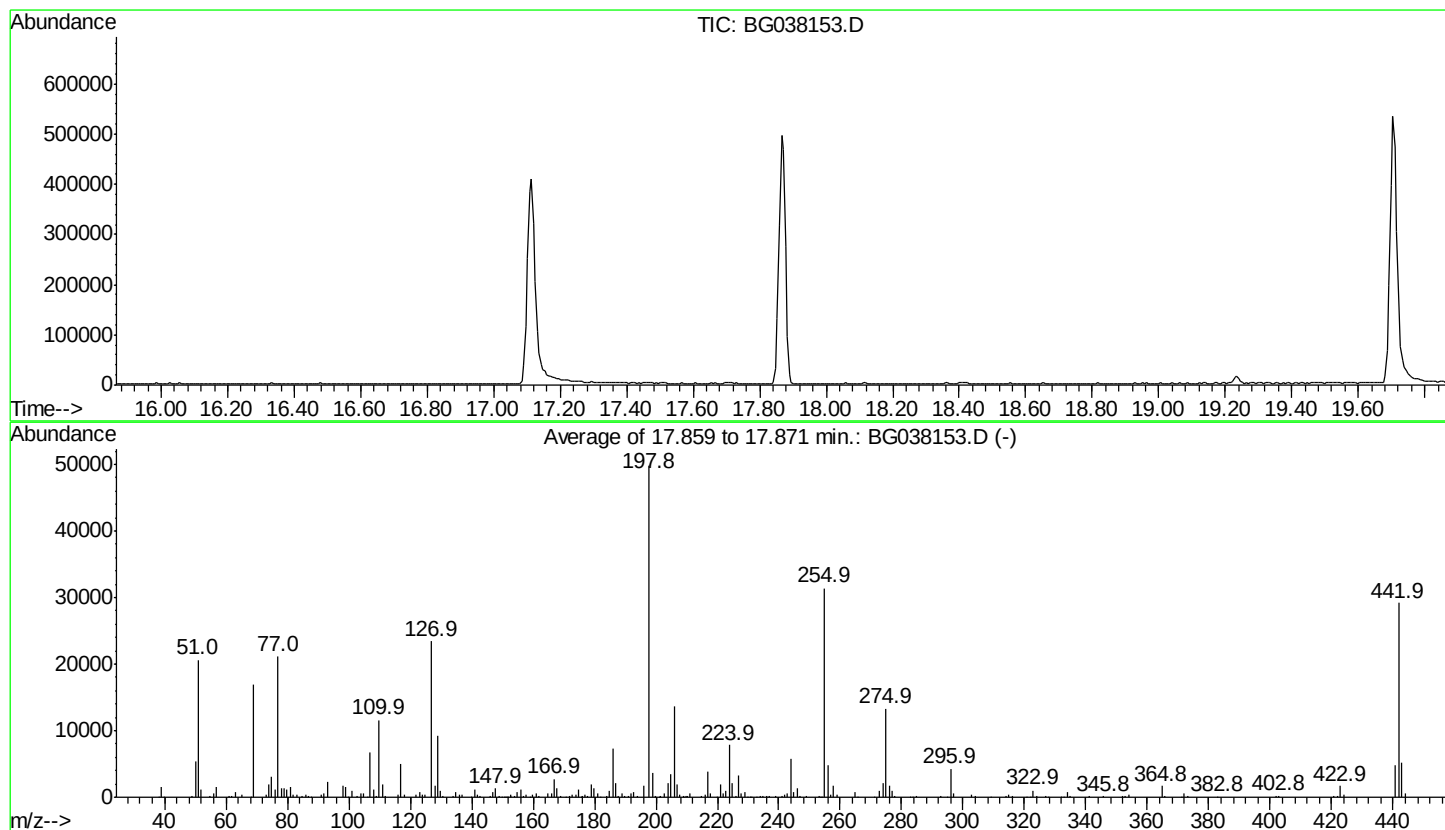

AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.5	20666	PASS
68	69	0.00	2	0.6	103	PASS
69	198	0.00	100	34.0	16944	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.0	23437	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	49829	PASS
199	198	5	9	7.2	3606	PASS
275	198	10	60	26.8	13334	PASS
365	198	1	100	3.4	1670	PASS
441	198	0.01	100	9.6	4779	PASS
442	198	50	100	58.6	29201	PASS
443	442	15	24	17.5	5124	PASS