




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112624\
 Data File : BG063559.D
 Acq On : 26 Nov 2024 13:08
 Operator : RC/JU
 Sample : PB165260BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK260

Manual IntegrationsAPPROVED

Quant Time: Nov 27 00:10:36 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 20 14:52:38 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
 Supervised By :mohammad ahmed 11/27/2024

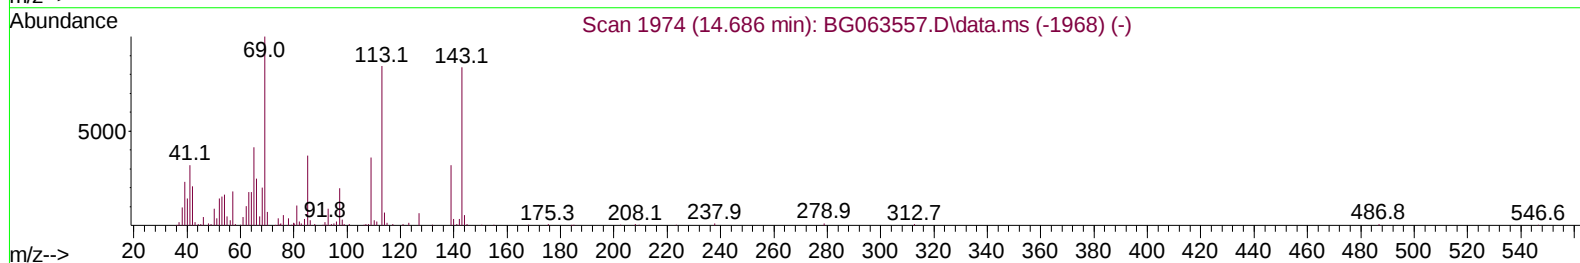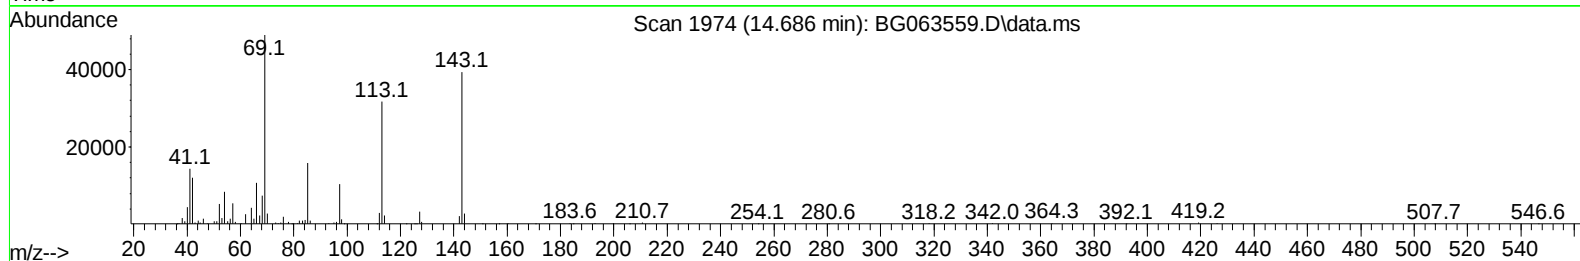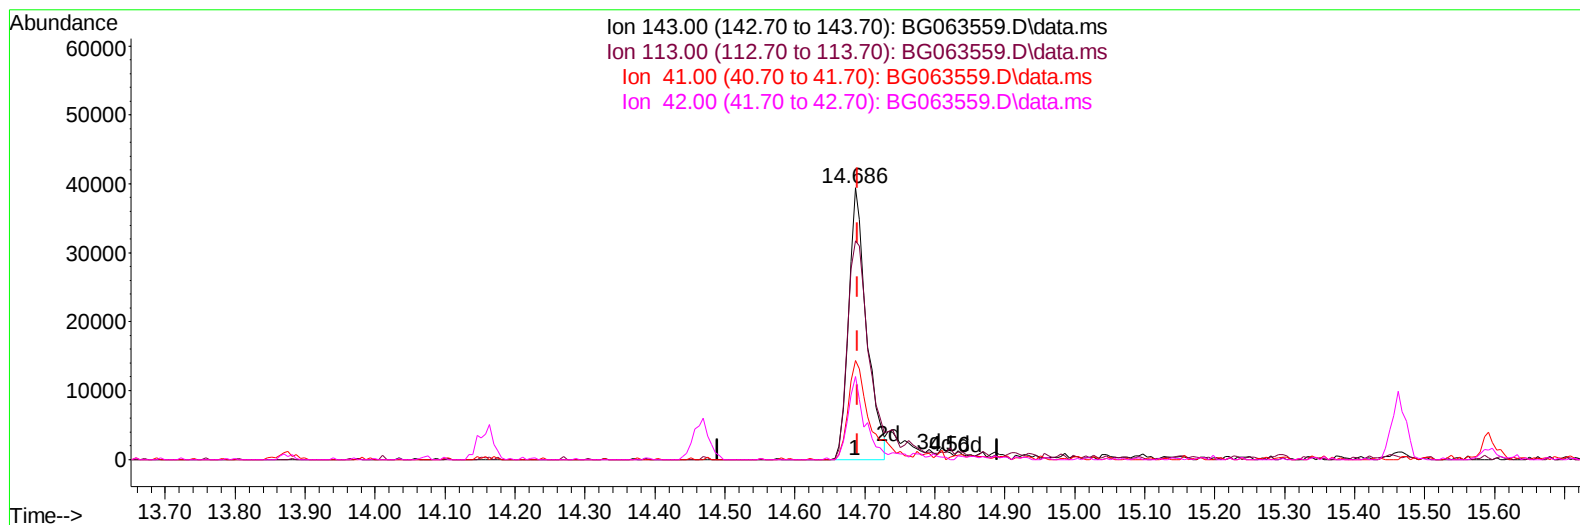

TIC: BG063559.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.686min (-0.003) 21.96 ng/u1

response 69852

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	103.10	80.47#
41.00	38.80	36.48
42.00	26.30	30.64




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112624\
Data File : BG063559.D
Acq On : 26 Nov 2024 13:08
Operator : RC/JU
Sample : PB165260BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK260

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/27/2024

Quant Time: Nov 27 00:10:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 20 14:52:38 2024
Response via : Initial Calibration

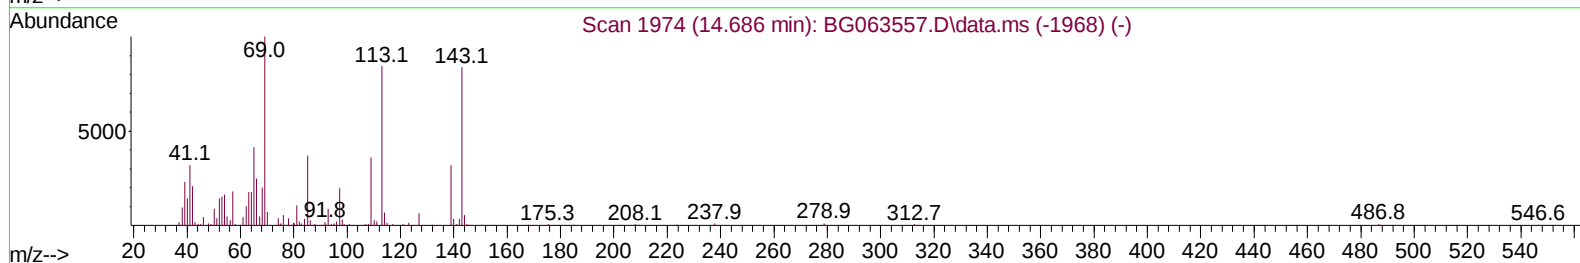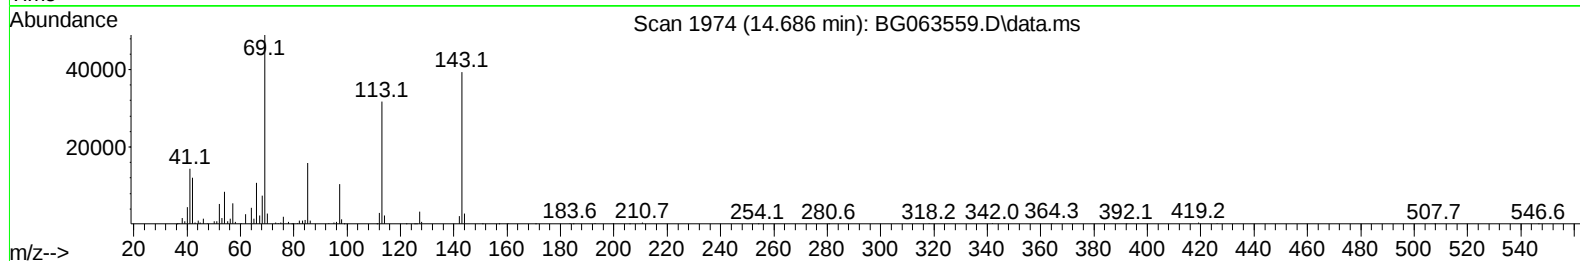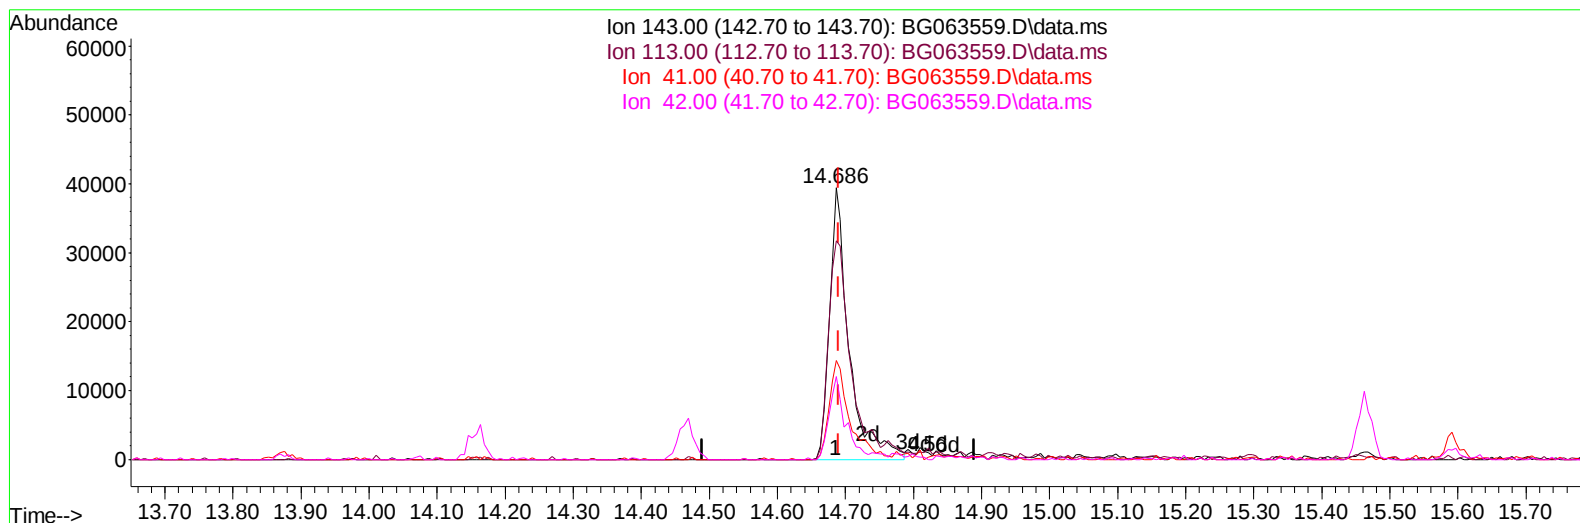

TIC: BG063559.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.686min (-0.003) 24.62 ng/ul m

response 78330

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	103.10	80.47#
41.00	38.80	36.48
42.00	26.30	30.64

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112624\
 Data File : BG063559.D
 Acq On : 26 Nov 2024 13:08
 Operator : RC/JU
 Sample : PB165260BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK260

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/27/2024
 Supervised By :mohammad ahmed 11/27/2024

Quant Time: Nov 27 00:11:27 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 20 14:52:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.824	152	94806	20.000	ng/ul	0.00
20) Naphthalene-d8	10.615	136	398671	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.469	164	315360	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.219	188	783555	20.000	ng/ul	0.00
79) Chrysene-d12	21.478	240	897753	20.000	ng/ul	0.00
88) Perylene-d12	24.516	264	978520	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.294	96	11874	4.943	ng/uL	0.00
4) Pyridine-d5	3.699	84	177691	23.601	ng/ul	0.00
7) Phenol-d5	7.001	99	214826	27.551	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.160	67	139497	27.894	ng/ul	0.00
11) 2-Chlorophenol-d4	7.360	132	152527	27.603	ng/ul	0.00
15) 4-Methylphenol-d8	8.535	113	177317	27.214	ng/ul	0.00
21) Nitrobenzene-d5	8.981	128	78335	27.362	ng/ul	0.00
24) 2-Nitrophenol-d4	9.704	143	96646	27.326	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.244	165	168652	24.983	ng/ul	0.00
31) 4-Chloroaniline-d4	10.756	131	225095	26.362	ng/ul	0.00
46) Dimethylphthalate-d6	13.876	166	624241	29.159	ng/ul	0.00
49) Acenaphthylene-d8	14.158	160	671947	27.524	ng/ul	0.00
54) 4-Nitrophenol-d4	14.686	143	78330m	24.625	ng/ul	0.00
60) Fluorene-d10	15.462	176	562978	28.941	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.591	200	103475	23.489	ng/ul	0.00
73) Anthracene-d10	17.319	188	1050376	30.856	ng/ul	0.00
81) Pyrene-d10	19.622	212	1401460	31.143	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.310	264	1425796	30.041	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112624\
Data File : BG063559.D
Acq On : 26 Nov 2024 13:08
Operator : RC/JU
Sample : PB165260BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK260

Manual IntegrationsAPPROVED

Quant Time: Nov 27 00:11:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 20 14:52:38 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/27/2024

