

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112624\
 Data File : BG063563.D
 Acq On : 26 Nov 2024 15:40
 Operator : RC/JU
 Sample : P4996-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BHF71

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063563.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.632	90	92	93	rBV2	7607	5454	0.14%	0.017%
2	3.708	101	105	115	rVB	54483	101606	2.59%	0.310%
3	4.031	157	160	166	rBV6	6394	10668	0.27%	0.033%
4	4.231	191	194	197	rVB3	4727	5915	0.15%	0.018%
5	4.478	232	236	241	rBV	14045	20972	0.54%	0.064%
6	6.540	584	587	591	rVB3	3820	5818	0.15%	0.018%
7	6.934	651	654	657	rBV4	4844	5500	0.14%	0.017%
8	6.975	657	661	662	rBV3	13952	15388	0.39%	0.047%
9	7.004	662	666	672	rVB2	105554	171397	4.37%	0.524%
10	7.104	677	683	685	rVB3	5316	5902	0.15%	0.018%
11	7.157	685	692	702	rBV	308579	507014	12.94%	1.549%
12	7.363	721	727	737	rBV	336216	574954	14.67%	1.756%
13	7.633	767	773	774	rVB2	5574	7826	0.20%	0.024%
14	7.827	798	806	819	rBV	383329	636017	16.23%	1.943%
15	8.015	837	838	843	rVB5	4897	6244	0.16%	0.019%
16	8.144	855	860	862	rBV3	4989	6764	0.17%	0.021%
17	8.450	909	912	916	rBV4	3358	6267	0.16%	0.019%
18	8.538	921	927	937	rBV2	311614	555681	14.18%	1.697%
19	8.978	995	1002	1013	rBV	374586	674222	17.20%	2.059%
20	9.237	1040	1046	1048	rBV4	12281	20714	0.53%	0.063%
21	9.255	1048	1049	1053	rVB4	9587	9473	0.24%	0.029%
22	9.290	1053	1055	1057	rBV3	5003	5920	0.15%	0.018%
23	9.401	1072	1074	1082	rVB6	11615	18209	0.46%	0.056%
24	9.701	1116	1125	1134	rBV2	345766	624718	15.94%	1.908%
25	10.248	1208	1218	1229	rBV	479692	924489	23.59%	2.824%
26	10.618	1273	1281	1289	rBV	544327	952487	24.30%	2.909%
27	10.753	1297	1304	1314	rBV2	332440	649436	16.57%	1.984%
28	11.899	1496	1499	1502	rBV2	6218	6905	0.18%	0.021%
29	12.210	1547	1552	1555	rBV4	8249	14192	0.36%	0.043%
30	12.586	1615	1616	1621	rVB3	4655	5753	0.15%	0.018%
31	12.639	1621	1625	1628	rBV3	4738	7766	0.20%	0.024%
32	13.391	1750	1753	1755	rBV2	5255	6109	0.16%	0.019%
33	13.873	1827	1835	1846	rBV	1087546	1539204	39.27%	4.702%
34	14.161	1877	1884	1892	rBV	1103280	1723593	43.97%	5.265%
35	14.466	1928	1936	1945	rBV	947085	1446463	36.90%	4.418%
36	14.695	1970	1975	1982	rBV3	57558	122726	3.13%	0.375%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112624\
 Data File : BG063563.D
 Acq On : 26 Nov 2024 15:40
 Operator : RC/JU
 Sample : P4996-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BHF71

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
 Title : SVOA CALIBRATION

37	15.330	2080	2083	2088	rVB2	5410	8168	0.21%	0.025%
38	15.465	2098	2106	2117	rBV	1580810	2382484	60.78%	7.277%
39	15.594	2122	2128	2139	rBV	501379	801207	20.44%	2.447%
40	15.706	2145	2147	2151	rVB4	14775	15214	0.39%	0.046%
41	15.829	2166	2168	2172	rVB4	7988	9175	0.23%	0.028%
42	16.035	2198	2203	2204	rBV5	6730	7468	0.19%	0.023%
43	16.135	2217	2220	2225	rBV5	3698	5567	0.14%	0.017%
44	16.364	2255	2259	2261	rBV2	5422	5866	0.15%	0.018%
45	16.887	2345	2348	2350	rBV2	5683	6353	0.16%	0.019%
46	16.975	2360	2363	2367	rBV4	5378	7218	0.18%	0.022%
47	17.134	2388	2390	2395	rBV4	4528	9371	0.24%	0.029%
48	17.222	2398	2405	2412	rVV	1313166	1985318	50.65%	6.064%
49	17.322	2415	2422	2434	rVB	2036995	3106073	79.24%	9.488%
50	17.615	2469	2472	2475	rBV5	6607	6674	0.17%	0.020%
51	17.892	2516	2519	2523	rBV3	12844	17934	0.46%	0.055%
52	18.179	2565	2568	2570	rBV3	8450	9163	0.23%	0.028%
53	18.414	2605	2608	2611	rVB3	5093	6670	0.17%	0.020%
54	18.479	2617	2619	2624	rBV4	7044	7581	0.19%	0.023%
55	19.184	2734	2739	2746	rVB4	33691	51069	1.30%	0.156%
56	19.255	2746	2751	2755	rVV2	27294	48445	1.24%	0.148%
57	19.308	2758	2760	2765	rVB6	11487	13351	0.34%	0.041%
58	19.619	2807	2813	2824	rBV	2800382	3919670	100.00%	11.973%
59	20.001	2875	2878	2881	rBV4	7220	11285	0.29%	0.034%
60	21.476	3123	3129	3142	rVB2	1518746	2460264	62.77%	7.515%
61	24.308	3600	3611	3625	rBV	1471790	3908923	99.73%	11.940%
62	24.513	3637	3646	3658	rVB	958117	2526078	64.45%	7.716%




Sum of corrected areas: 32738355

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112624\
Data File : BG063563.D
Acq On : 26 Nov 2024 15:40
Operator : RC/JU
Sample : P4996-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BHF71

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

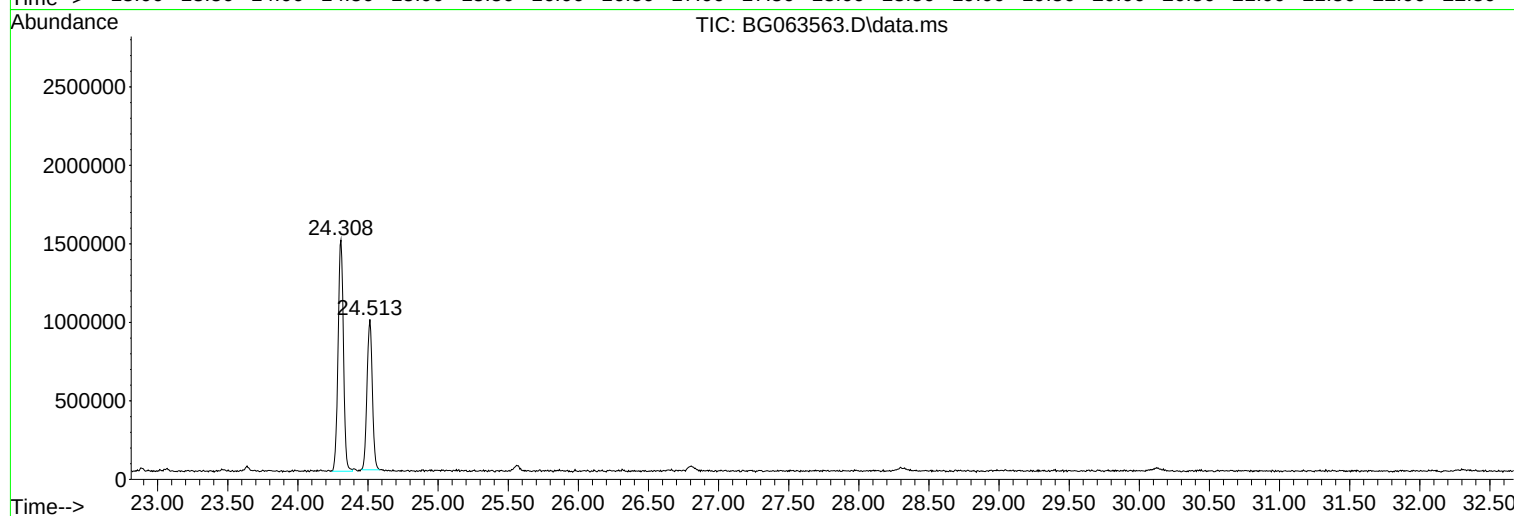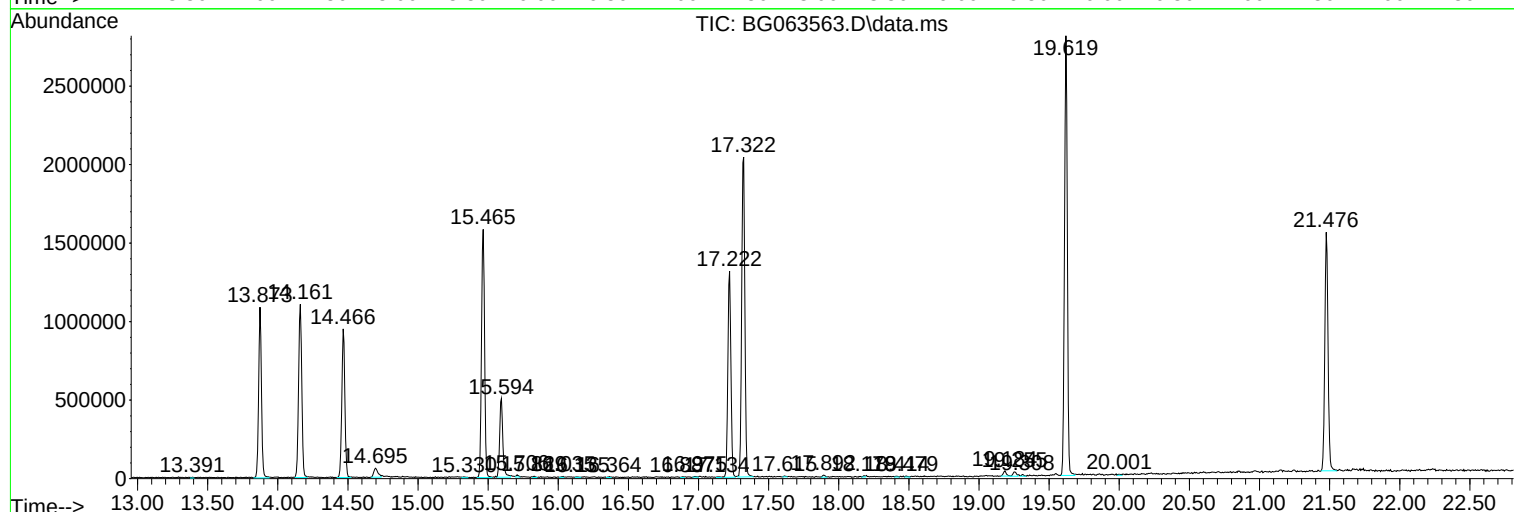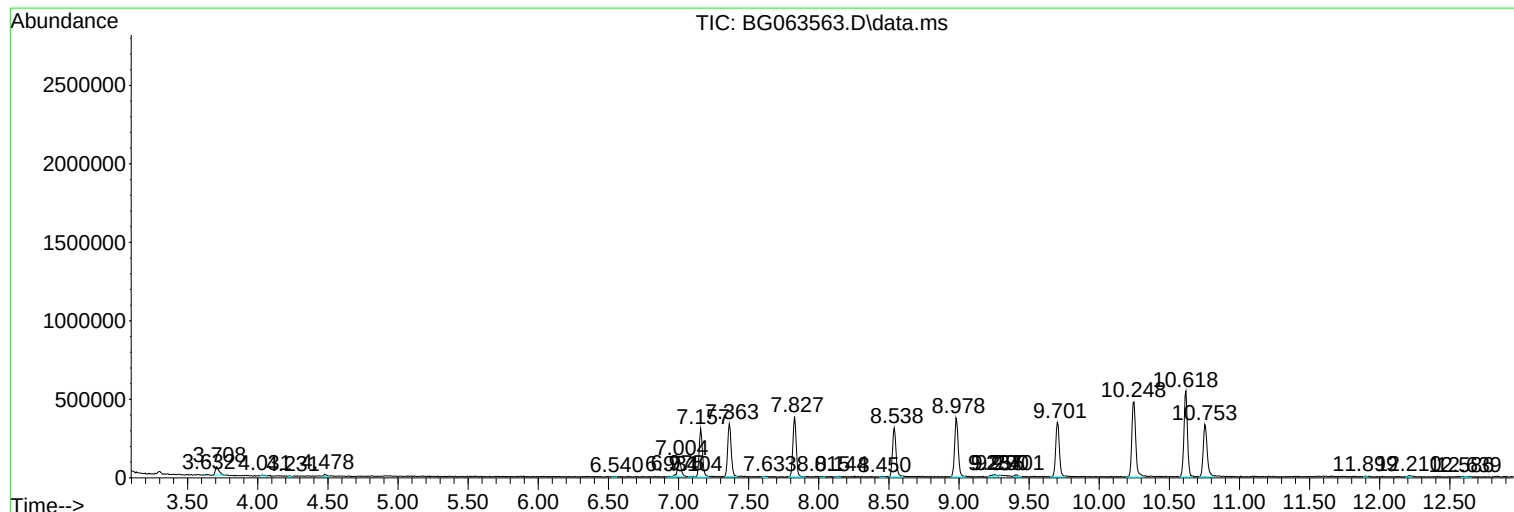

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112624\
Data File : BG063563.D
Acq On : 26 Nov 2024 15:40
Operator : RC/JU
Sample : P4996-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BHF71

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112624\
Data File : BG063563.D
Acq On : 26 Nov 2024 15:40
Operator : RC/JU
Sample : P4996-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BHF71

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc