

Data Path : Z:\HPCHEM1\BNA G\DATA\BG112717\
 Data File : BG031250.D
 Acq On : 28 Nov 2017 4:20
 Operator : SJ/JU
 Sample : I6506-19
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Nov 28 07:26:33 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG111617-PAH.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 28 07:19:57 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.13	152	71356	20.00	ng/ul	0.00
2) Naphthalene-d8	10.95	136	320766	20.00	ng/ul	0.00
6) Acenaphthene-d10	14.75	164	209117	20.00	ng/ul	0.00
12) Phenanthrene-d10	17.49	188	512361	20.00	ng/ul	0.00
18) Chrysene-d12	21.76	240	575840	20.00	ng/ul	0.00
23) Perylene-d12	25.06	264	573260	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 2,4-Dichlorophenol-d3	10.58	165	118488	19.58	ng/uL	0.00
7) Acenaphthylene-d8	14.45	160	511594	23.52	ng/ul	0.00
10) Fluorene-d10	15.74	176	388859	22.26	ng/ul	0.00
15) Anthracene-d10	17.59	188	608021	23.71	ng/ul	0.00
19) Pyrene-d10	19.87	212	724093	27.53	ng/ul	0.00
26) Benzo(a)pyrene-d12	24.84	264	682651	24.07	ng/ul	0.00
Target Compounds						
20) Pyrene	19.89	202	33229	1.09	ng/ul#	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG112717\
Data File : BG031250.D
Acq On : 28 Nov 2017 4:20
Operator : SJ/JU
Sample : I6506-19
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Nov 28 07:26:33 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG111617-PAH.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 28 07:19:57 2017
Response via : Initial Calibration

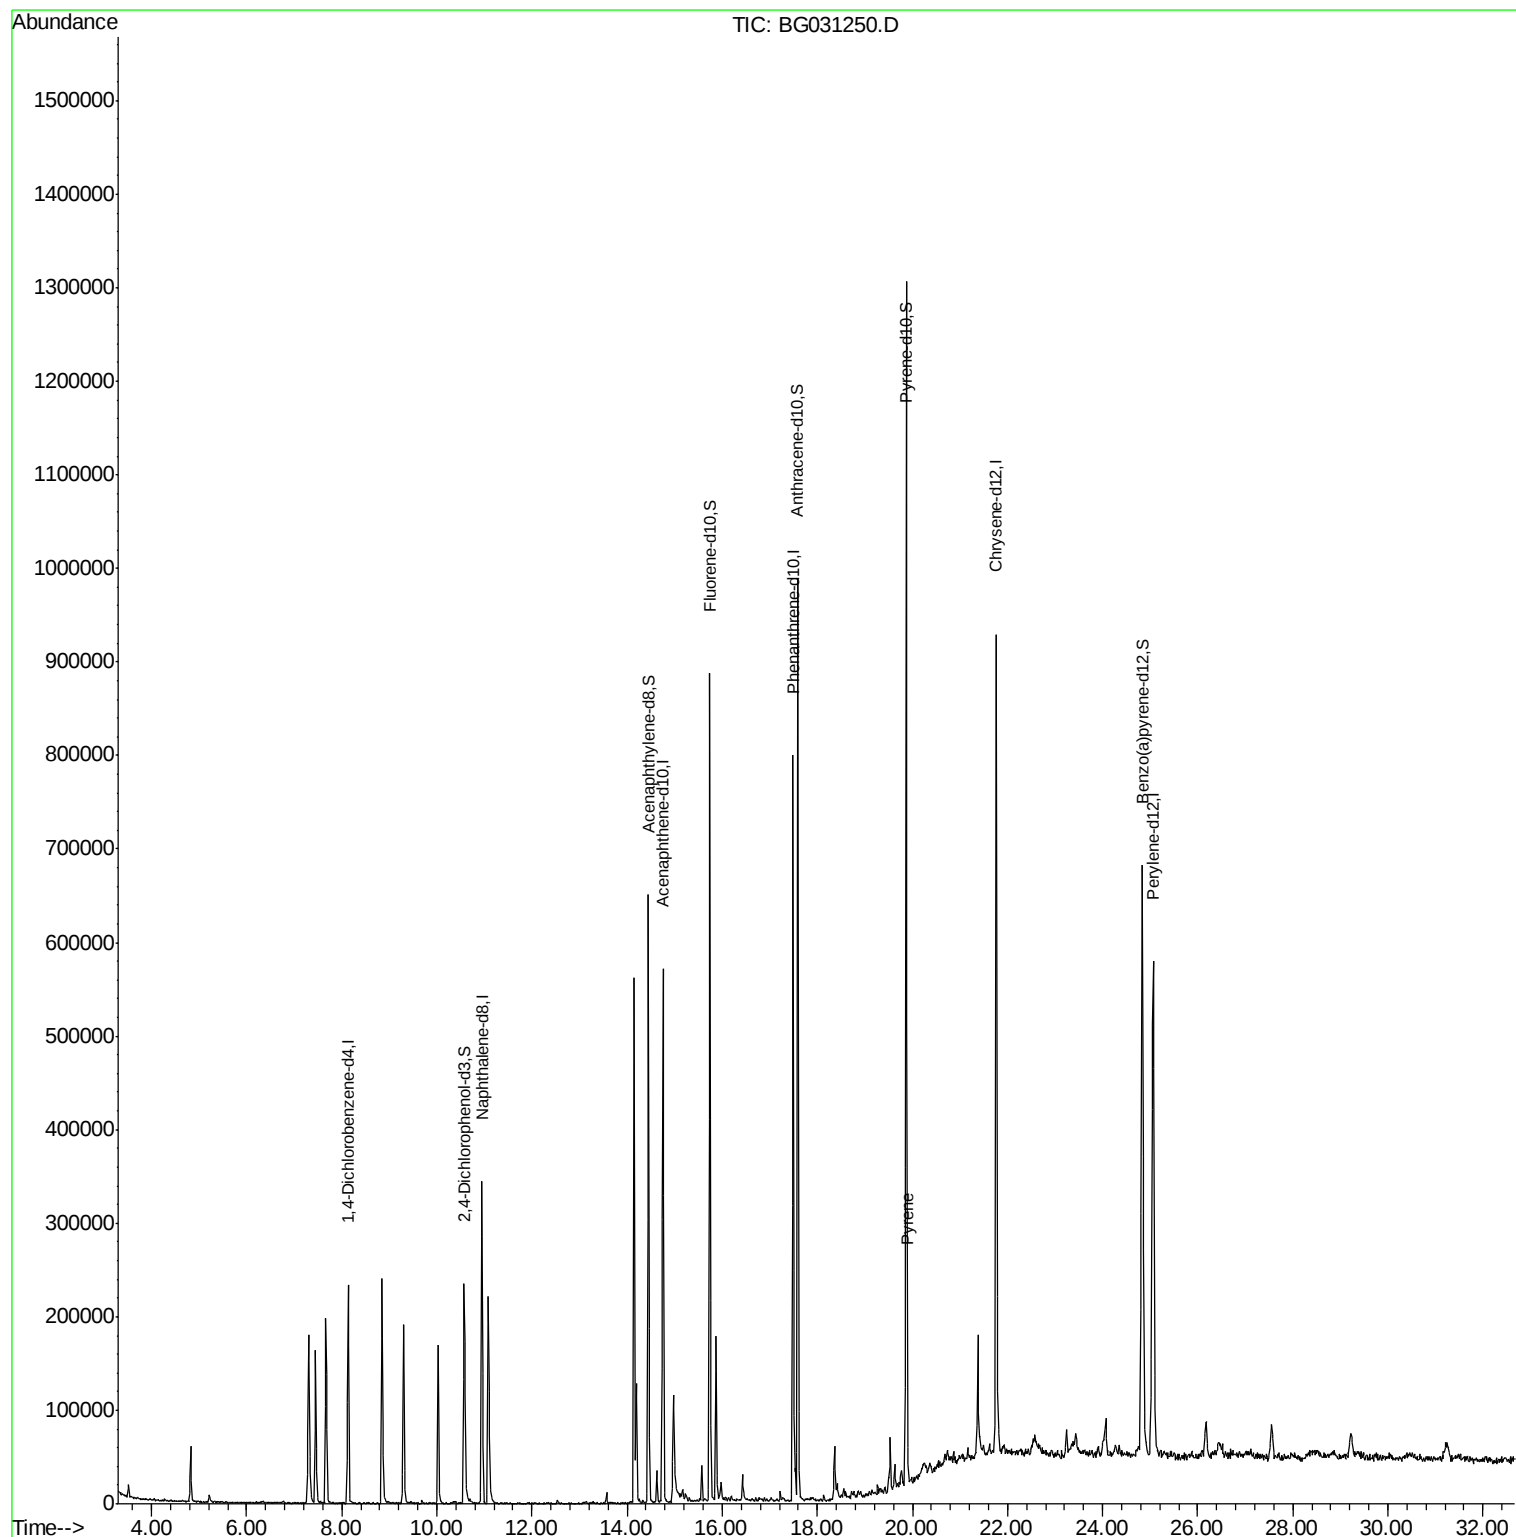


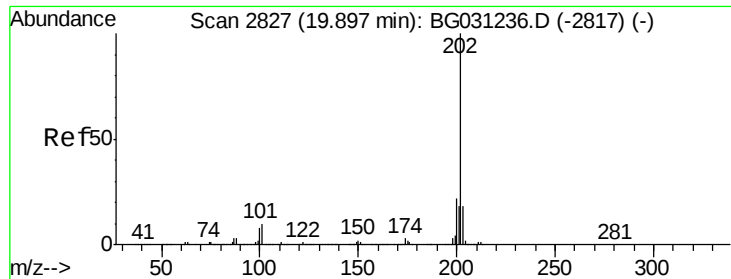

#20
 Pvrene
 Concen: 1.09 ng/ul
 RT: 19.89 min Scan# 2826
 Delta R.T. -0.00 min
 Lab File: BG031250.D
 Acq: 28 Nov 2017 4:20

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
202	100		
101	10.1	11.2	16.8#
100	8.2	9.8	14.6#

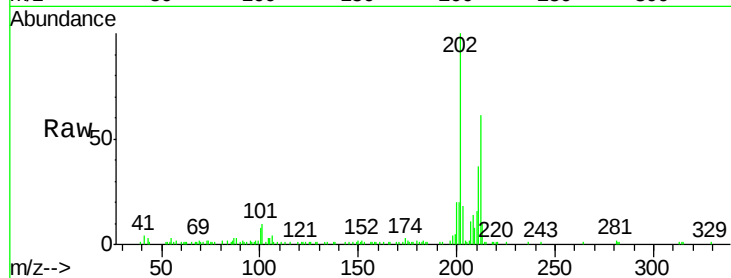

Abundance

Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

